


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110122\
 Data File : BG055391.D
 Acq On : 1 Nov 2022 12:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 02 05:05:12 2022

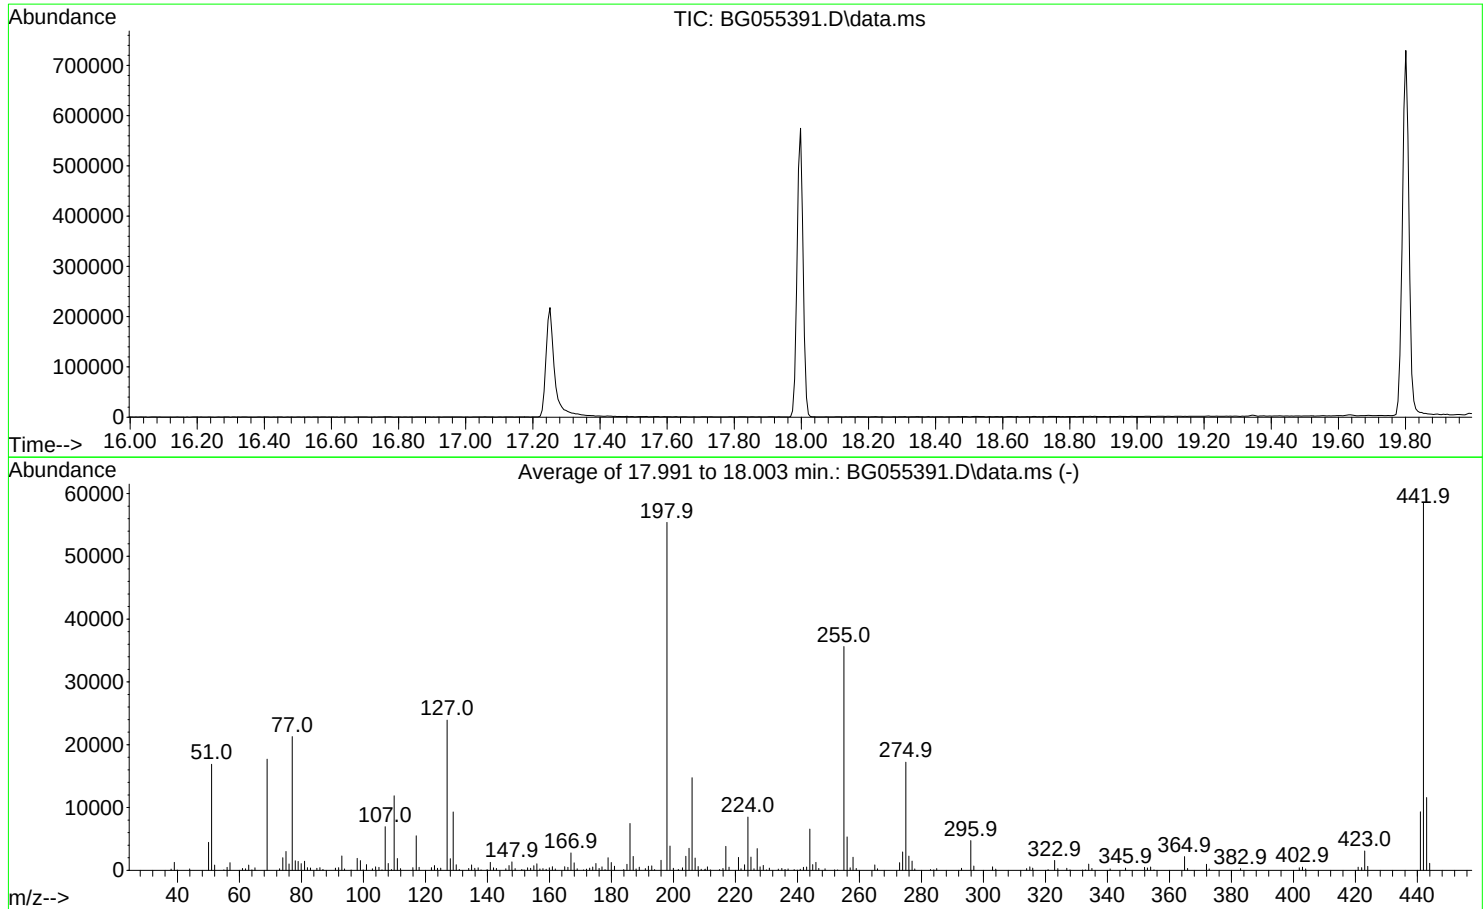




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	16874	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.9	17704	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	23923	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55424	PASS
199	198	5	9	7.0	3861	PASS
275	198	10	60	31.1	17221	PASS
365	198	1	100	4.0	2193	PASS
441	198	0.01	100	16.8	9326	PASS
442	442	50	100	100.0	58587	PASS
443	442	15	24	19.8	11590	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110122\
Data File : BG055391.D
Acq On : 1 Nov 2022 12:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 02 06:53:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

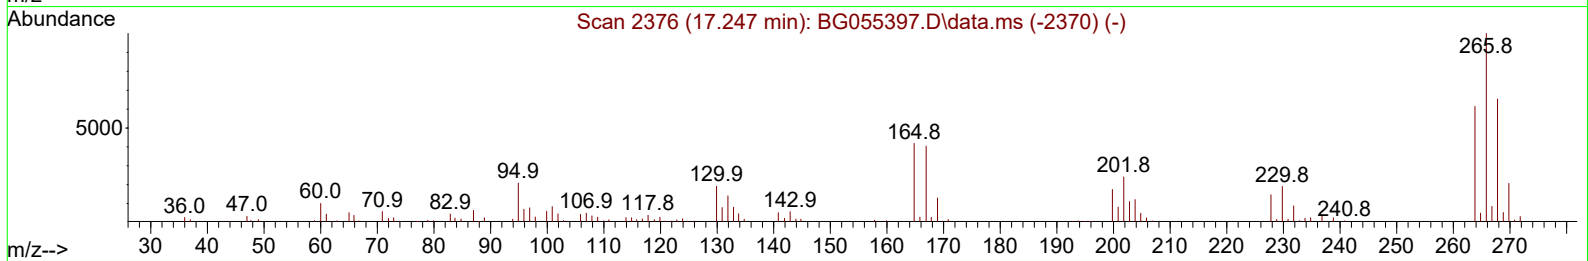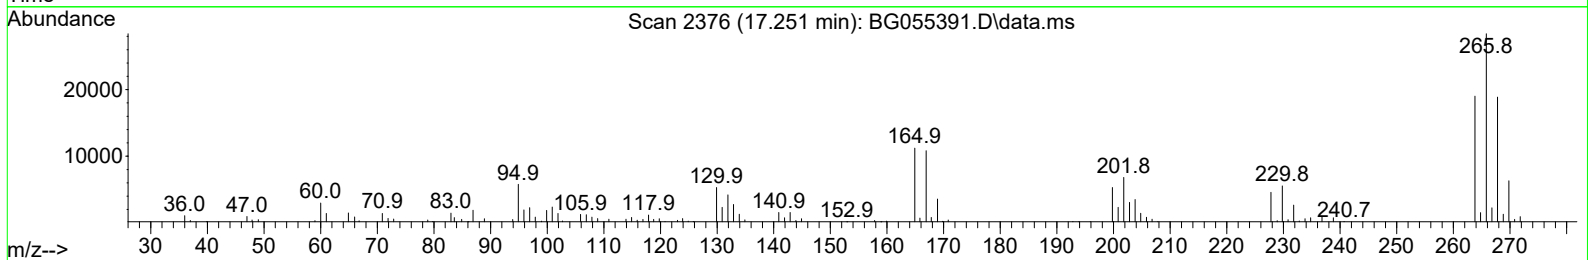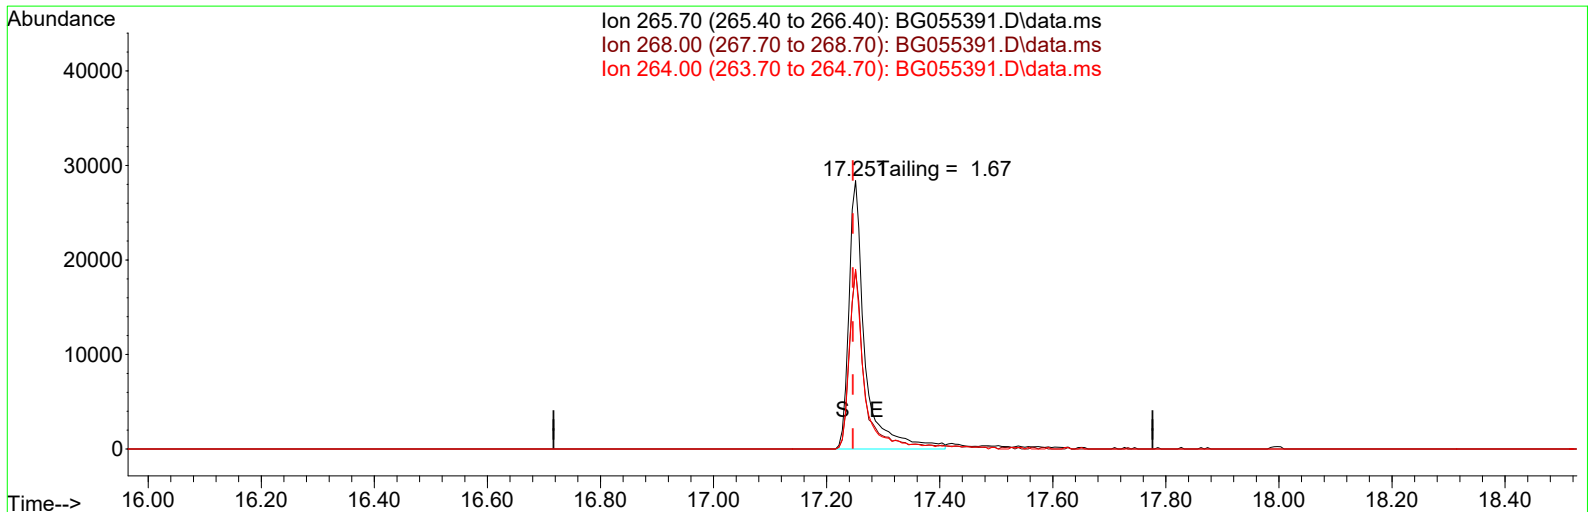

TIC: BG055391.D\data.ms

(70) Pentachlorophenol (C)

17.251min (+ 0.004) 33671.03 ng




response 56111

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	66.50
264.00	61.50	66.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110122\
Data File : BG055391.D
Acq On : 1 Nov 2022 12:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 02 06:53:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

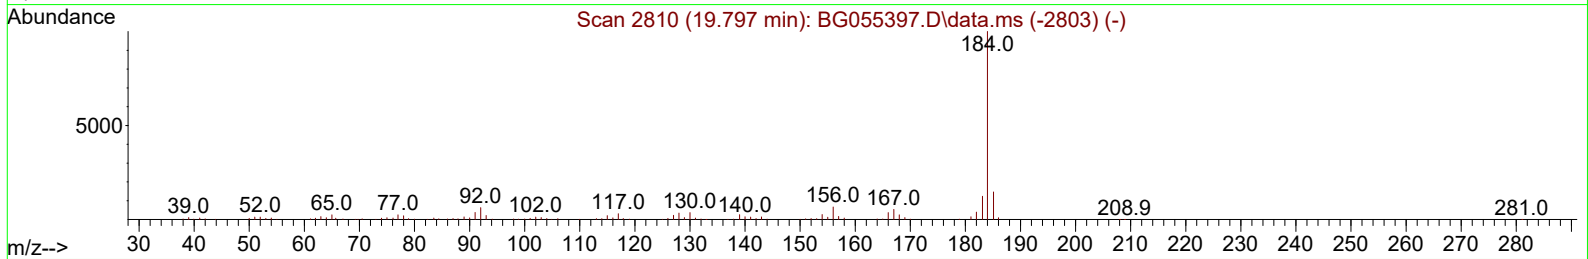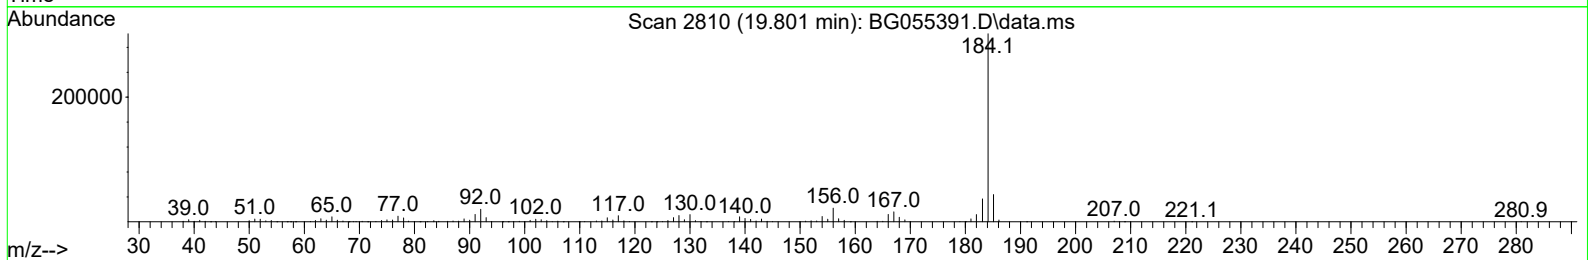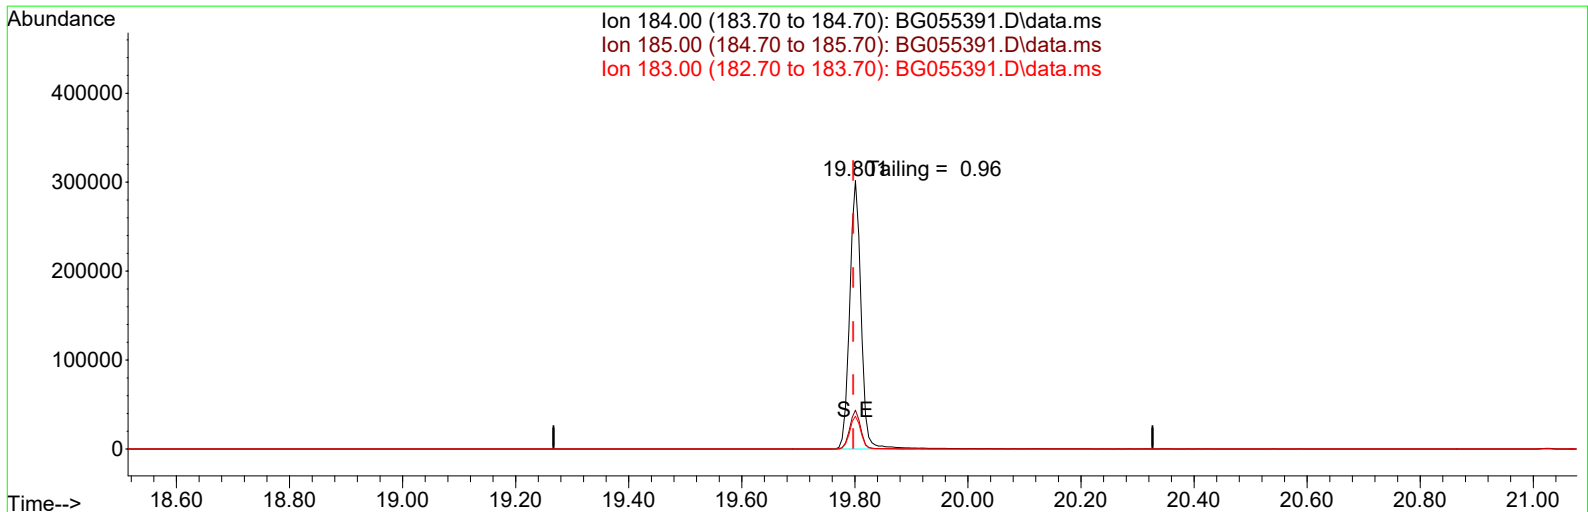

TIC: BG055391.D\data.ms

(77) Benzidine

19.801min (+ 0.004) 60656.94 ng

response 423050

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.51
183.00	12.30	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2022	BNA_G	<u>BG055391.D</u>
Compound Name	Response	Retention Time
DDT	197216	21.023
DDD	2342	20.63
DDE	0	20.089
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2342	199558	1.17

Instrument :
BNA_G
ClientSampleId :
DFTPP