
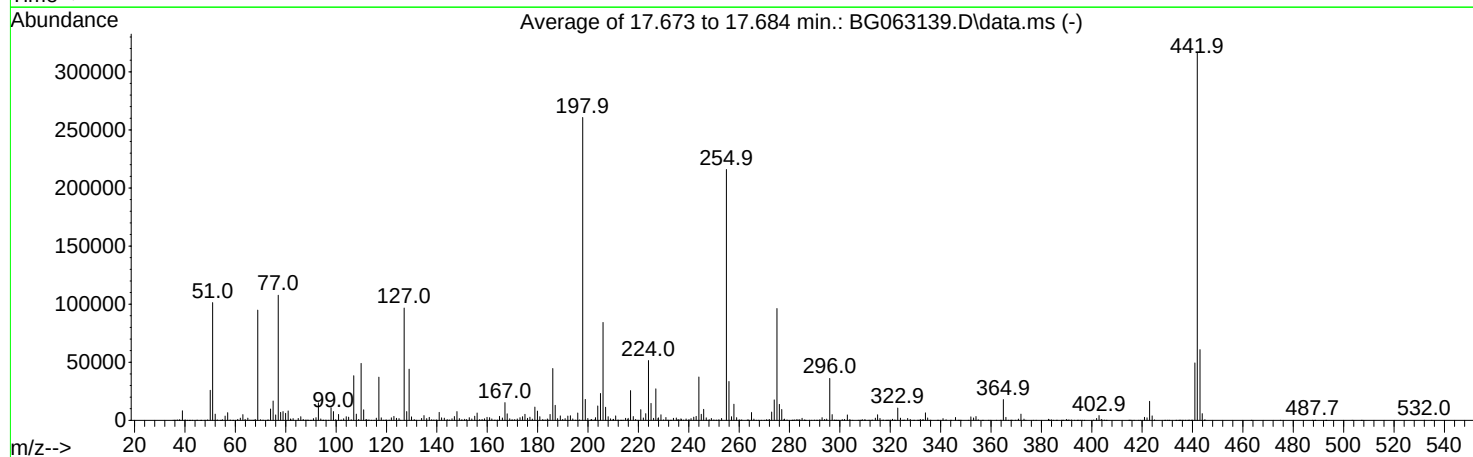


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110124\
Data File : BG063139.D
Acq On : 1 Nov 2024 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG103124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 01 05:13:40 2024

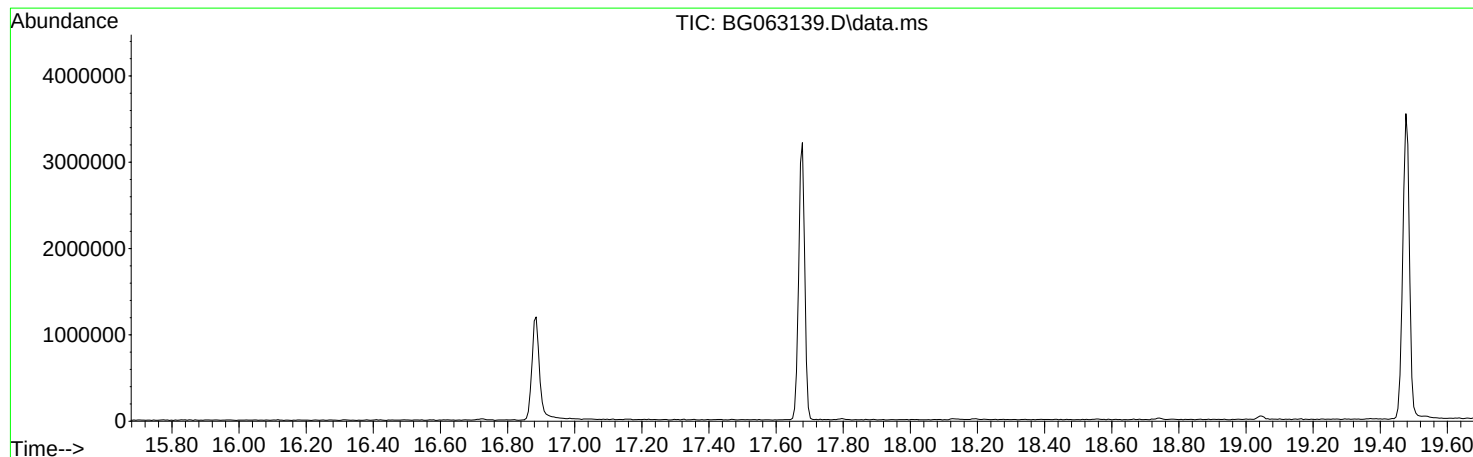

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	101435	PASS
68	69	0.00	2	0.9	834	PASS
69	198	0.00	100	36.4	94944	PASS
70	69	0.00	2	0.6	605	PASS
127	198	10	80	37.1	96667	PASS
197	198	0.00	2	0.2	465	PASS
198	198	100	100	100.0	260757	PASS
199	198	5	9	6.9	18022	PASS
275	198	10	60	36.9	96219	PASS
365	198	1	100	6.9	17897	PASS
441	198	0.01	100	19.0	49461	PASS
442	442	50	100	100.0	316608	PASS
443	442	15	24	19.2	60816	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/1/2024	BNA_G	<u>BG063139.D</u>
Compound Name	Response	Retention Time
DDT	1099676	20.716
DDD	25290	20.27
DDE	2331	19.77
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27621	1127297	2.45

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110124\
Data File : BG063139.D
Acq On : 1 Nov 2024 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 01 16:50:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 01 05:13:40 2024
Response via : Initial Calibration

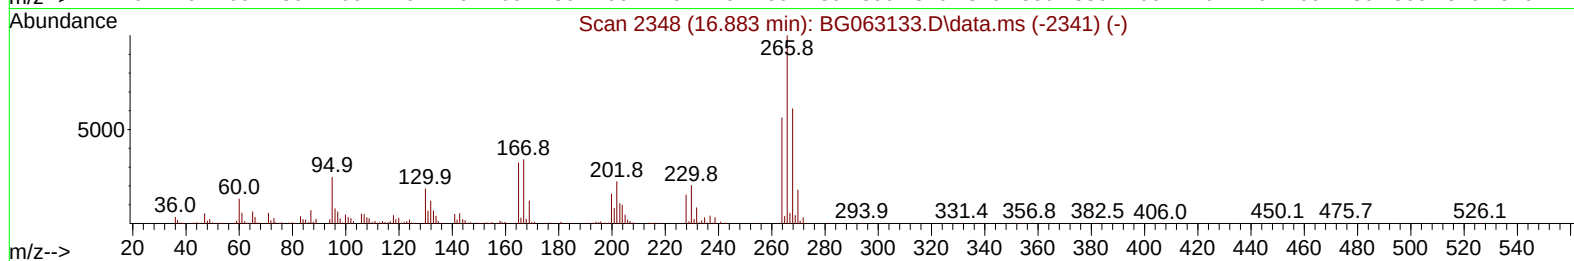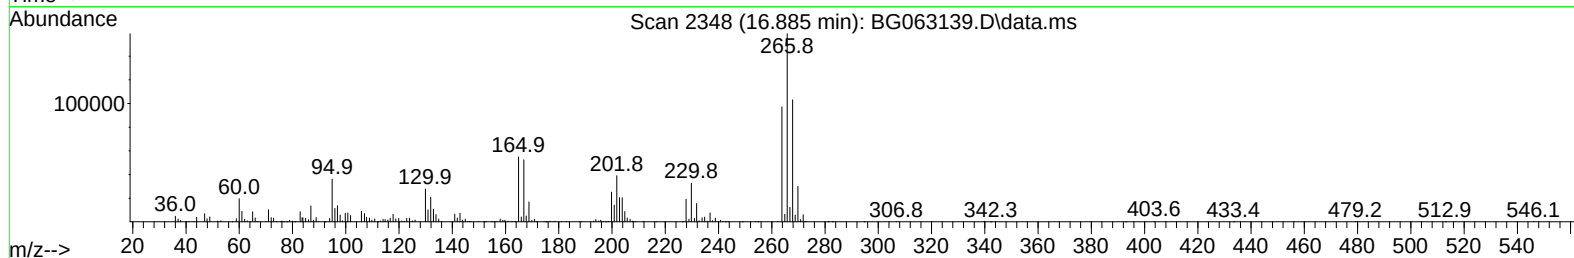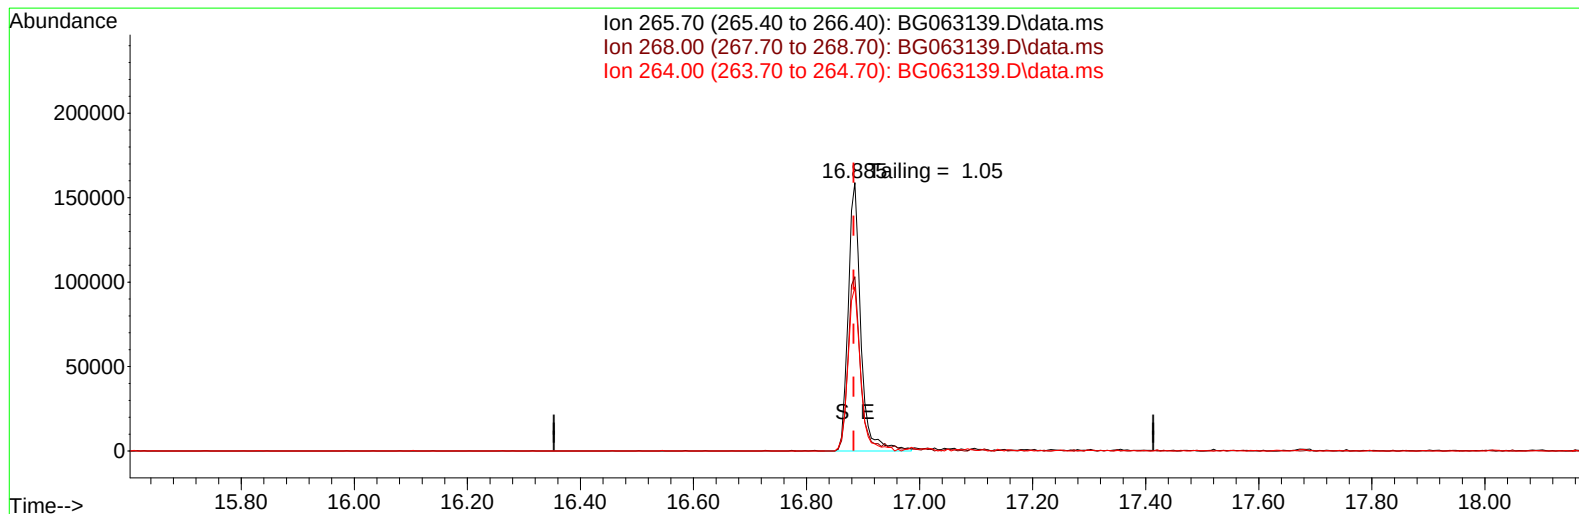

TIC: BG063139.D\data.ms

(70) Pentachlorophenol (C)

16.885min (+ 0.002) 513825.18 ng




response 246805

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.93
264.00	56.20	61.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110124\
Data File : BG063139.D
Acq On : 1 Nov 2024 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 01 16:50:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 01 05:13:40 2024
Response via : Initial Calibration

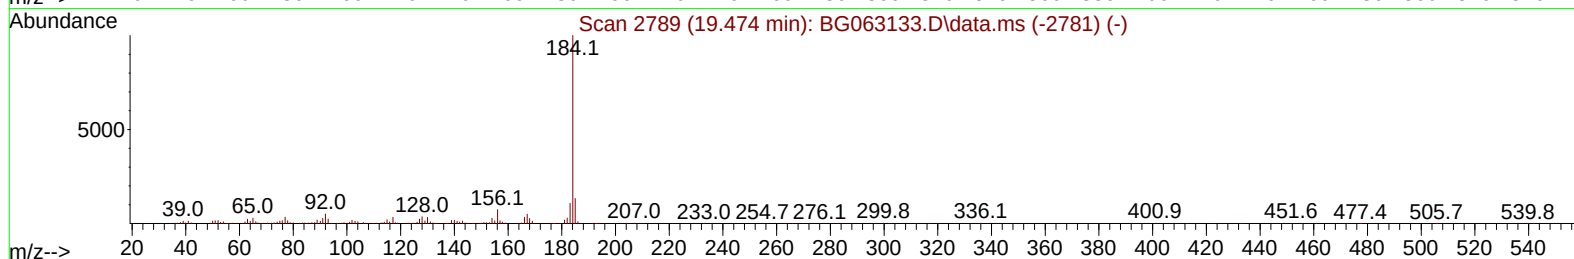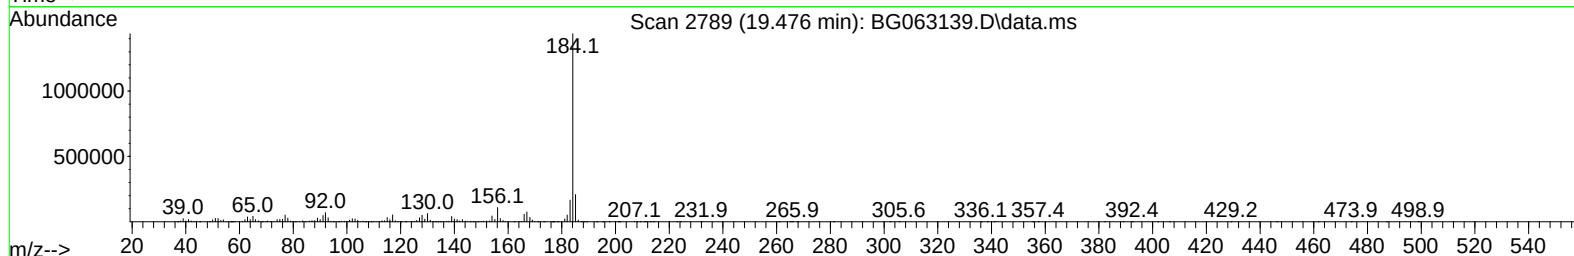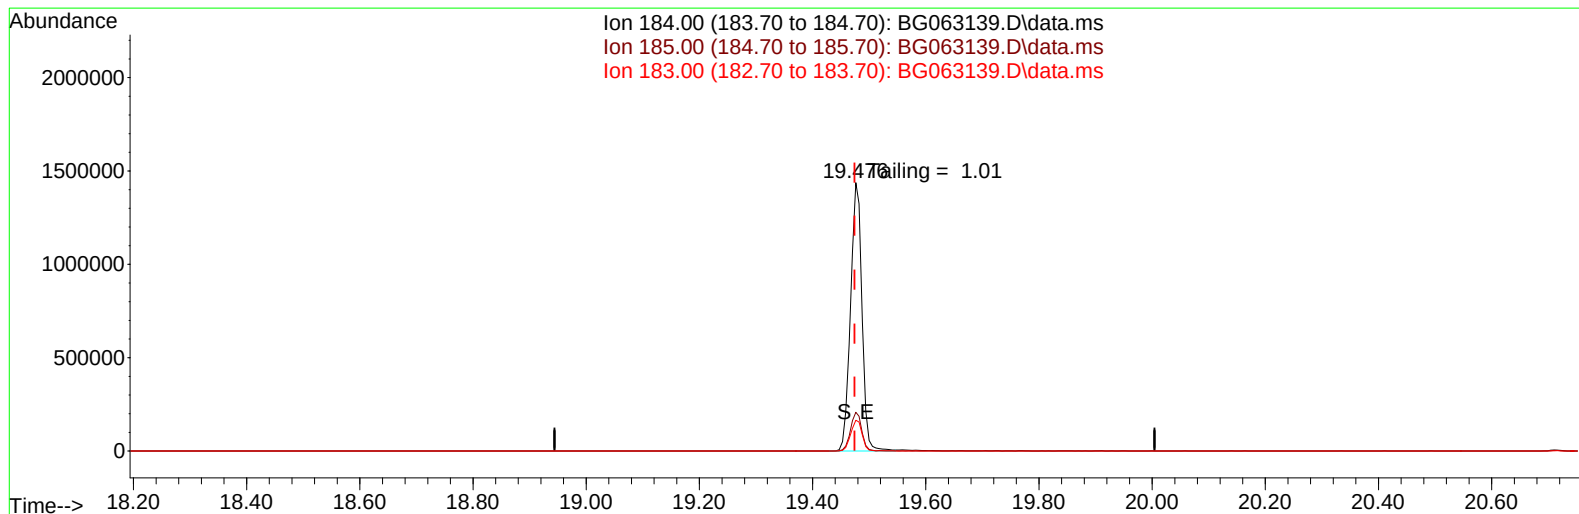

TIC: BG063139.D\data.ms

(77) Benzidine

19.476min (+ 0.002) 606286.85 ng

response 2017736

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.44
183.00	10.70	11.49
0.00	0.00	0.00