

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110215\
 Data File : BG019441.D
 Acq On : 2 Nov 2015 20:27
 Operator : UM/NP
 Sample : G4202-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCY54

Manual Integrations
 APPROVED

Mmdadoda
 11/3/2015 5:57:31 PM

Quant Time: Nov 03 00:46:12 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 03 00:19:25 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.19	152	26966	20.00	ng/ul	0.00
18) Naphthalene-d8	11.02	136	109018	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.82	164	87479	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.56	188	259023	20.00	ng/ul	0.00
78) Chrysene-d12	21.84	240	355984	20.00	ng/ul	0.00
86) Perylene-d12	25.21	264	334476	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	810m	1.44	ng/uL	0.00
5) Phenol-d5	7.34	99	16140	6.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.50	67	53590	34.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.72	132	41344	26.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.89	113	29945	15.19	ng/ul	0.00
19) Nitrobenzene-d5	9.36	128	26109	32.59	ng/ul	0.00
22) 2-Nitrophenol-d4	10.09	143	31996	33.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.63	165	57515	27.87	ng/ul	0.00
29) 4-Chloroaniline-d4	11.14	131	1007	0.48	ng/ul	0.00
44) Dimethylphthalate-d6	14.22	166	266271	36.92	ng/ul	0.00
47) Acenaphthylene-d8	14.52	160	252726	31.64	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	9480	8.27	ng/ul	-0.01
58) Fluorene-d10	15.81	176	225354	33.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.91	200	37779	22.53	ng/ul	0.00
71) Anthracene-d10	17.66	188	433942m	36.75	ng/ul	0.00
79) Pyrene-d10	19.93	212	546043	35.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.97	264	599853	35.74	ng/ul	0.00

Target Compounds					Ovalue
50) Acenaphthene	14.89	153	13923	2.52 ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG110215\
Data File : BG019441.D
Acq On : 2 Nov 2015 20:27
Operator : UM/NP
Sample : G4202-04
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BCY54

Manual Integrations
APPROVED

Mmdadoda
11/3/2015 5:57:31 PM

Quant Time: Nov 03 00:46:12 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 03 00:19:25 2015
Response via : Initial Calibration

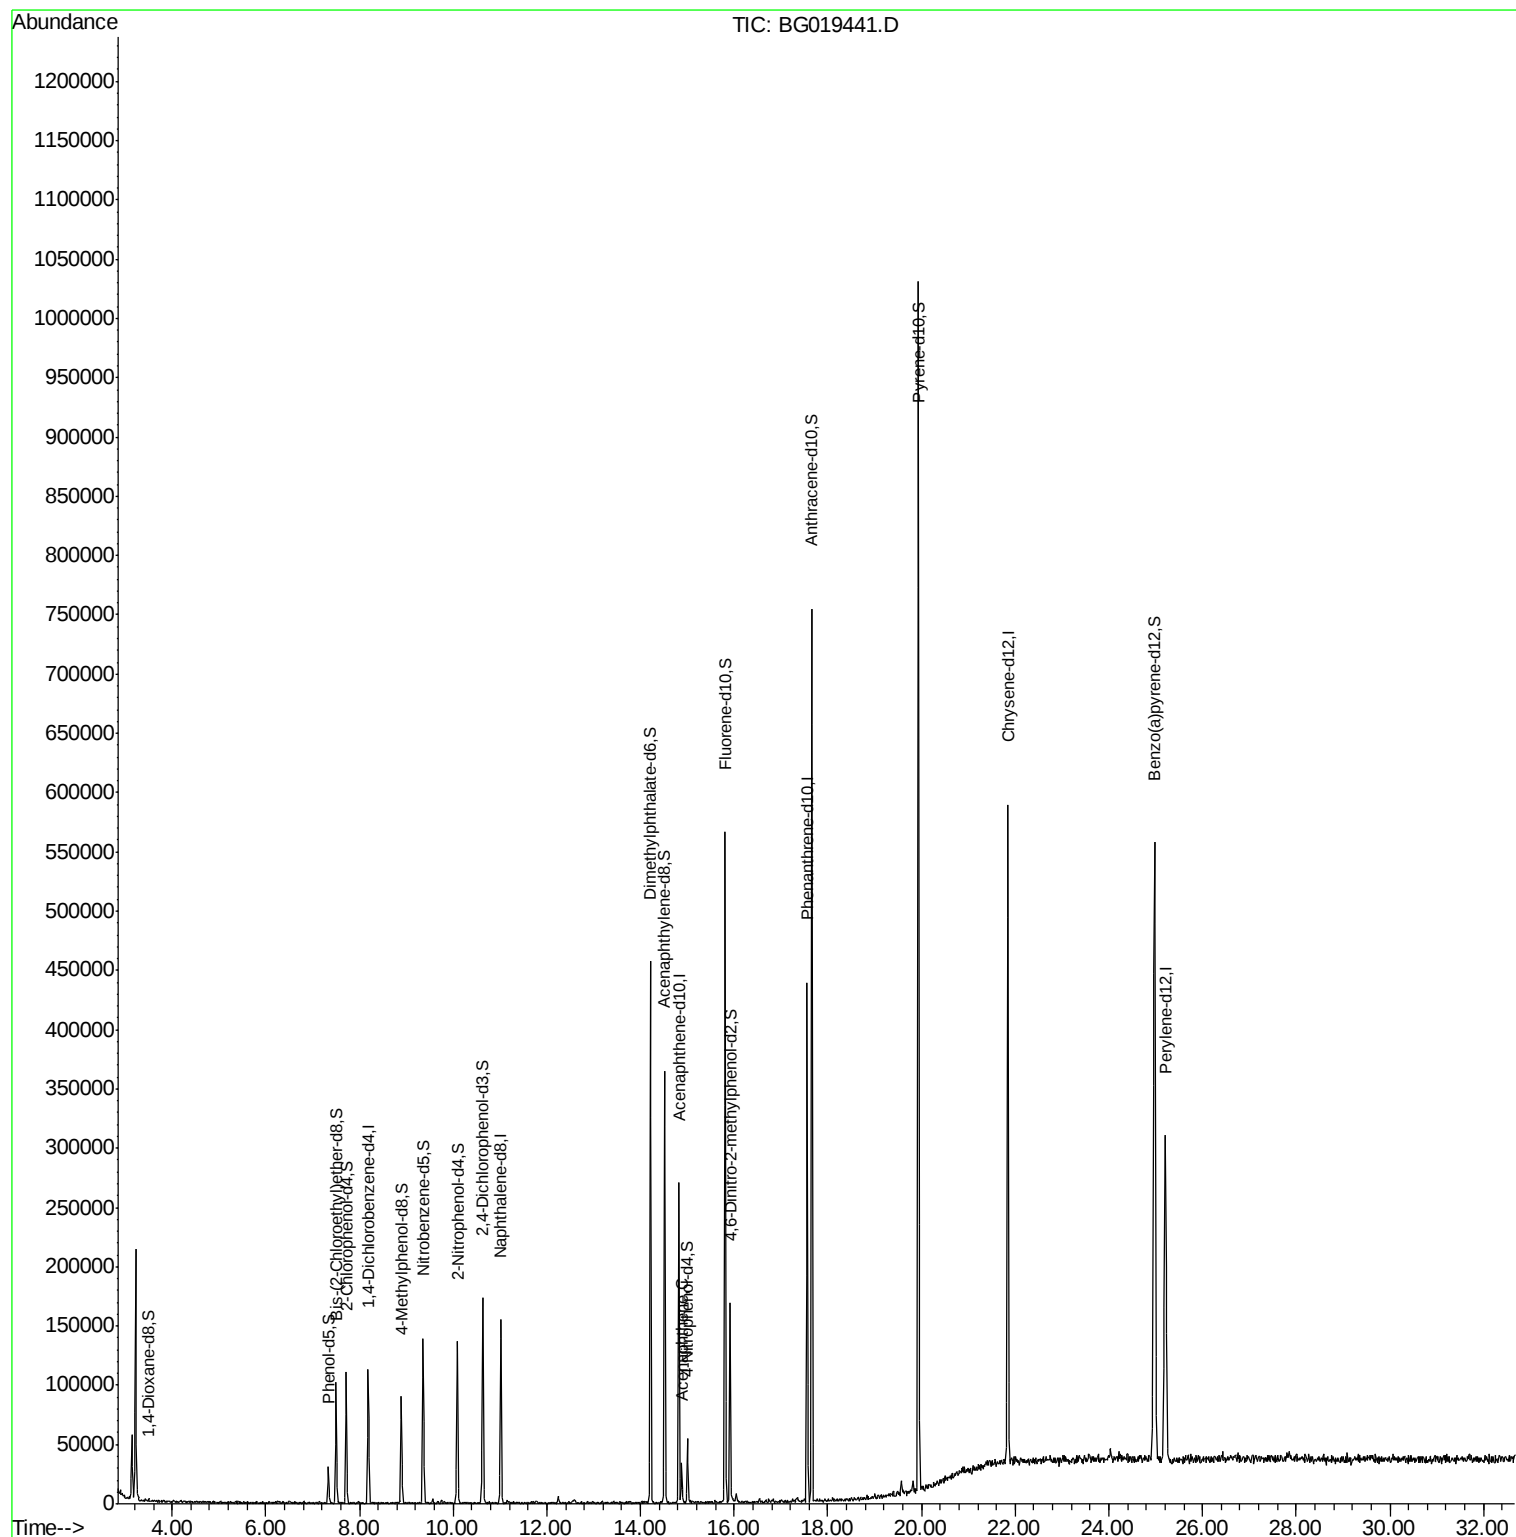

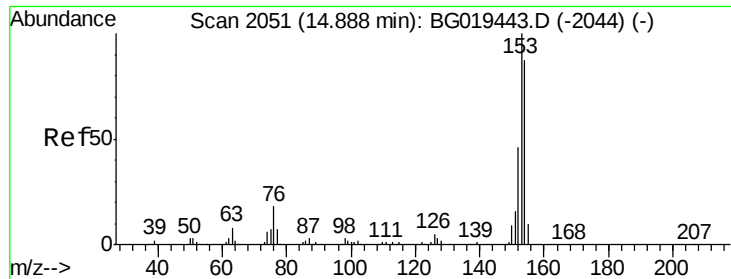

#50

Acenaphthene

Concen: 2.52 ng/ul

RT: 14.89 min Scan# 2050

Delta R.T. 0.00 min

Lab File: BG019441.D

Acq: 2 Nov 2015 20:27

Instrument :

BNA_G

ClientSampleId :

BCY54

Tot Ion:153 Resp: 13923

Ion Ratio Lower Upper


153 100

152 38.4 38.8 58.2#

154 76.2 71.5 107.3

Manual Integrations
APPROVED

Mmdadoda
11/3/2015 5:57:31 PM

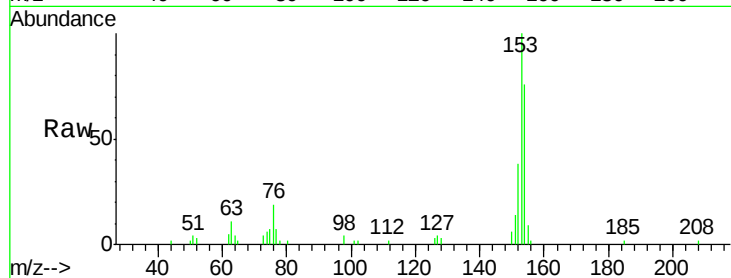

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

