
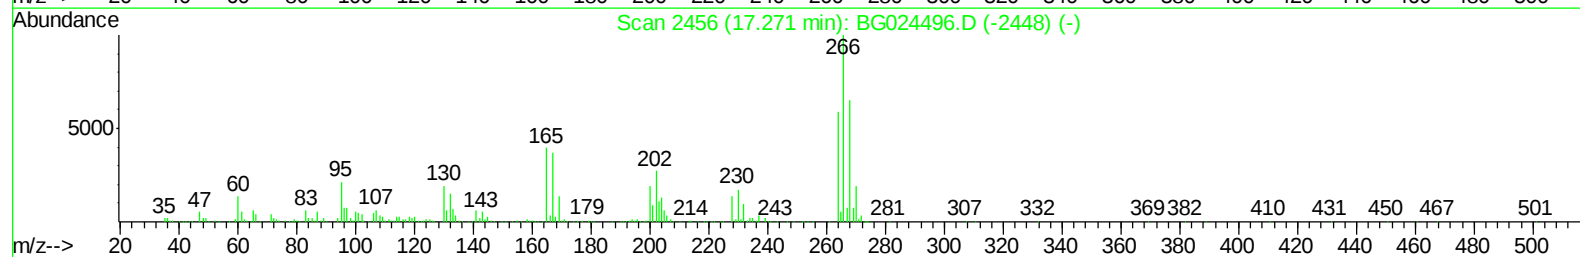
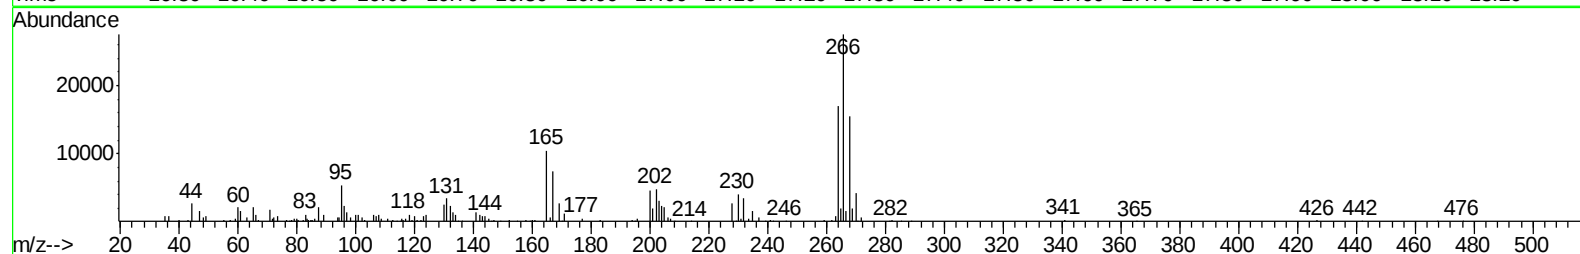


Data Path : Z:\HPCHEM1\BNA_G\Data\BG110216\
Data File : BG024627.D
Acq On : 2 Nov 2016 16:04
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:56:12 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

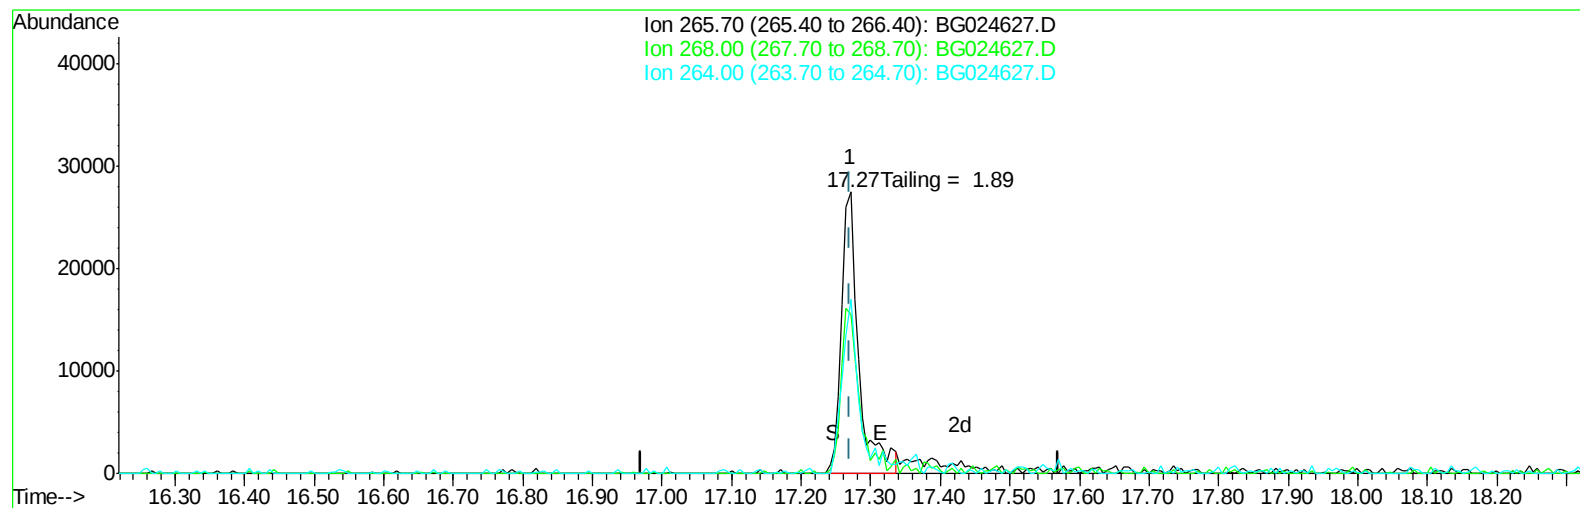

TIC: BG024627.D

(69) Pentachlorophenol (C)




17.271min (-0.000) 489.60ng

response 45616

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	56.39
264.00	62.60	61.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110216\
Data File : BG024627.D
Acq On : 2 Nov 2016 16:04
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 06:56:12 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

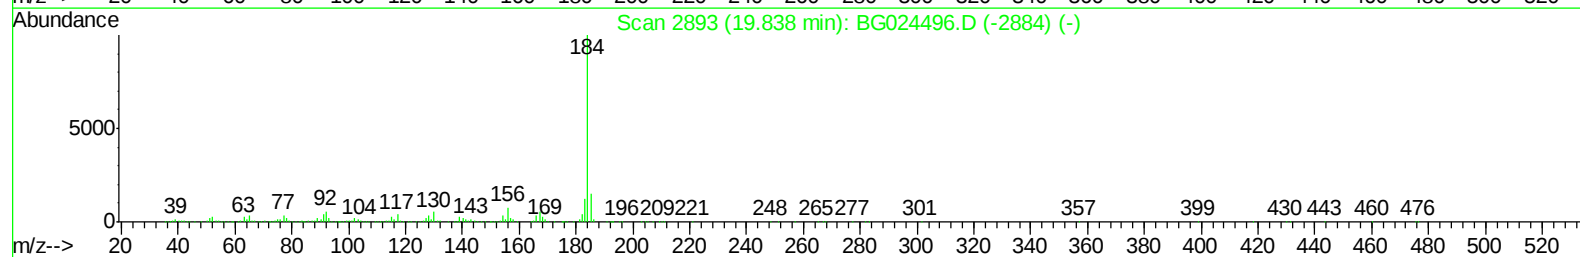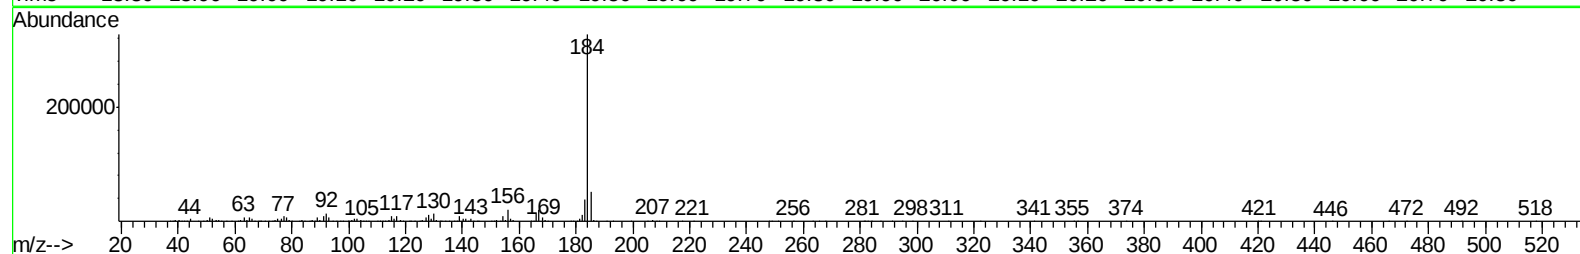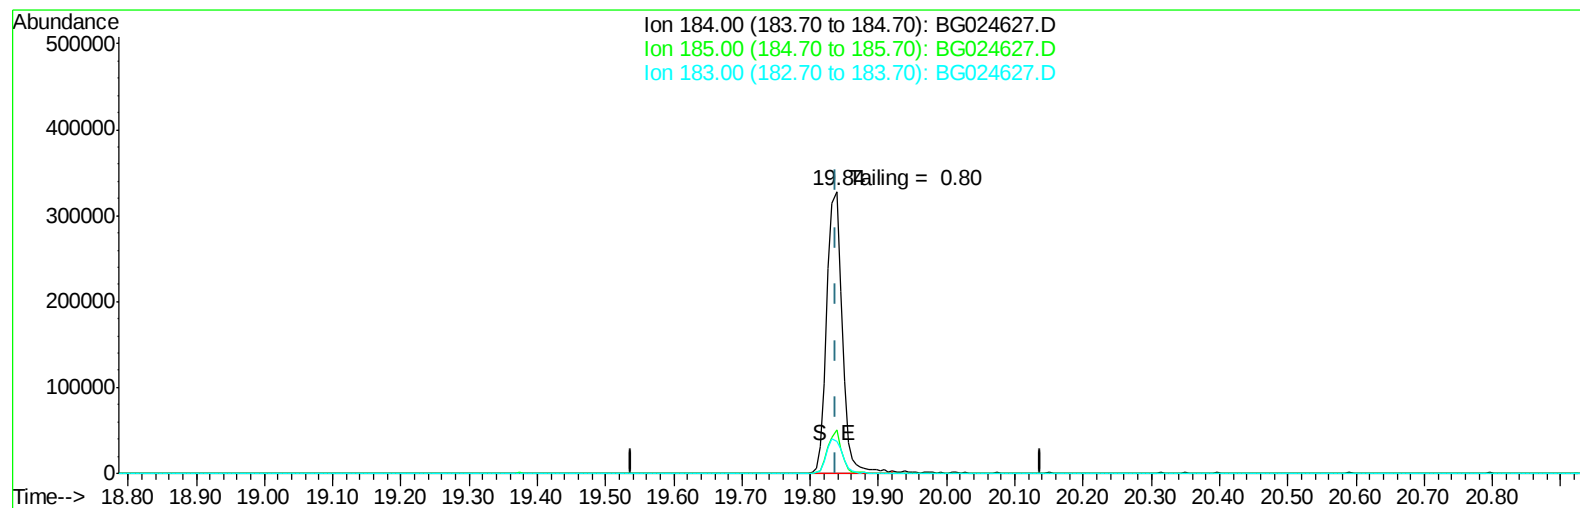

TIC: BG024627.D

(76) Benzidine

19.838min (-0.000) 1892.98ng

response 510545

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.49
183.00	13.80	11.37
0.00	0.00	0.00