

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110216\
 Data File : BG024633.D
 Acq On : 2 Nov 2016 19:58
 Operator : UM/SJ
 Sample : PB94494BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB94494BL

Quant Time: Nov 03 02:32:08 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	111312	20.00	ng	0.00
21) Naphthalene-d8	11.09	136	422254	20.00	ng	0.00
38) Acenaphthene-d10	14.88	164	314170	20.00	ng	0.00
63) Phenanthrene-d10	17.62	188	704641	20.00	ng	0.00
75) Chrysene-d12	21.92	240	1046180	20.00	ng	-0.01
86) Perylene-d12	25.35	264	1080296	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.80	112	812407	119.62	ng	0.00
7) Phenol-d6	7.40	99	1137917	122.15	ng	0.00
23) Nitrobenzene-d5	9.44	82	793775	85.59	ng	0.00
41) 2,4,6-Tribromophenol	16.37	330	564276	120.22	ng	0.00
44) 2-Fluorobiphenyl	13.51	172	1596041	84.44	ng	0.00
78) Terphenyl-d14	20.21	244	2905863	83.00	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110216\
Data File : BG024633.D
Acq On : 2 Nov 2016 19:58
Operator : UM/SJ
Sample : PB94494BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB94494BL

Quant Time: Nov 03 02:32:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

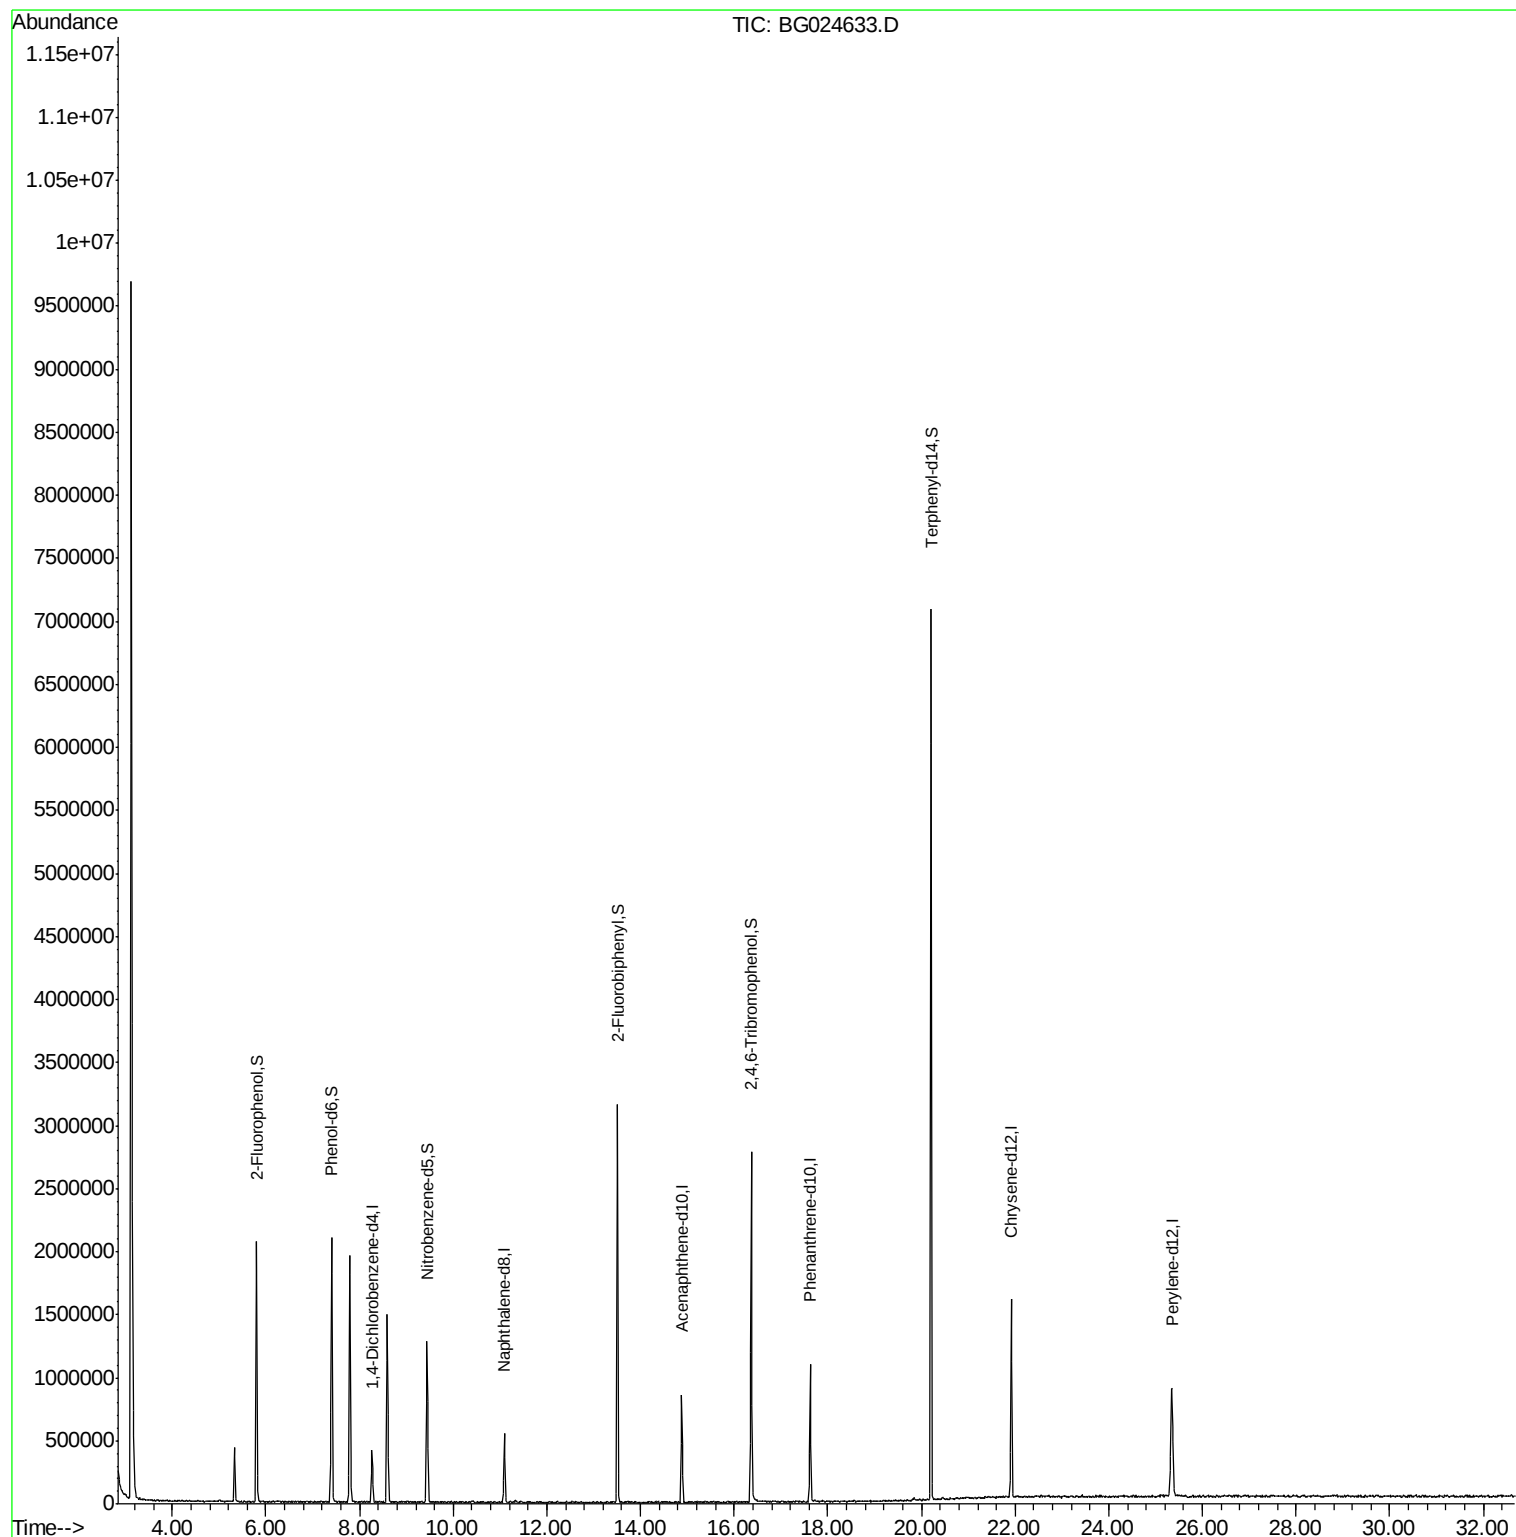

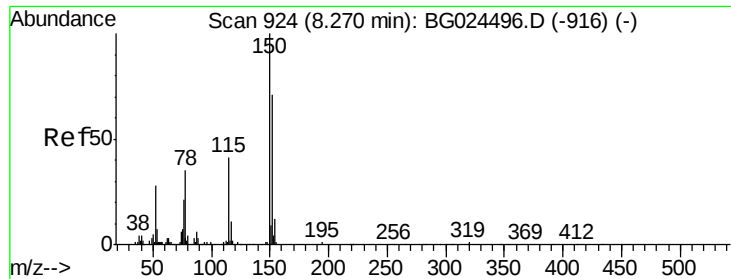

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.27 min Scan# 924

Delta R.T. -0.00 min

Lab File: BG024633.D

Acq: 2 Nov 2016 19:58

Instrument :

BNA_G

ClientSampleId :

PB94494BL


Tgt Ion:152 Resp: 111312

Ion Ratio Lower Upper

152 100

150 150.5 114.0 171.0



115 61.8 48.1 72.1

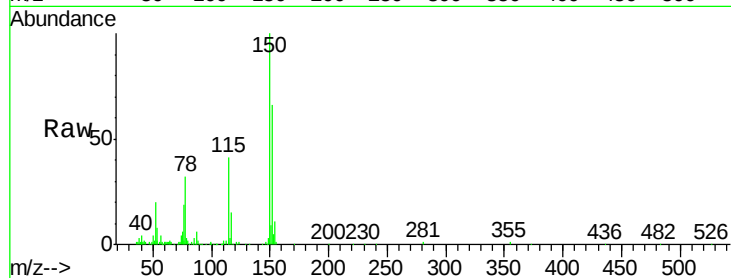


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

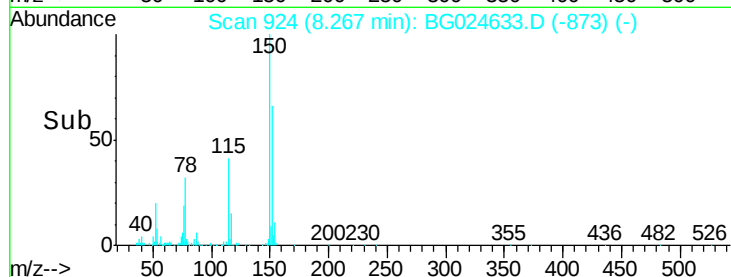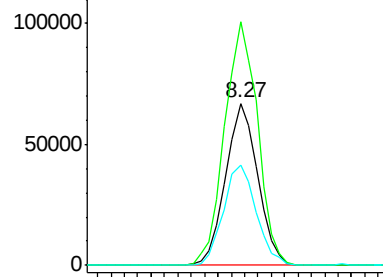

Time-->

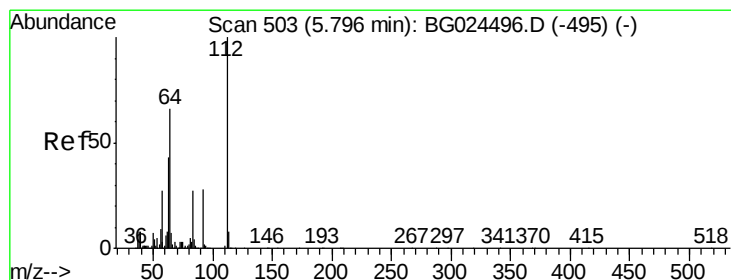

#5

2-Fluorophenol

Concen: 119.62 ng

RT: 5.80 min Scan# 504

Delta R.T. 0.00 min

Lab File: BG024633.D

Acq: 2 Nov 2016 19:58


Tgt Ion:112 Resp: 812407

Ion Ratio Lower Upper

112 100

64 72.7 61.8 92.6



63 41.9 37.2 55.8

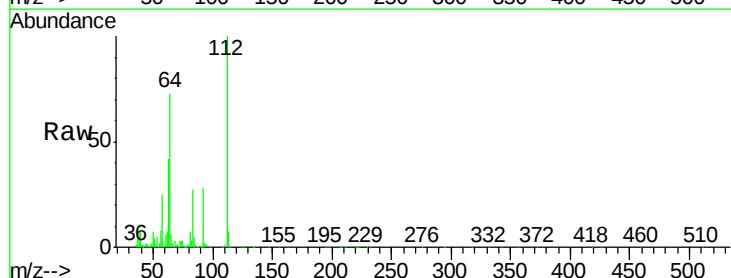


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

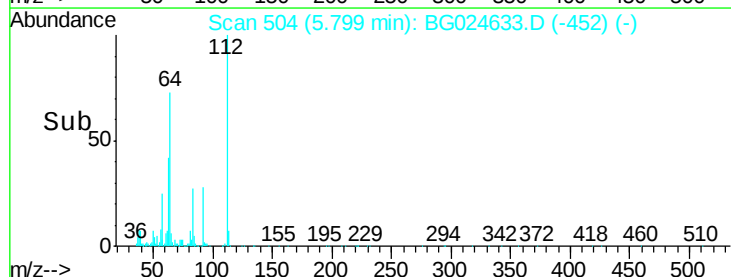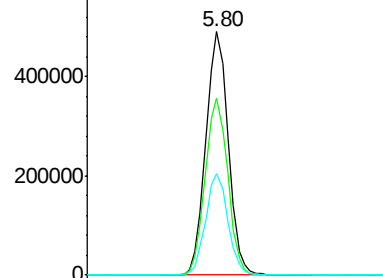

Time-->

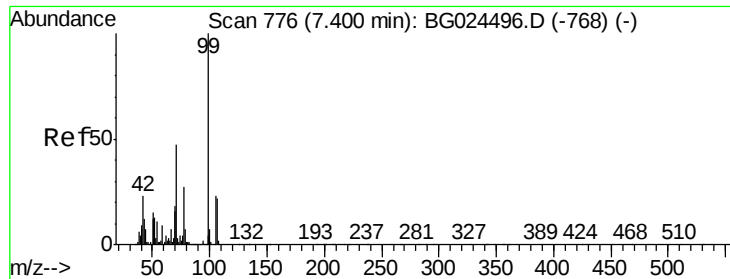

#7

Phenol-d6

Concen: 122.15 ng

RT: 7.40 min Scan# 777

Delta R.T. 0.00 min

Lab File: BG024633.D

Acq: 2 Nov 2016 19:58

Instrument :

BNA_G

ClientSampleId :

PB94494BL


Tgt Ion: 99 Resp: 1137917

Ion Ratio Lower Upper




99 100

42 22.2 20.5 30.7

71 47.8 37.6 56.4

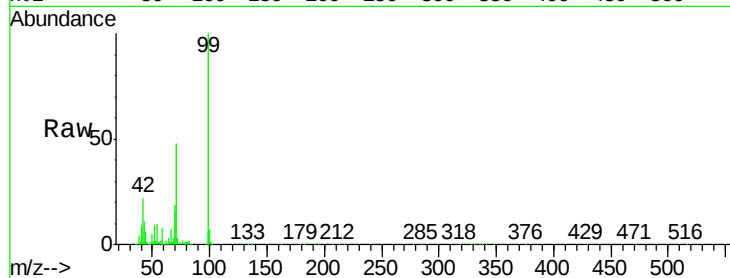

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

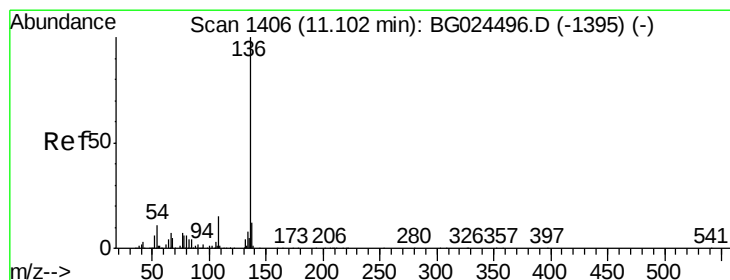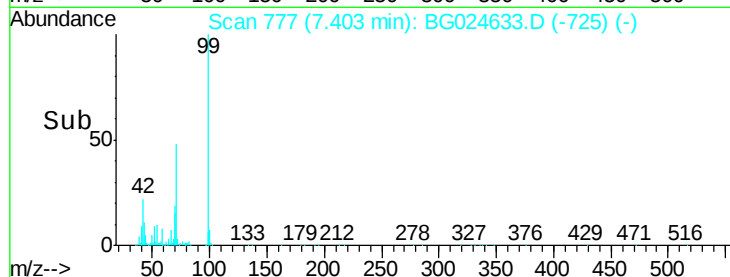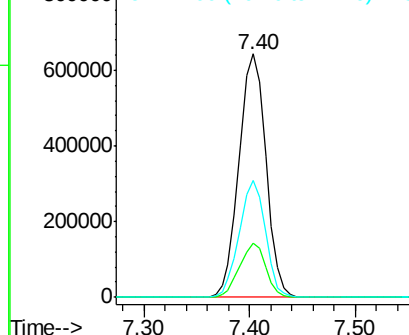

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.09 min Scan# 1405

Delta R.T. -0.01 min

Lab File: BG024633.D

Acq: 2 Nov 2016 19:58

Tgt Ion: 136 Resp: 422254


Ion Ratio Lower Upper

136 100



137 11.9 8.9 13.3


54 10.2 9.3 13.9

68 5.3 5.1 7.7

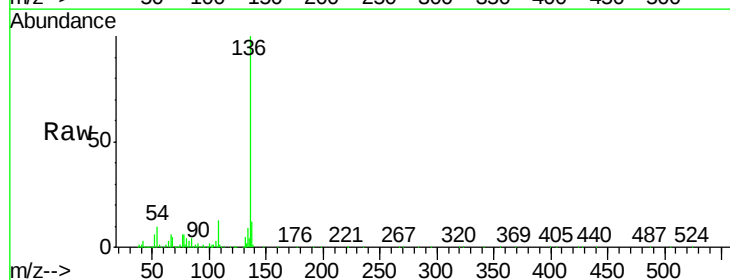

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



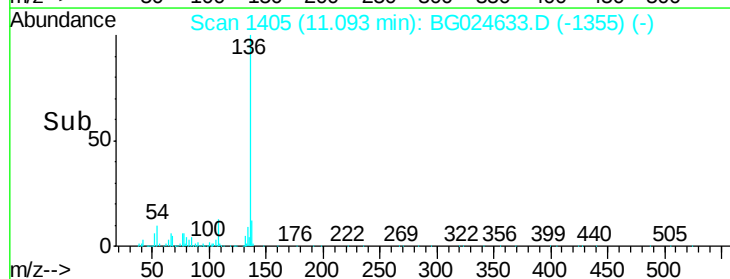
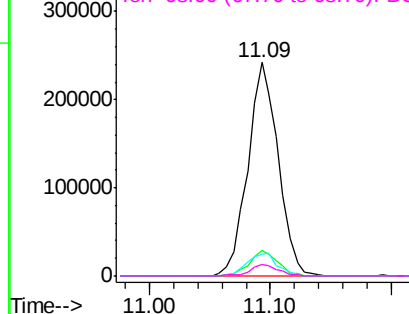


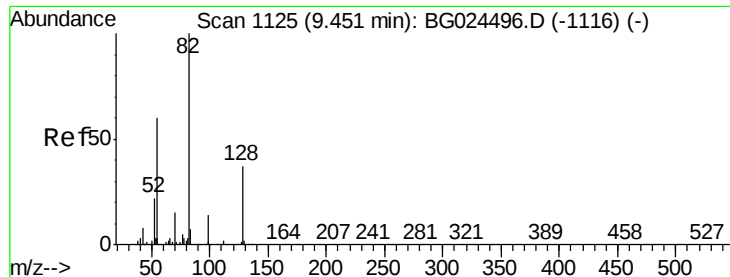

#23
Nitrobenzene-d5
Concen: 85.59 ng
RT: 9.44 min Scan# 1124
Delta R.T. -0.01 min
Lab File: BG024633.D
Acq: 2 Nov 2016 19:58




Instrument :
BNA_G
ClientSampleId :
PB94494BL


Tgt Ion	Ratio	Lower	Upper
82	100		
128	33.7	26.4	39.6
54	57.6	49.4	74.2

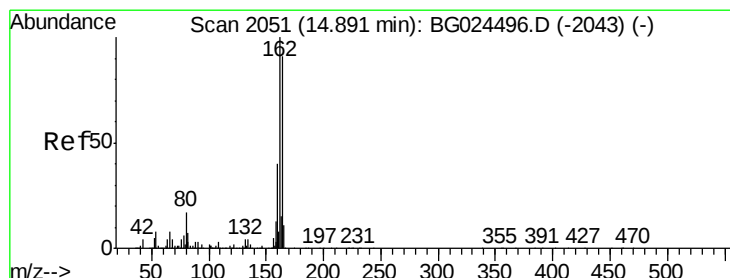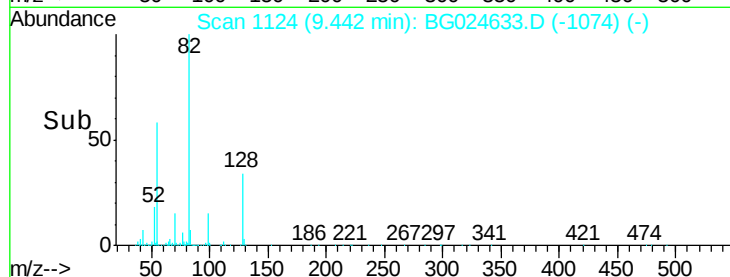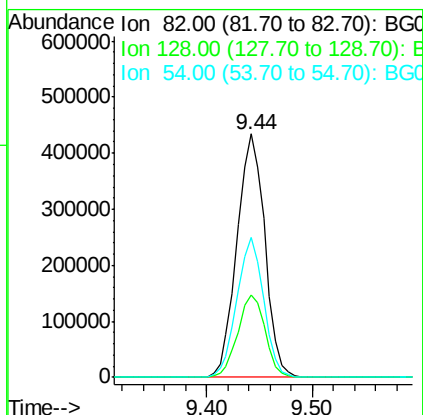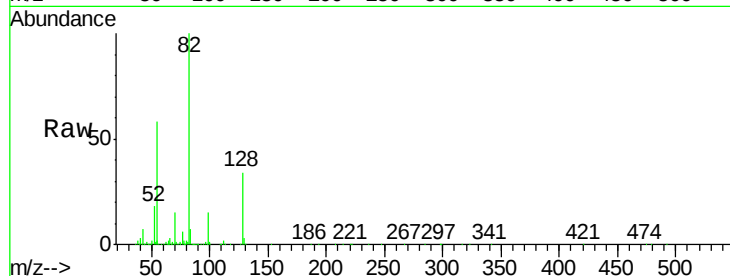

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.88 min Scan# 2050
Delta R.T. -0.01 min
Lab File: BG024633.D
Acq: 2 Nov 2016 19:58

Tgt Ion	Ratio	Lower	Upper
164	100		
162	111.7	85.1	127.7
160	40.1	34.7	52.1


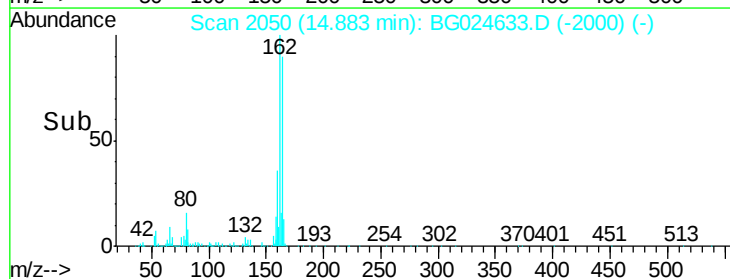
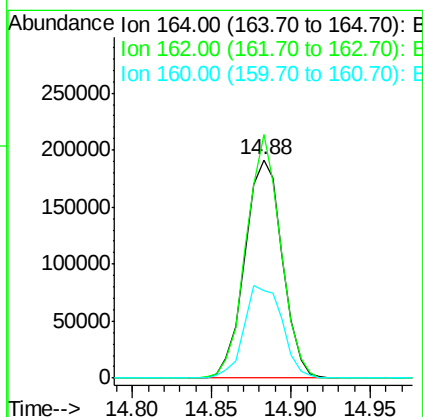
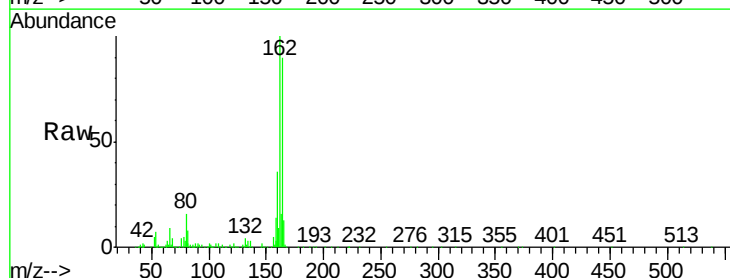


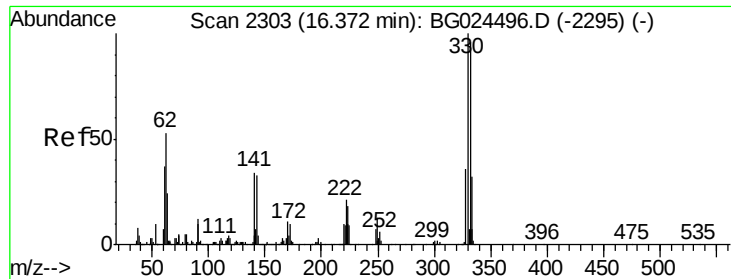

#41
 2,4,6-Tribromophenol
 Concen: 120.22 ng
 RT: 16.37 min Scan# 2303
 Delta R.T. -0.00 min
 Lab File: BG024633.D
 Acq: 2 Nov 2016 19:58




Instrument :
 BNA_G
 ClientSampleId :
 PB94494BL


Tgt Ion:330 Resp: 564276
 Ion Ratio Lower Upper
 330 100
 332 94.7 77.3 115.9
 141 31.0 32.1 48.1#

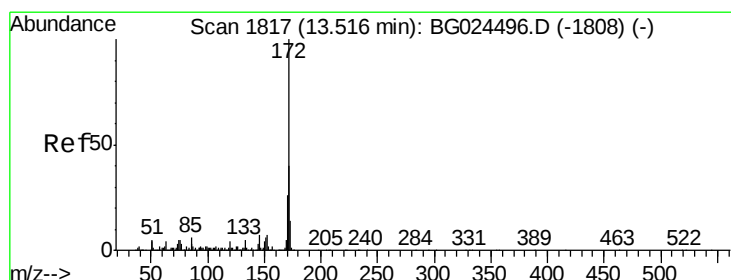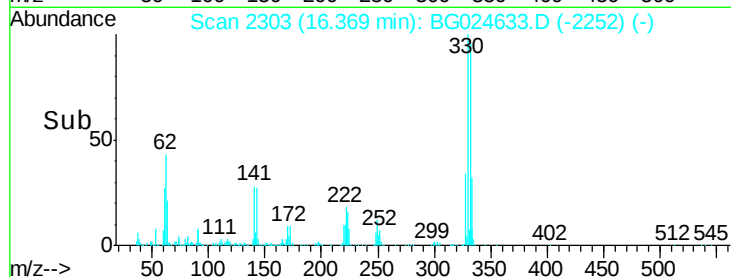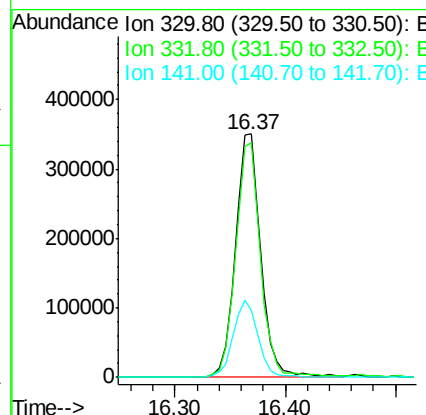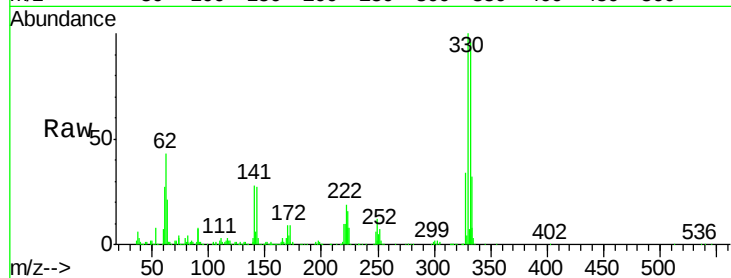

#44
 2-Fluorobiphenyl
 Concen: 84.44 ng
 RT: 13.51 min Scan# 1816
 Delta R.T. -0.01 min
 Lab File: BG024633.D
 Acq: 2 Nov 2016 19:58

Tgt Ion:172 Resp: 1596041
 Ion Ratio Lower Upper
 172 100
 171 38.7 32.2 48.2
 170 26.6 21.8 32.6

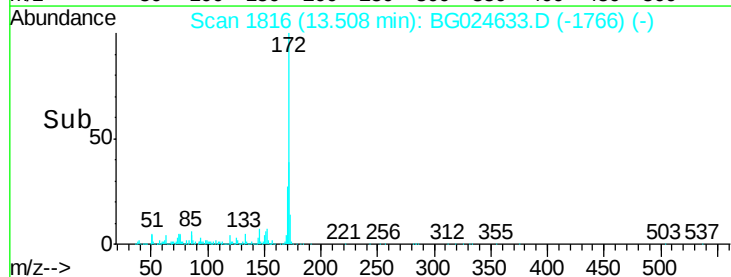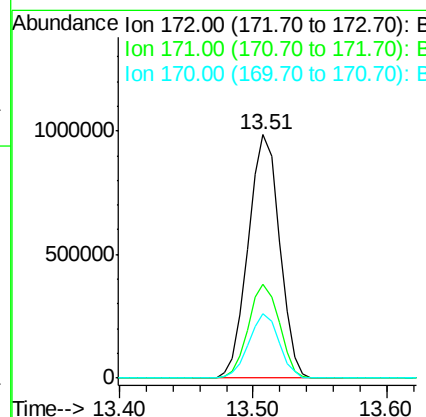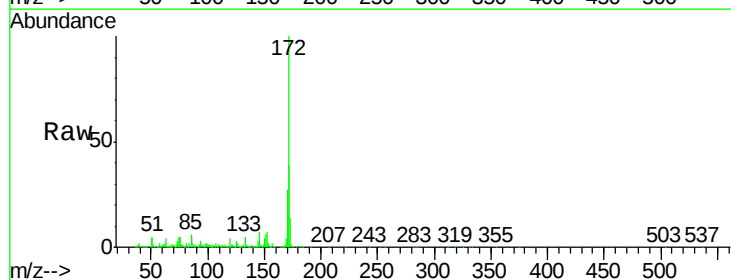

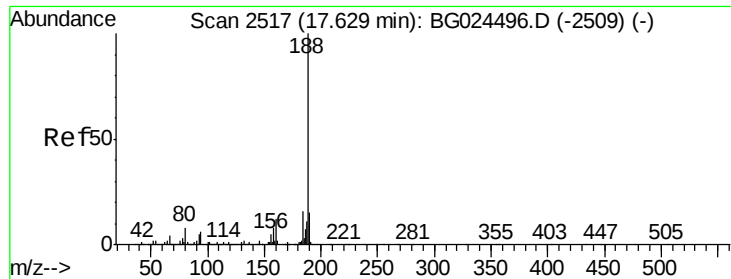

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.62 min Scan# 2516

Delta R.T. -0.01 min

Lab File: BG024633.D

Acq: 2 Nov 2016 19:58

Instrument :

BNA_G

ClientSampleId :

PB94494BL


Tgt Ion:188 Resp: 704641

Ion Ratio Lower Upper

188 100

94 6.8 5.8 8.8




80 8.7 7.5 11.3

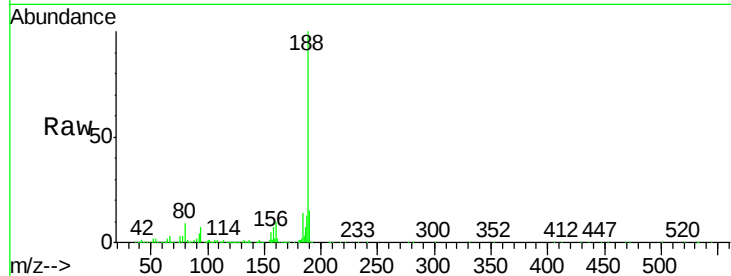

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

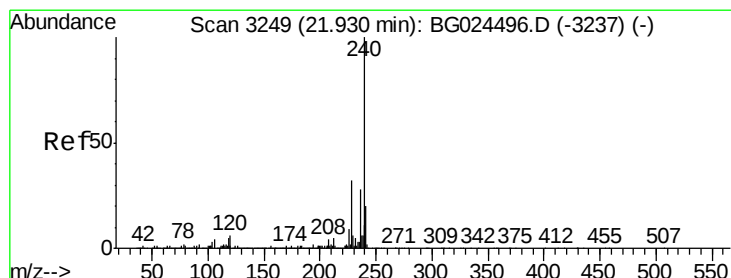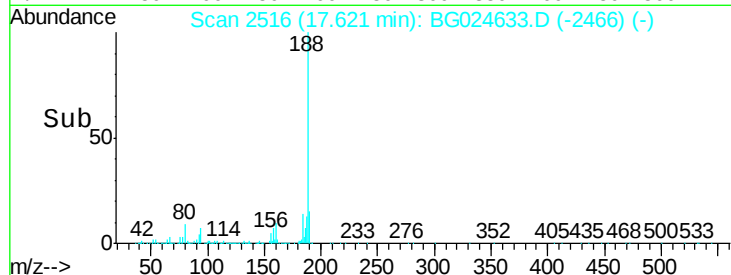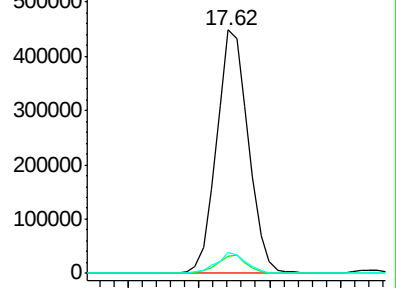

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.92 min Scan# 3247

Delta R.T. -0.01 min

Lab File: BG024633.D

Acq: 2 Nov 2016 19:58


Tgt Ion:240 Resp: 1046180

Ion Ratio Lower Upper

240 100

120 5.9 5.7 8.5



236 27.9 22.2 33.4

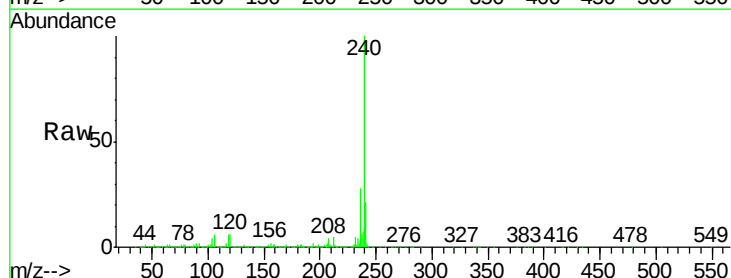


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

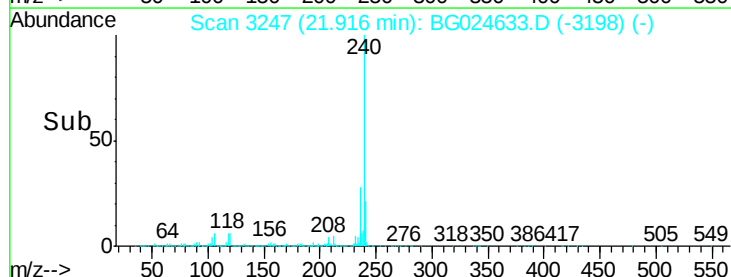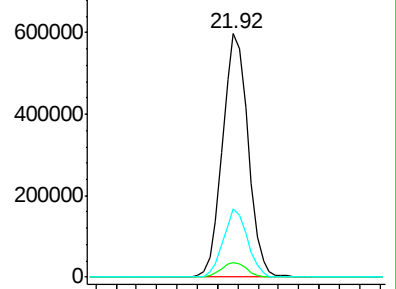

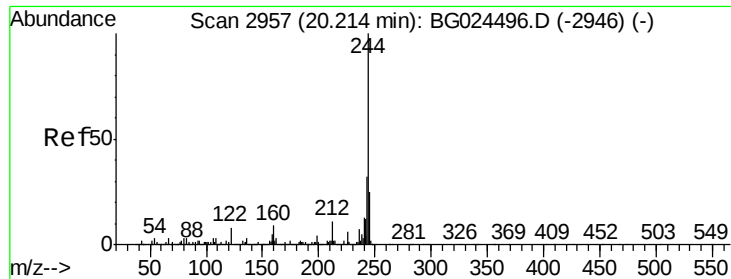

#78

Terphenyl-d14

Concen: 83.00 ng

RT: 20.21 min Scan# 2956

Delta R.T. -0.01 min

Lab File: BG024633.D

Acq: 2 Nov 2016 19:58

Instrument :

BNA_G

ClientSampleId :

PB94494BL


Tgt Ion:244 Resp: 2905863

Ion Ratio Lower Upper

244 100

212 11.0 10.0 15.0




122 9.3 8.6 12.8

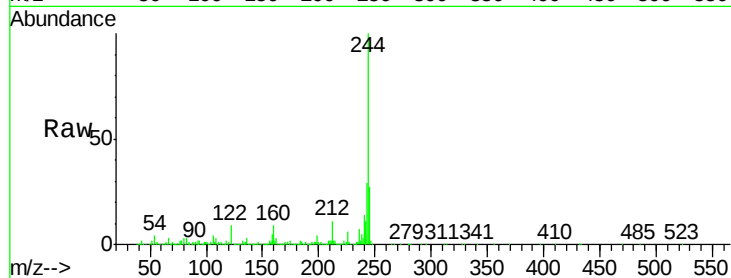

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

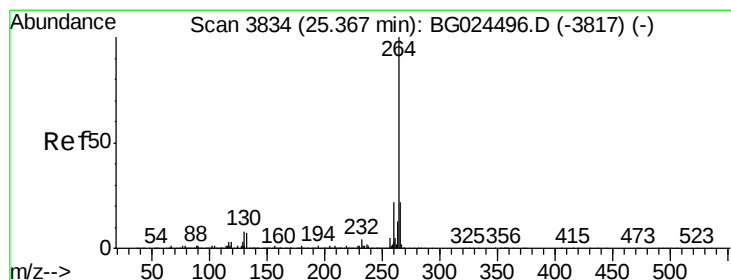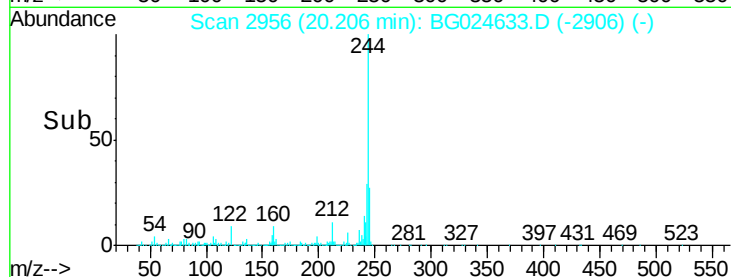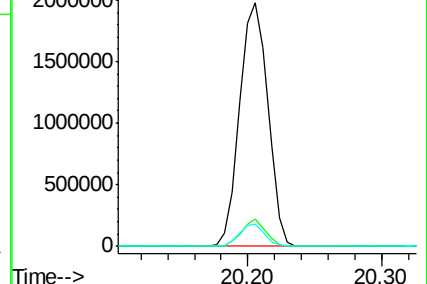

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.35 min Scan# 3831

Delta R.T. -0.02 min

Lab File: BG024633.D

Acq: 2 Nov 2016 19:58


Tgt Ion:264 Resp: 1080296

Ion Ratio Lower Upper

264 100

260 23.2 21.8 32.8

265 21.5 18.2 27.4

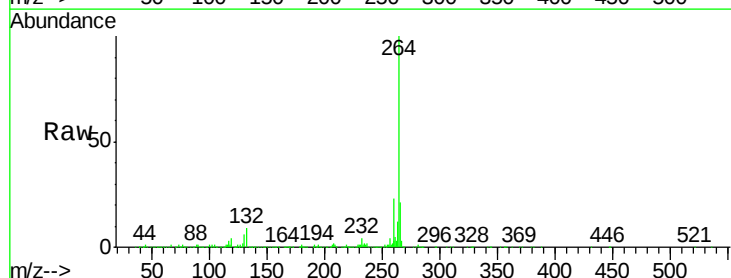

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

