

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110216\
 Data File : BG024642.D
 Acq On : 3 Nov 2016 1:47
 Operator : UM/SJ
 Sample : H5491-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GW-76-6.8-18.0

Quant Time: Nov 03 02:36:12 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	115573	20.00	ng	0.00
21) Naphthalene-d8	11.10	136	430777	20.00	ng	0.00
38) Acenaphthene-d10	14.88	164	332461	20.00	ng	0.00
63) Phenanthrene-d10	17.63	188	725546	20.00	ng	0.00
75) Chrysene-d12	21.92	240	1045401	20.00	ng	-0.01
86) Perylene-d12	25.35	264	1068772	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.80	112	110822	15.72	ng	0.00
7) Phenol-d6	7.40	99	114541	11.84	ng	0.00
23) Nitrobenzene-d5	9.44	82	651854	68.90	ng	0.00
41) 2,4,6-Tribromophenol	16.36	330	80313	16.17	ng	0.00
44) 2-Fluorobiphenyl	13.51	172	1352678	67.63	ng	0.00
78) Terphenyl-d14	20.21	244	2422851	69.25	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110216\
Data File : BG024642.D
Acq On : 3 Nov 2016 1:47
Operator : UM/SJ
Sample : H5491-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-76-6.8-18.0

Quant Time: Nov 03 02:36:12 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

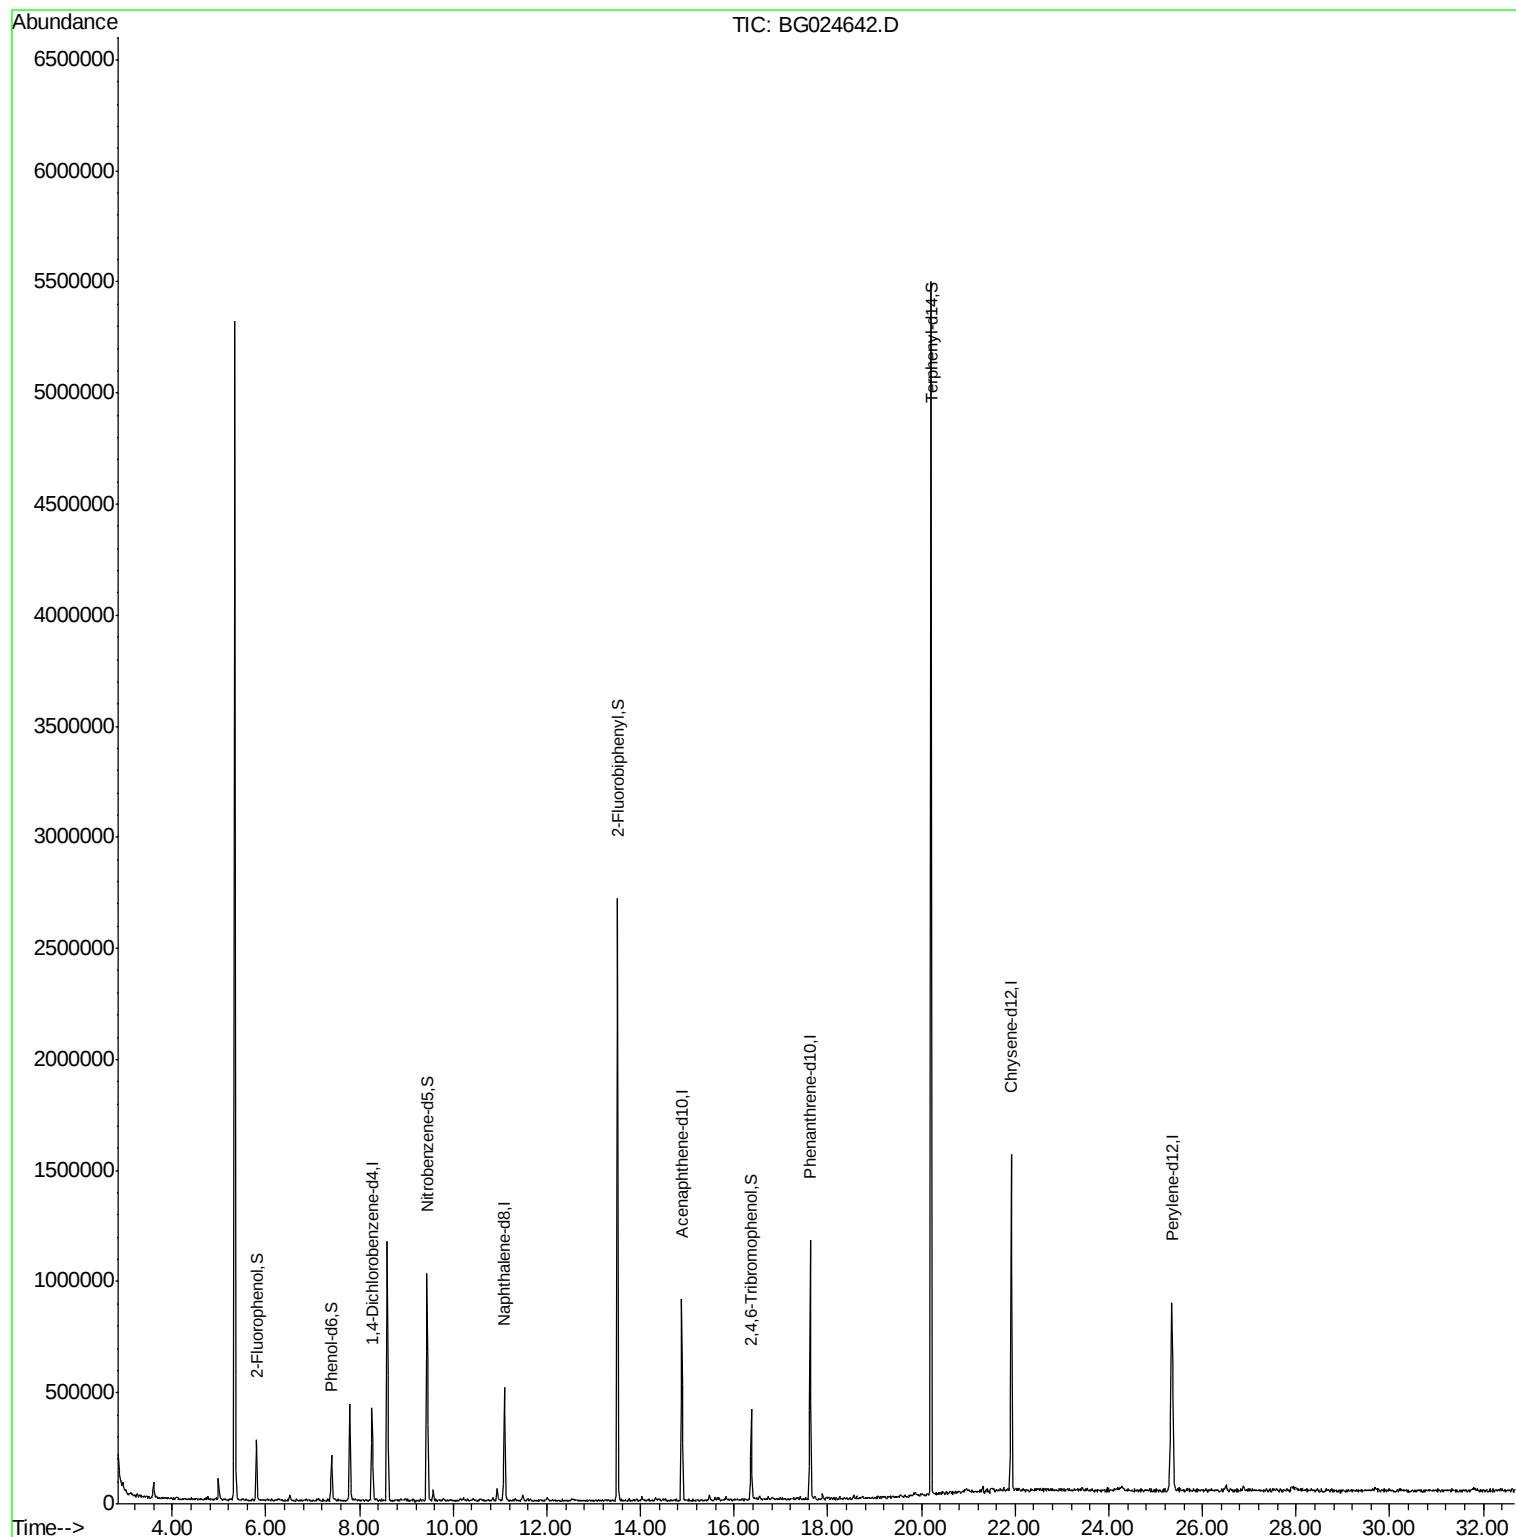

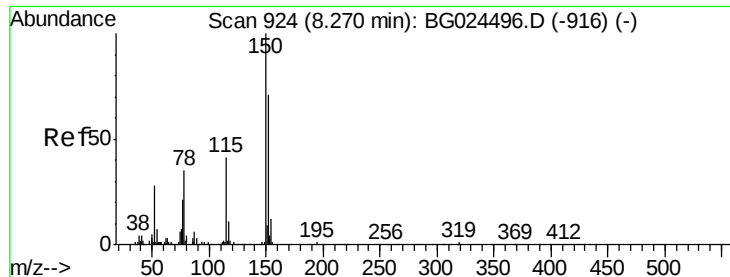

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.27 min Scan# 924

Delta R.T. -0.00 min

Lab File: BG024642.D

Acq: 3 Nov 2016 1:47

Instrument :

BNA_G

ClientSampleId :

GW-76-6.8-18.0


Tgt Ion:152 Resp: 115573

Ion Ratio Lower Upper

152 100

150 153.8 114.0 171.0




115 62.4 48.1 72.1

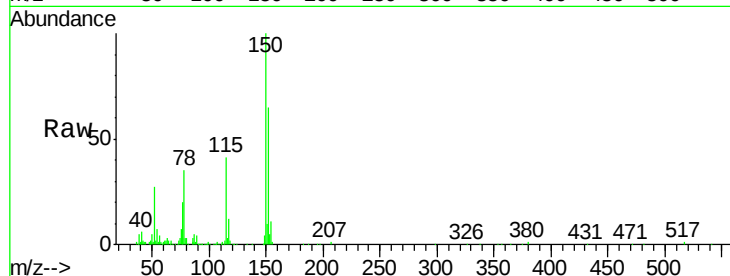

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

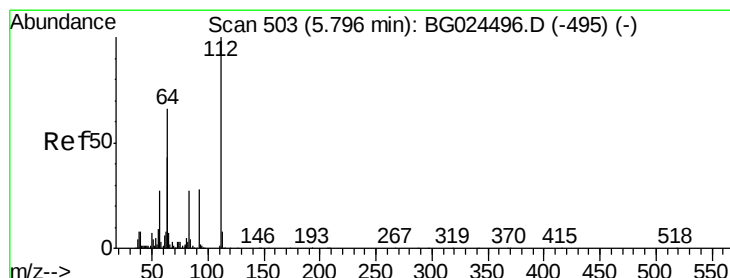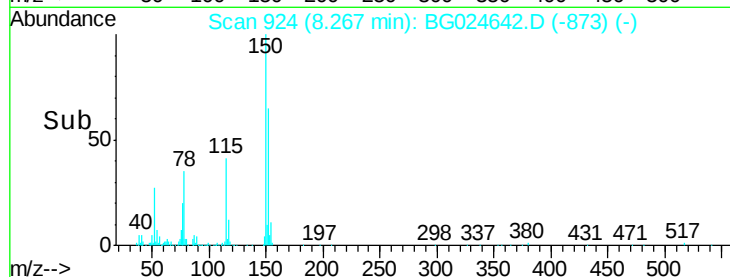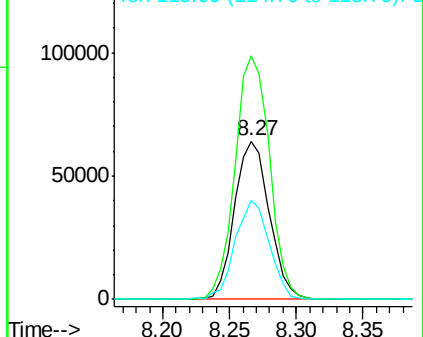

#5

2-Fluorophenol

Concen: 15.72 ng

RT: 5.80 min Scan# 504

Delta R.T. 0.00 min

Lab File: BG024642.D

Acq: 3 Nov 2016 1:47


Tgt Ion:112 Resp: 110822

Ion Ratio Lower Upper

112 100

64 70.9 61.8 92.6



63 40.3 37.2 55.8

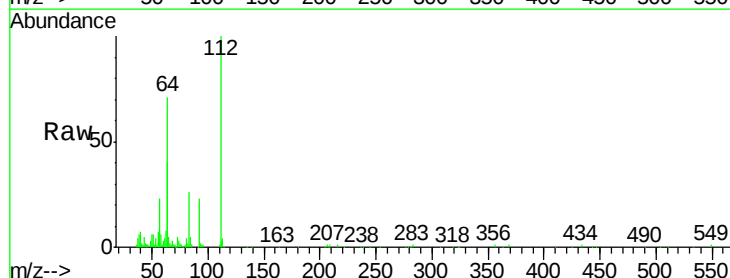

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

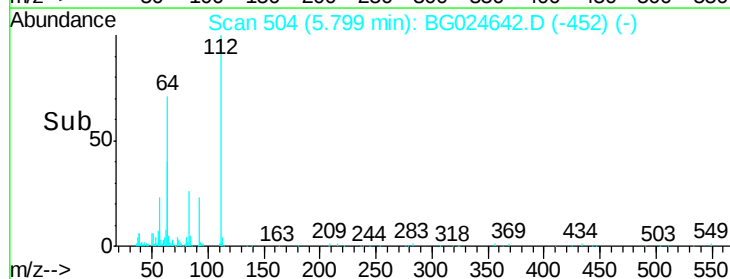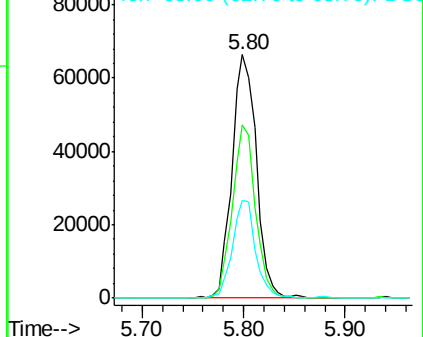



#7

Phenol-d6

Concen: 11.84 ng

RT: 7.40 min Scan# 777

Delta R.T. 0.00 min

Lab File: BG024642.D

Acq: 3 Nov 2016 1:47

Instrument :

BNA_G

ClientSampleId :

GW-76-6.8-18.0


Tgt Ion: 99 Resp: 114541

Ion Ratio Lower Upper




99 100

42 20.3 20.5 30.7#

71 41.9 37.6 56.4

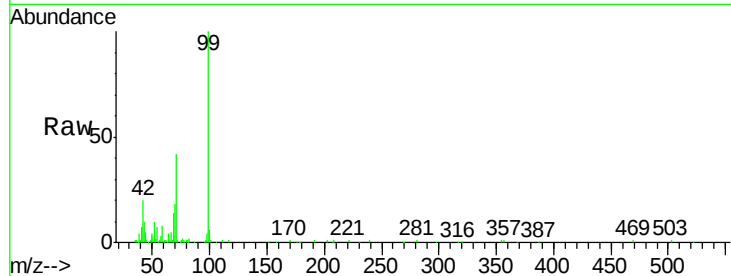

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

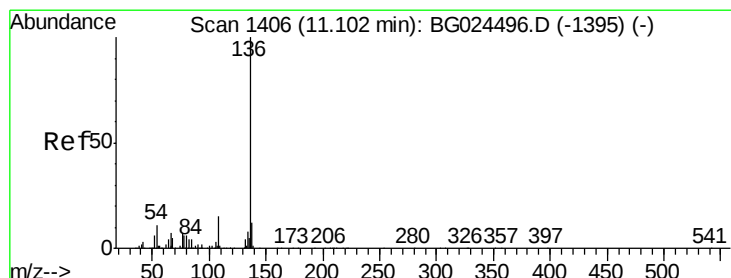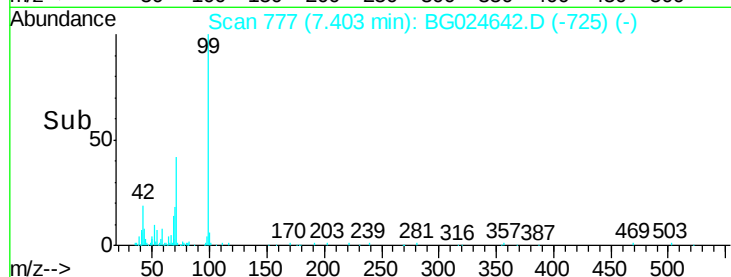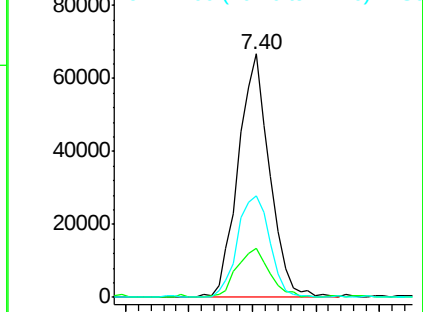

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.10 min Scan# 1406

Delta R.T. -0.00 min

Lab File: BG024642.D

Acq: 3 Nov 2016 1:47

Tgt Ion: 136 Resp: 430777


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 11.7 9.3 13.9

68 4.5 5.1 7.7#

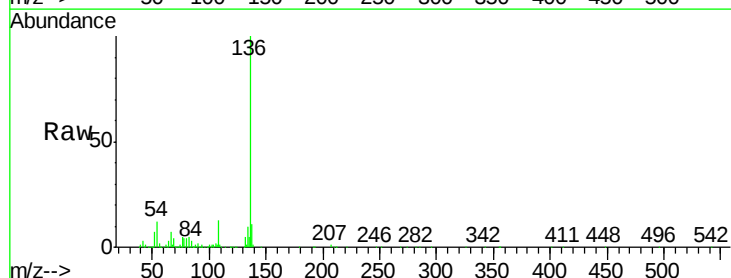

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



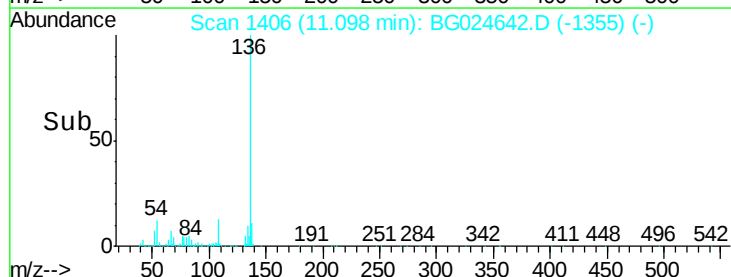
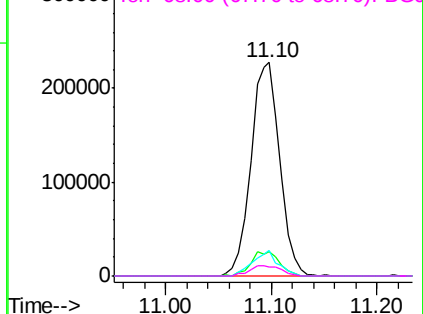


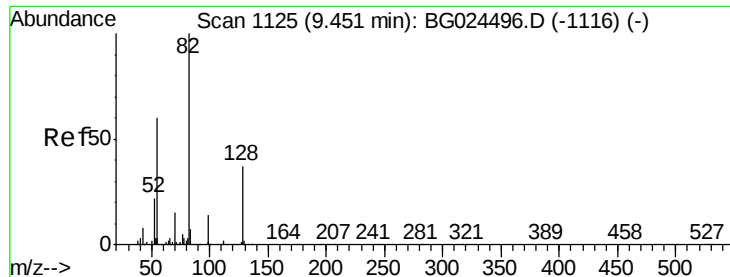

#23
 Nitrobenzene-d5
 Concen: 68.90 ng
 RT: 9.44 min Scan# 1124
 Delta R.T. -0.01 min
 Lab File: BG024642.D
 Acq: 3 Nov 2016 1:47




Instrument :
 BNA_G
 ClientSampleId :
 GW-76-6.8-18.0

Tgt Ion	Ratio	Lower	Upper
82	100		
128	33.7	26.4	39.6
54	53.0	49.4	74.2

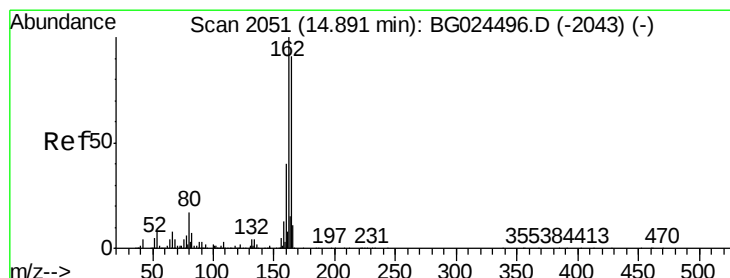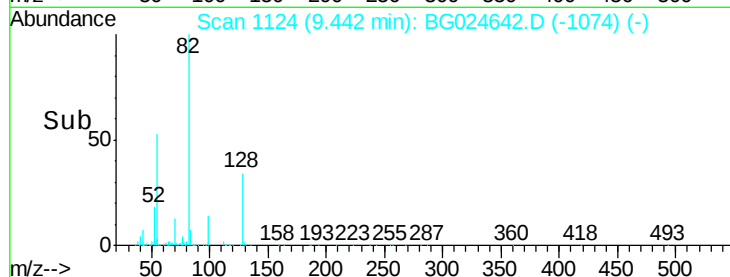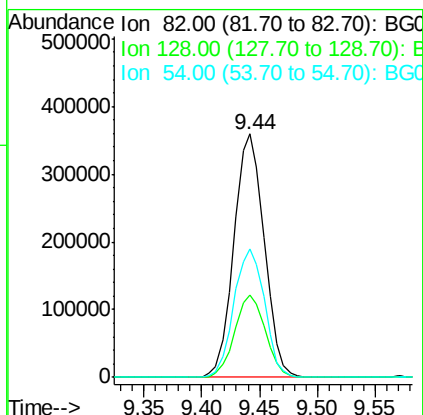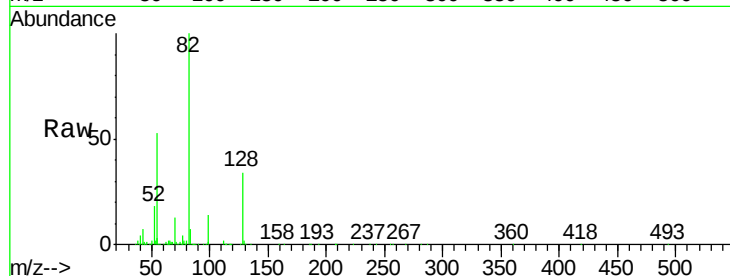

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.88 min Scan# 2050
 Delta R.T. -0.01 min
 Lab File: BG024642.D
 Acq: 3 Nov 2016 1:47

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.9	85.1	127.7
160	44.5	34.7	52.1

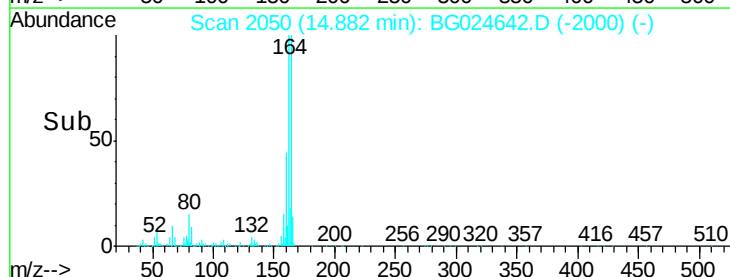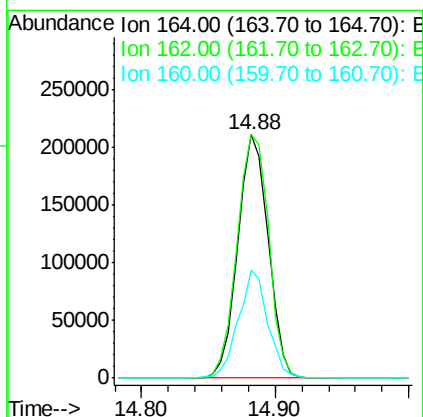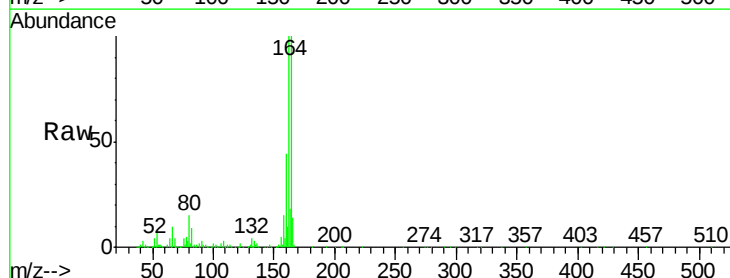







#41
 2,4,6-Tribromophenol
 Concen: 16.17 ng
 RT: 16.36 min Scan# 2302
 Delta R.T. -0.01 min
 Lab File: BG024642.D
 Acq: 3 Nov 2016 1:47

Instrument :
 BNA_G
 ClientSampleId :
 GW-76-6.8-18.0

Tgt Ion:330 Resp: 80313
 Ion Ratio Lower Upper
 330 100
 332 103.4 77.3 115.9
 141 31.0 32.1 48.1#

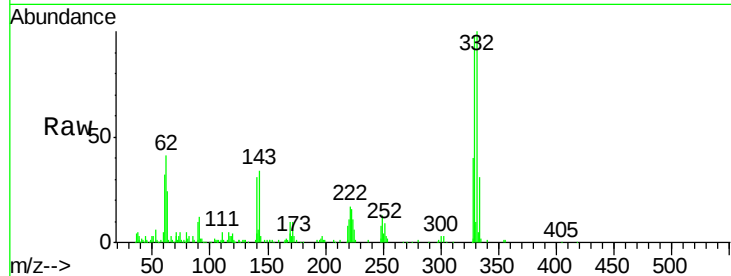


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

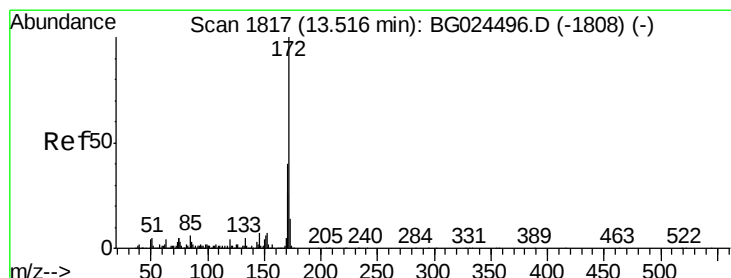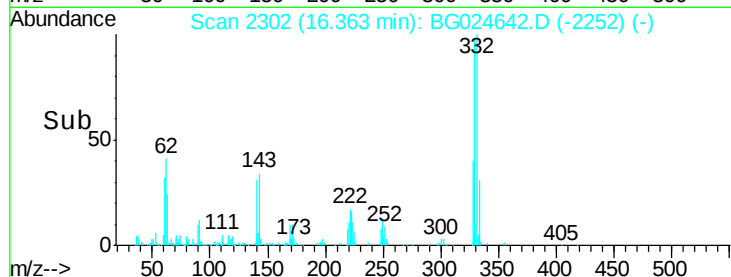
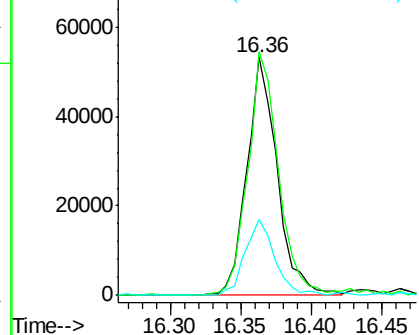



#44
 2-Fluorobiphenyl
 Concen: 67.63 ng
 RT: 13.51 min Scan# 1816
 Delta R.T. -0.01 min
 Lab File: BG024642.D
 Acq: 3 Nov 2016 1:47

Tgt Ion:172 Resp: 1352678
 Ion Ratio Lower Upper
 172 100
 171 39.1 32.2 48.2
 170 26.0 21.8 32.6

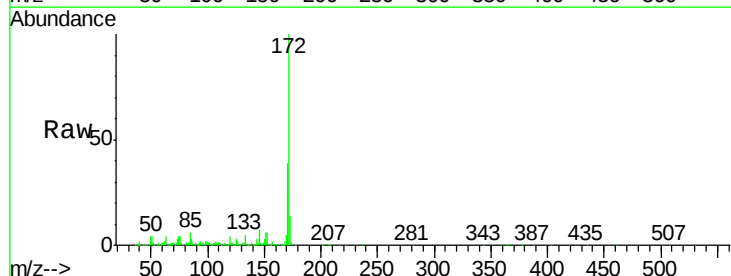

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

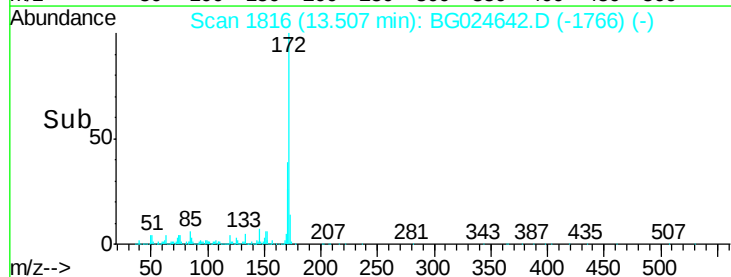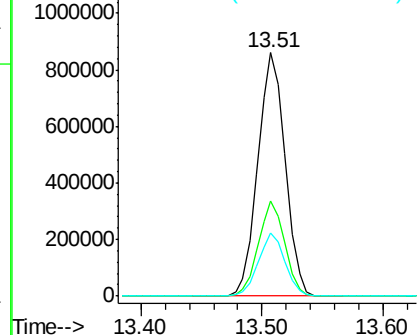

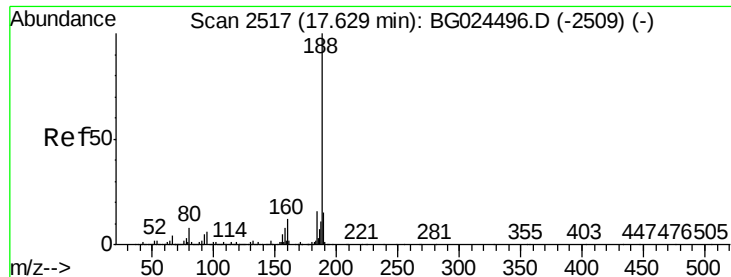

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.63 min Scan# 2517

Delta R.T. -0.00 min

Lab File: BG024642.D

Acq: 3 Nov 2016 1:47

Instrument :

BNA_G

ClientSampleId :

GW-76-6.8-18.0


Tgt Ion:188 Resp: 725546

Ion Ratio Lower Upper

188 100

94 6.4 5.8 8.8

80 8.8 7.5 11.3

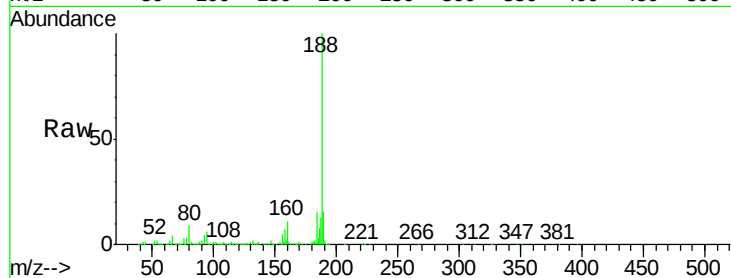

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

600000

500000

400000

300000

200000

100000



0

17.63

17.60

17.70

Time-->

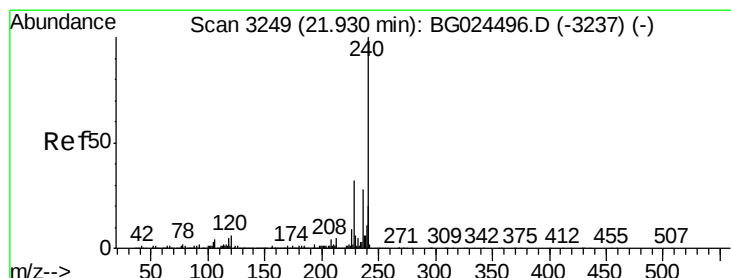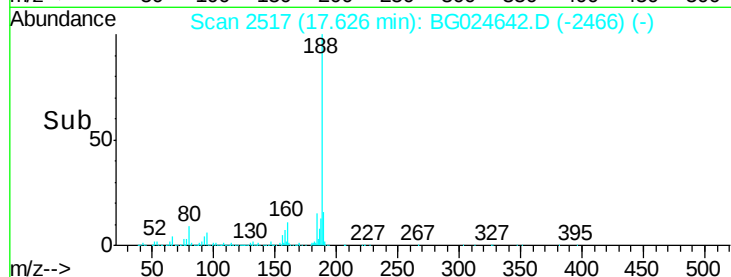

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.92 min Scan# 3247

Delta R.T. -0.01 min

Lab File: BG024642.D

Acq: 3 Nov 2016 1:47


Tgt Ion:240 Resp: 1045401

Ion Ratio Lower Upper

240 100

120 5.5 5.7 8.5#

236 27.4 22.2 33.4

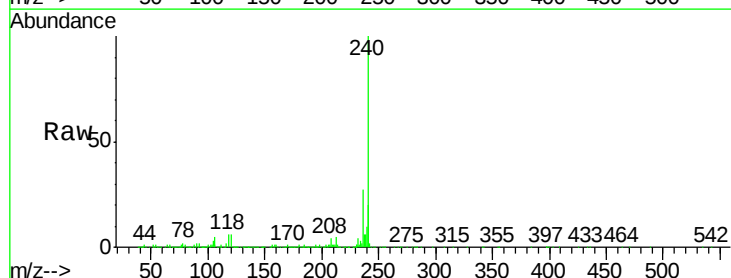

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

800000

600000

400000

200000


0


21.92

21.80

22.00

Time-->

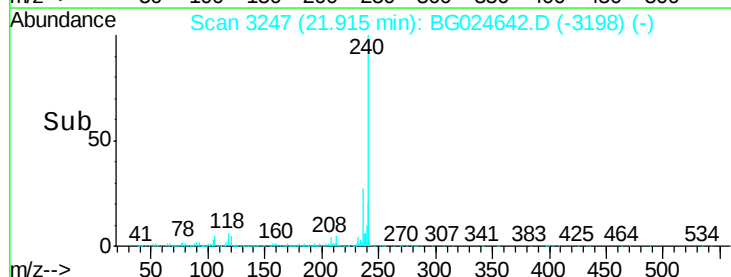

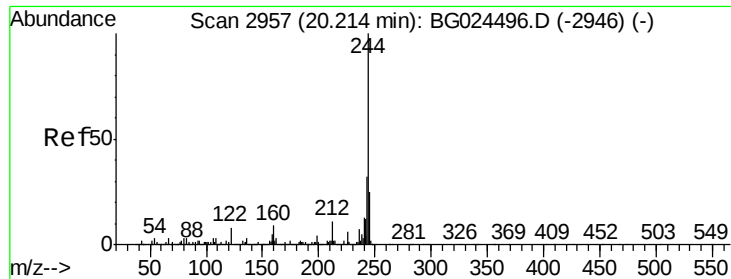

#78

Terphenyl-d14

Concen: 69.25 ng

RT: 20.21 min Scan# 2956

Delta R.T. -0.01 min

Lab File: BG024642.D

Acq: 3 Nov 2016 1:47

Instrument :

BNA_G

ClientSampleId :

GW-76-6.8-18.0


Tgt Ion:244 Resp: 2422851

Ion Ratio Lower Upper

244 100

212 9.0 10.0 15.0#




122 7.8 8.6 12.8#

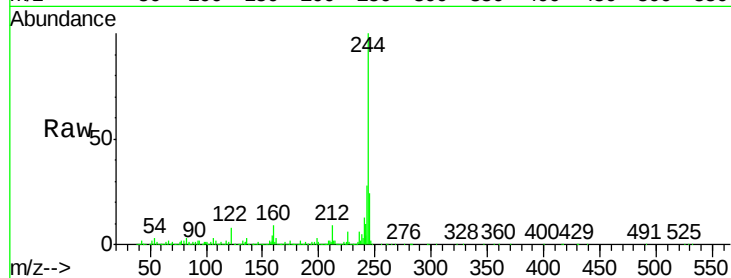

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

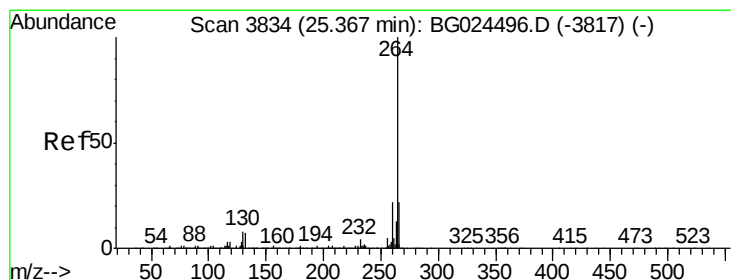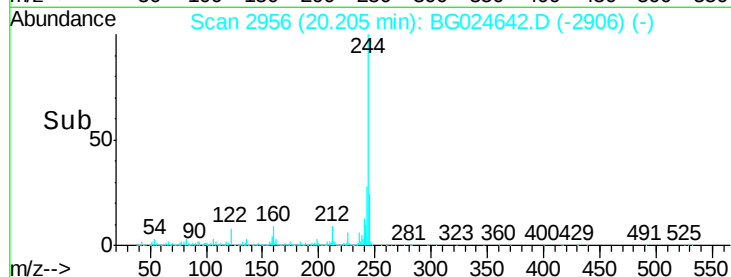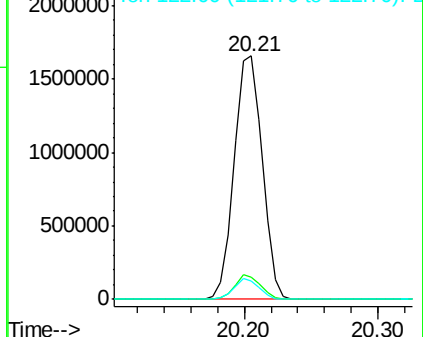

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.35 min Scan# 3831

Delta R.T. -0.02 min

Lab File: BG024642.D

Acq: 3 Nov 2016 1:47


Tgt Ion:264 Resp: 1068772

Ion Ratio Lower Upper

264 100

260 22.3 21.8 32.8

265 19.9 18.2 27.4

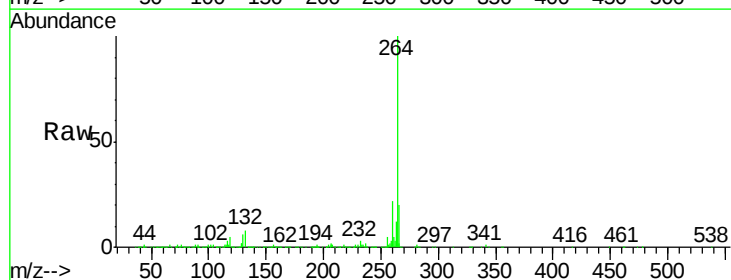

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

