


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110216\
 Data File : BG024627.D
 Acq On : 2 Nov 2016 16:04
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

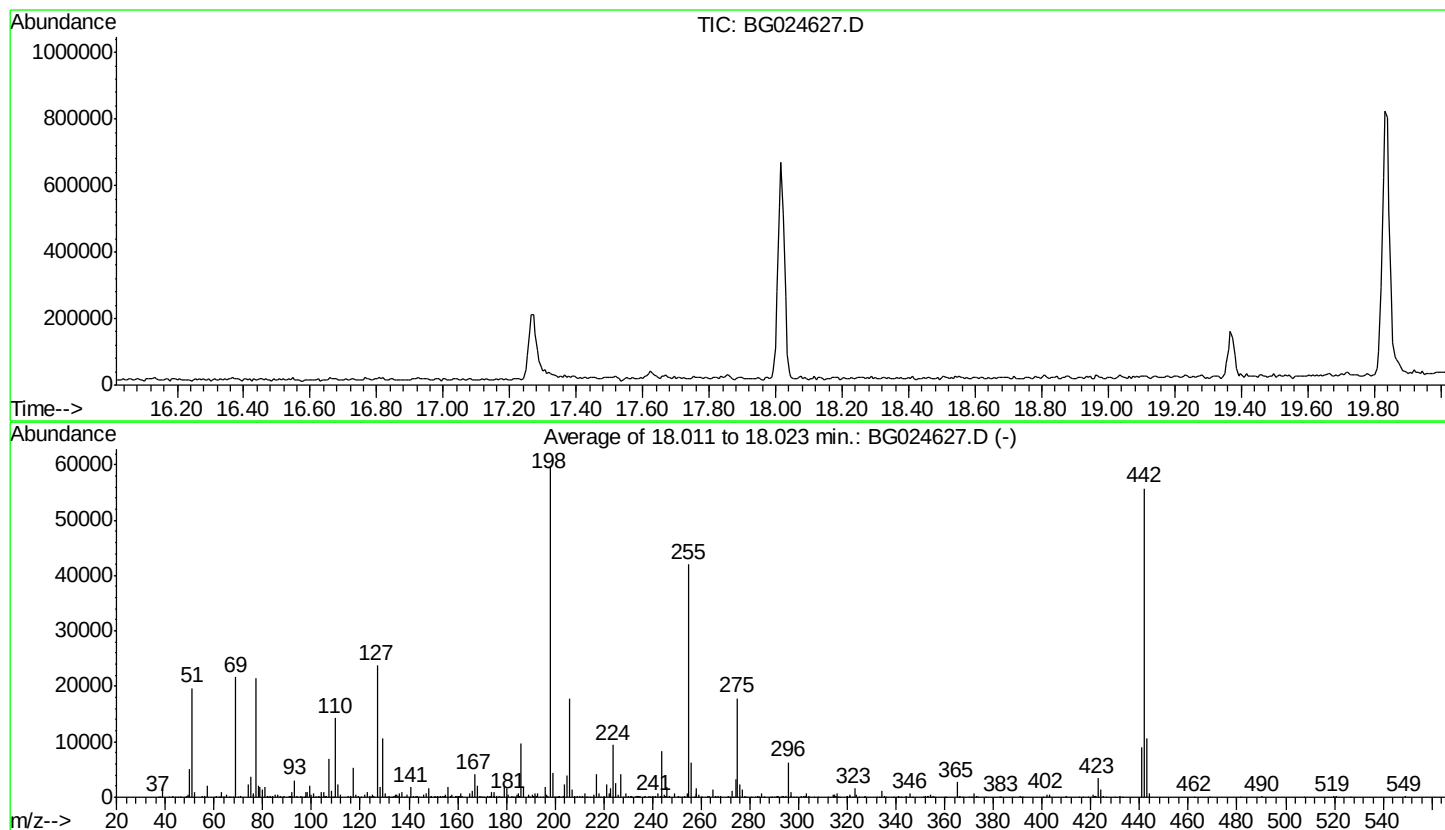

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	19647	PASS
68	69	0.00	2	0.4	91	PASS
69	198	0.00	100	36.2	21629	PASS
70	69	0.00	2	0.3	59	PASS
127	198	10	80	39.7	23757	PASS
197	198	0.00	2	0.7	396	PASS
198	198	100	100	100.0	59826	PASS
199	198	5	9	7.4	4429	PASS
275	198	10	60	29.8	17802	PASS
365	198	1	100	4.5	2709	PASS
441	442	0.01	24	16.1	8937	PASS
442	198	50	100	93.0	55664	PASS
443	442	15	24	19.2	10709	PASS