
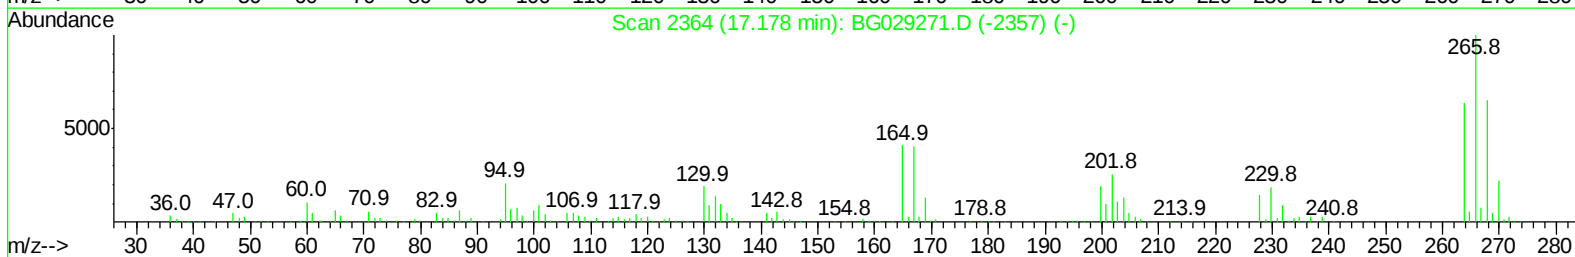
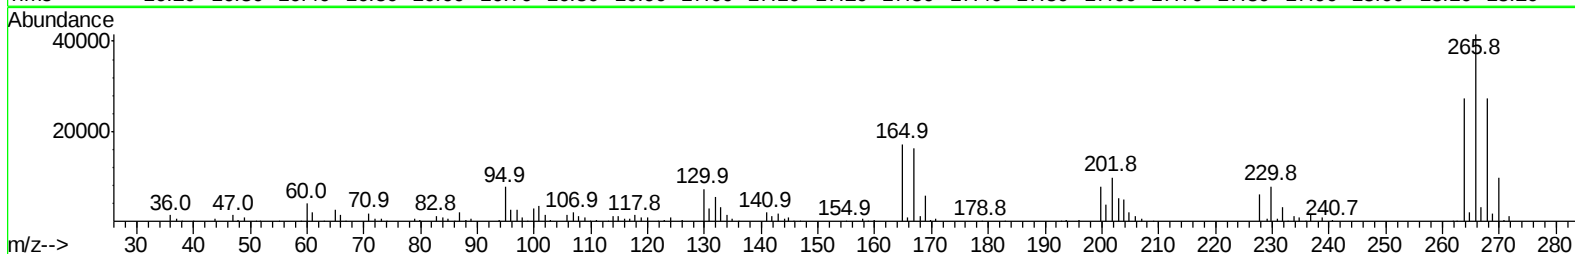


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110217\
Data File : BG030663.D
Acq On : 2 Nov 2017 15:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 07:59:02 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

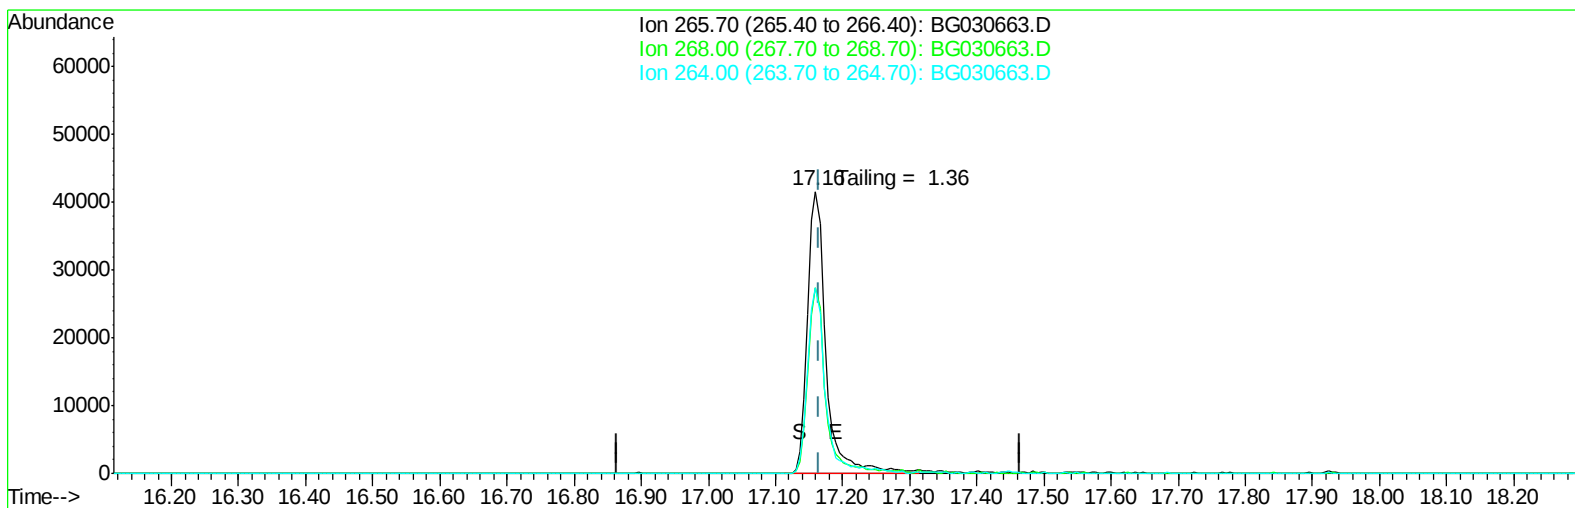

TIC: BG030663.D

(69) Pentachlorophenol (C)




17.160min (-0.005) 0.00ng

response 77254

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.01
264.00	62.00	65.77
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110217\
Data File : BG030663.D
Acq On : 2 Nov 2017 15:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 07:59:02 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

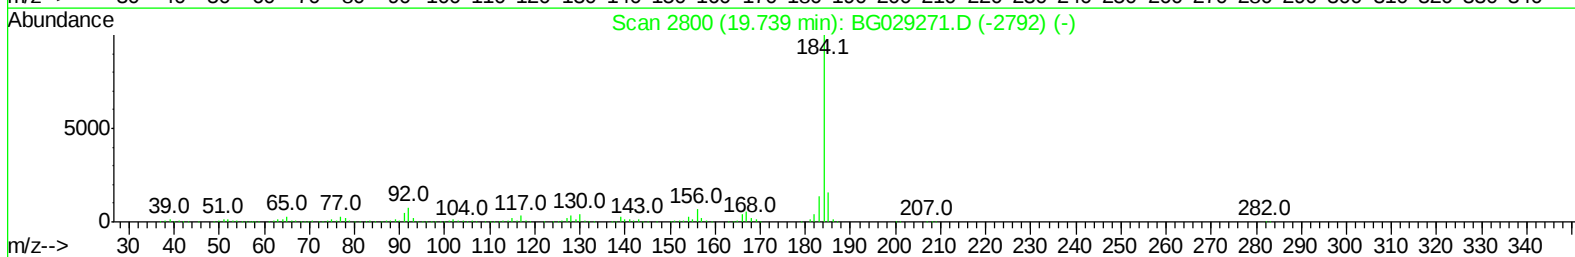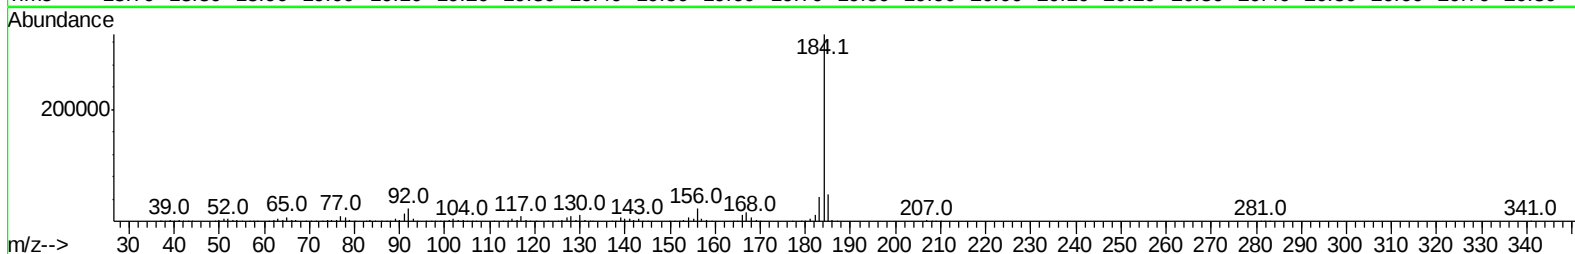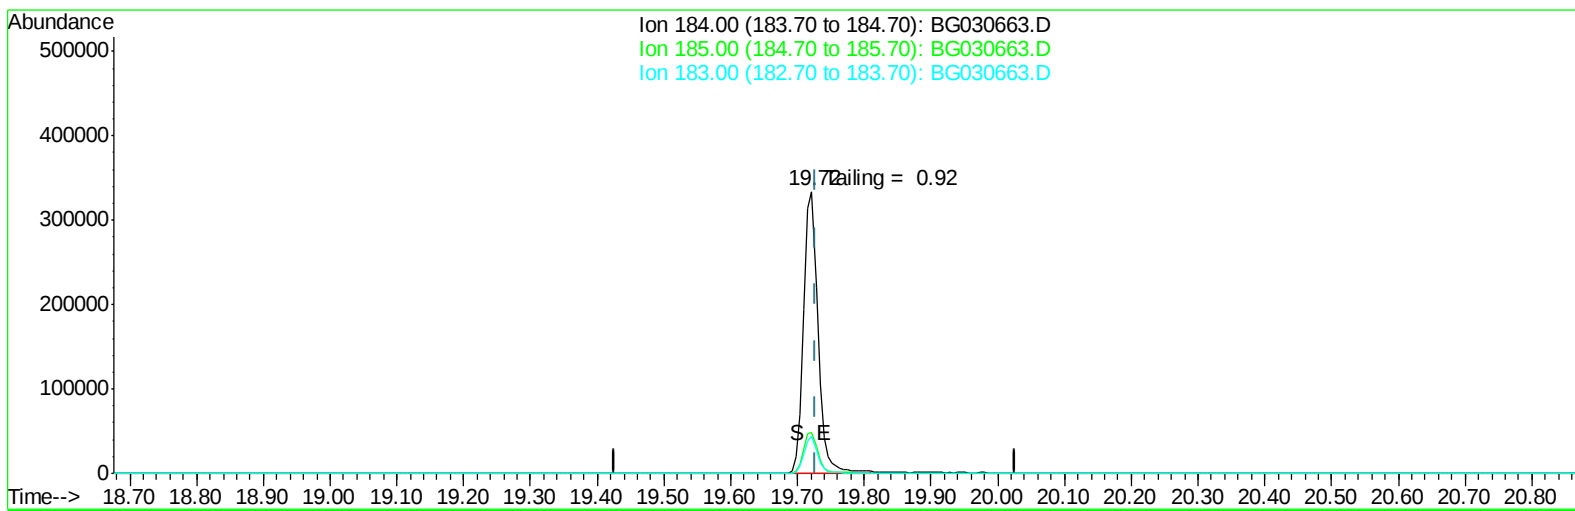

TIC: BG030663.D

(76) Benzidine

19.722min (-0.005) 0.00ng

response 490452

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.62
183.00	13.30	13.28
0.00	0.00	0.00