
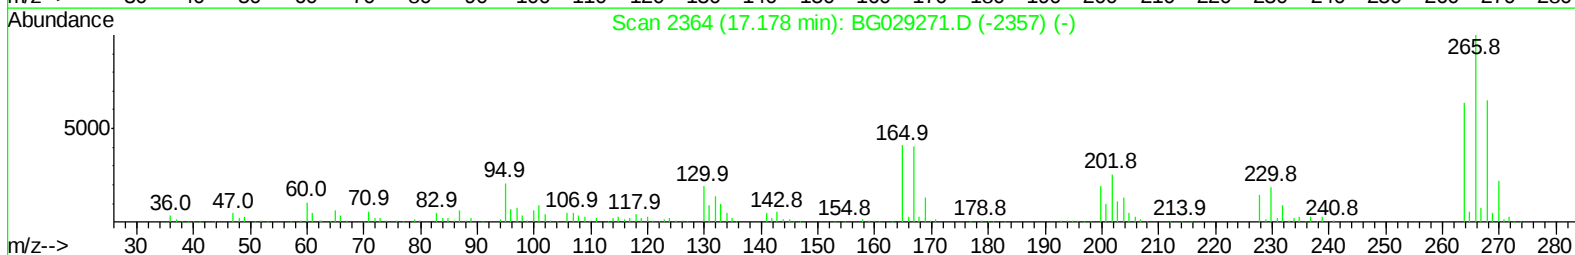
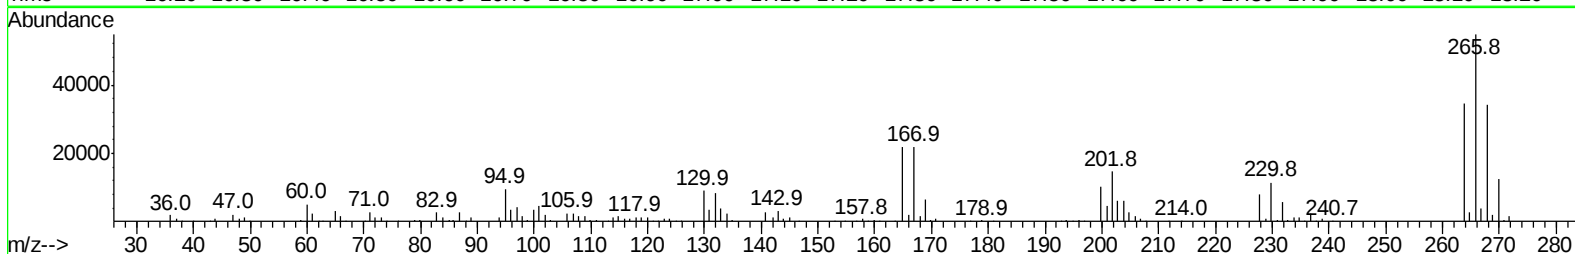


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110217\
Data File : BG030682.D
Acq On : 3 Nov 2017 3:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 08:00:03 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

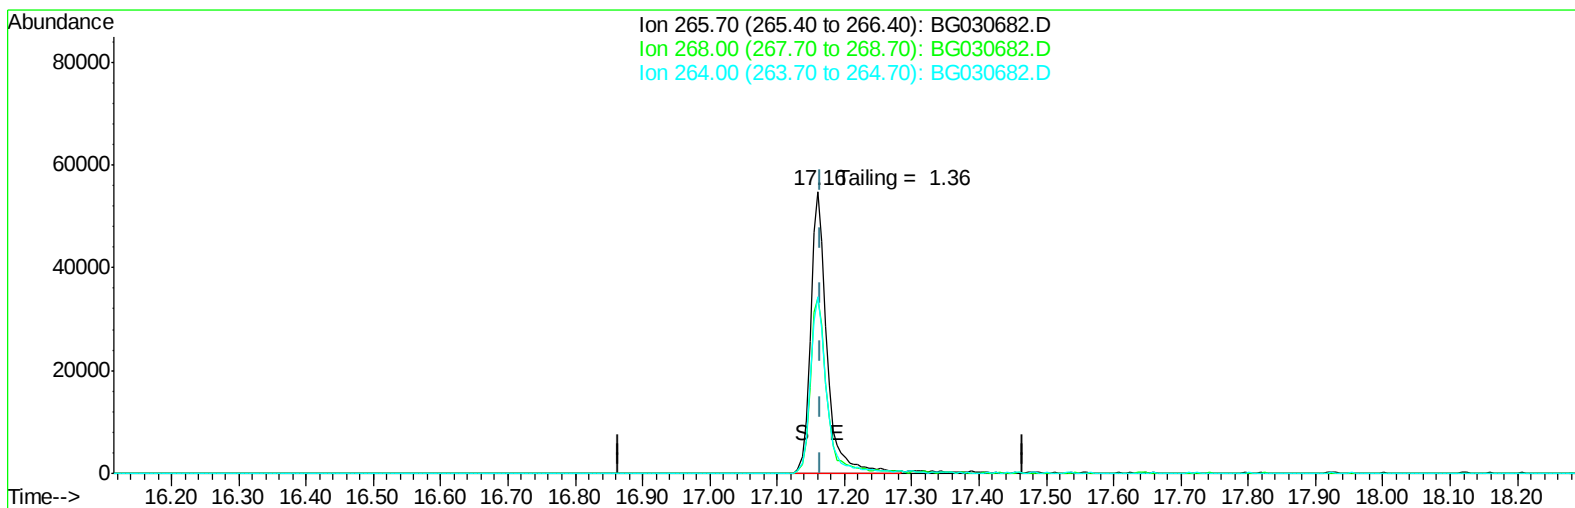

TIC: BG030682.D

(69) Pentachlorophenol (C)




17.160min (-0.005) 0.00ng

response 94204

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.47
264.00	62.00	62.80
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110217\
Data File : BG030682.D
Acq On : 3 Nov 2017 3:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 08:00:03 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

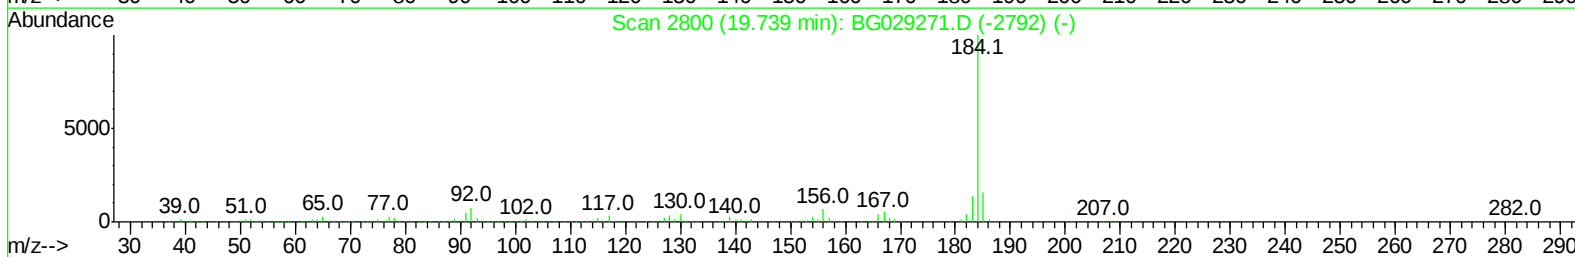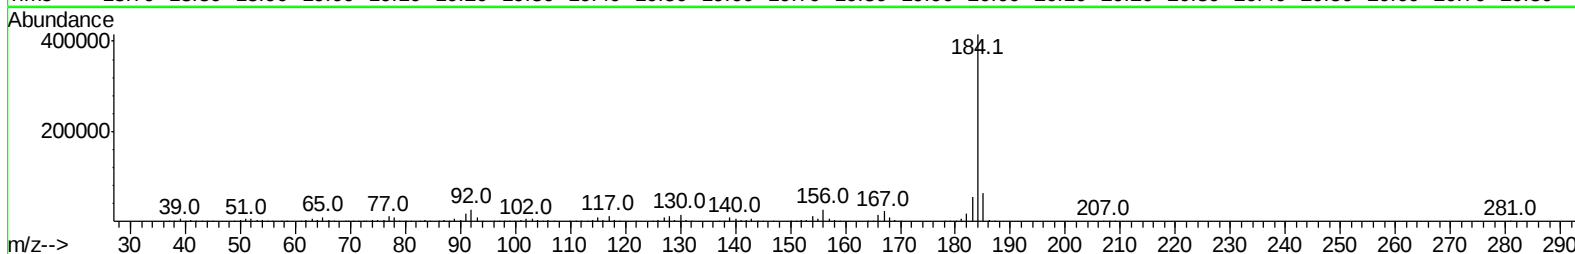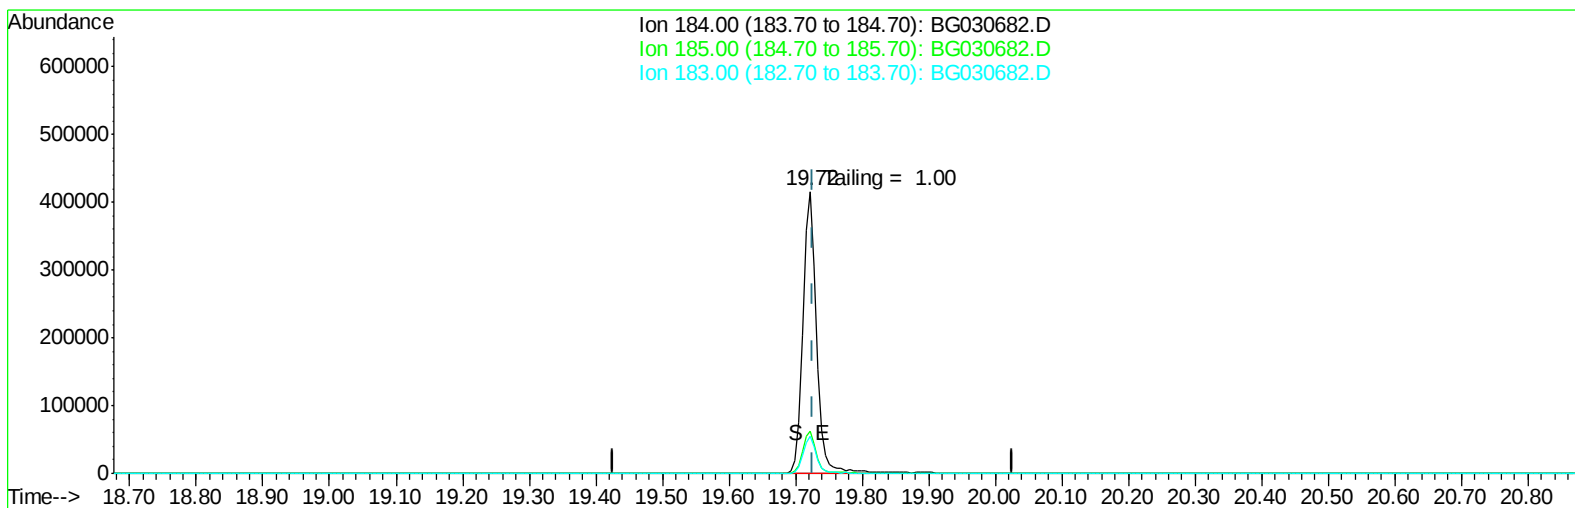

TIC: BG030682.D

(76) Benzidine

19.722min (-0.005) 349817.95ng

response 602049

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.88
183.00	13.30	13.03
0.00	0.00	0.00