

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110217\
 Data File : BG030660.D
 Acq On : 2 Nov 2017 13:44
 Operator : SJ/JU
 Sample : I6249-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMP-1

Quant Time: Nov 03 00:49:22 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 17:41:24 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	62727	20.00	ng	0.00
21) Naphthalene-d8	10.97	136	282903	20.00	ng	0.00
38) Acenaphthene-d10	14.77	164	198945	20.00	ng	0.00
63) Phenanthrene-d10	17.51	188	509851	20.00	ng	0.00
75) Chrysene-d12	21.78	240	571545	20.00	ng	-0.01
86) Perylene-d12	25.07	264	579639	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.71	112	474629	126.40	ng	0.00
7) Phenol-d6	7.31	99	579306	109.91	ng	0.00
23) Nitrobenzene-d5	9.32	82	395370	88.81	ng	0.00
41) 2,4,6-Tribromophenol	16.25	330	389146	151.50	ng	0.00
44) 2-Fluorobiphenyl	13.39	172	1107073	81.62	ng	0.00
78) Terphenyl-d14	20.10	244	2075877	82.63	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110217\
Data File : BG030660.D
Acq On : 2 Nov 2017 13:44
Operator : SJ/JU
Sample : I6249-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-1

Quant Time: Nov 03 00:49:22 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

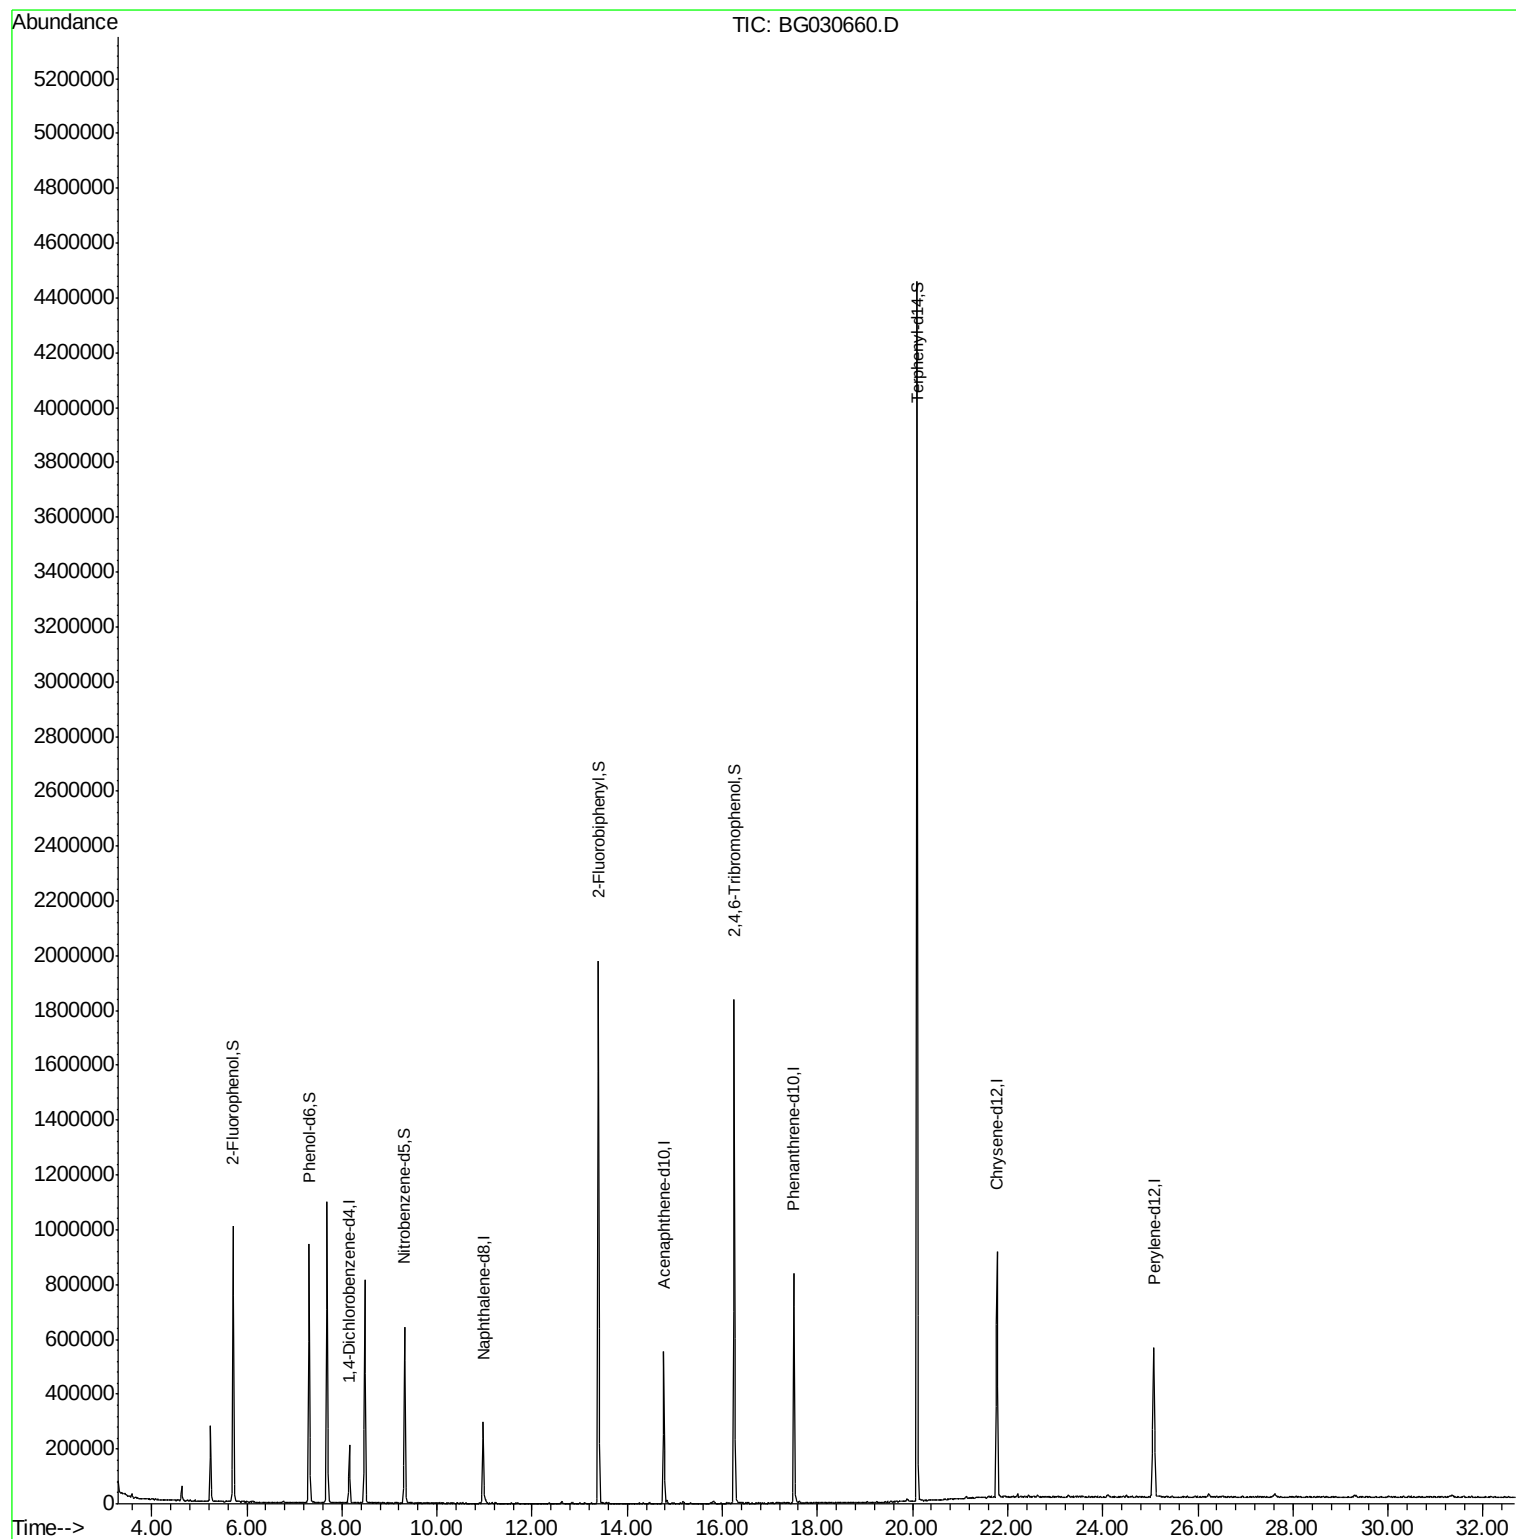

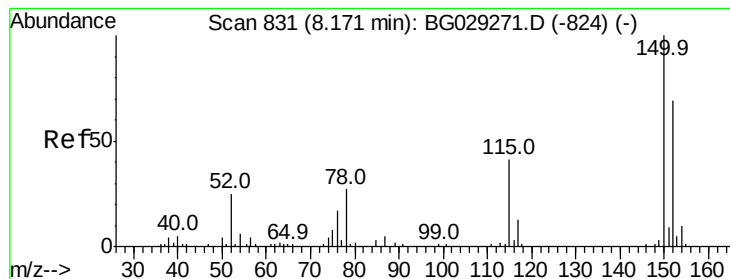


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.15 min Scan# 828
Delta R.T. -0.01 min
Lab File: BG030660.D
Acq: 2 Nov 2017 13:44

Instrument :
BNA_G
ClientSampleId :
COMP-1

Tot Ion:152 Resp: 62727
Ion Ratio Lower Upper
152 100
150 152.7 126.6 189.8
115 58.7 53.0 79.4

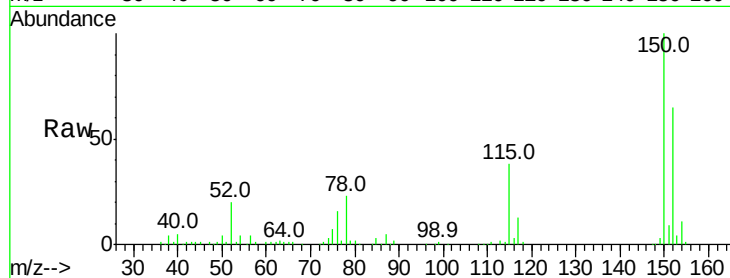


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

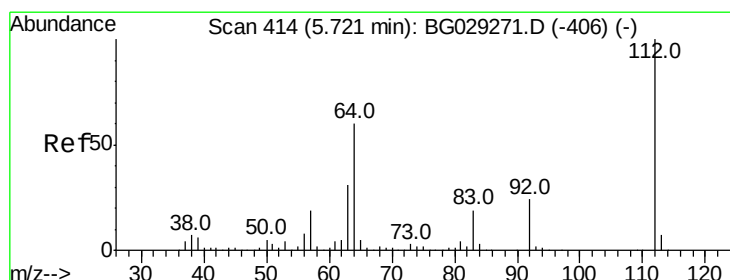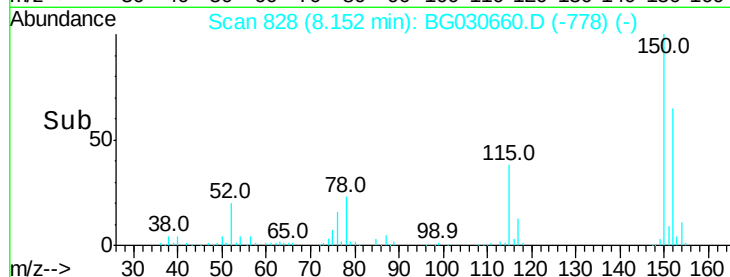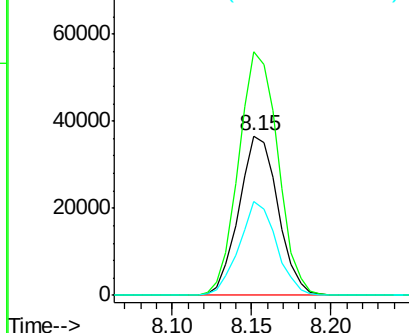



#5


2-Fluorophenol
Concen: 126.404 ng
RT: 5.71 min Scan# 413
Delta R.T. -0.00 min
Lab File: BG030660.D
Acq: 2 Nov 2017 13:44

Tgt Ion:112 Resp: 474629
Ion Ratio Lower Upper
112 100
64 57.5 56.3 84.5
63 29.3 30.1 45.1#

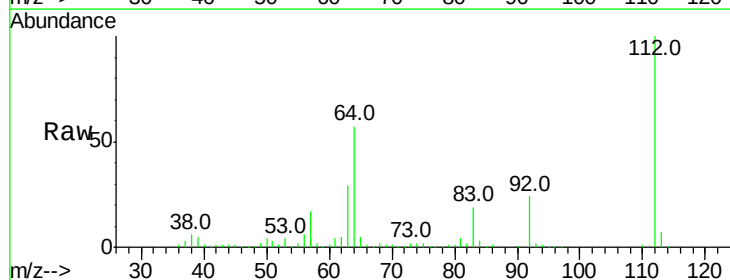

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

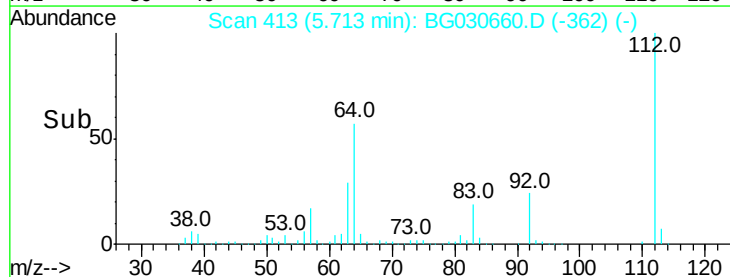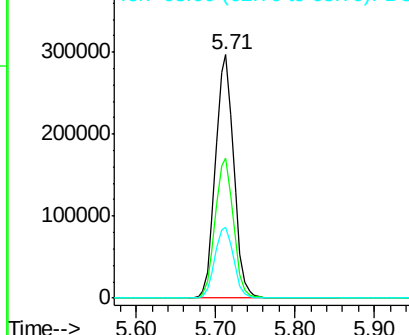

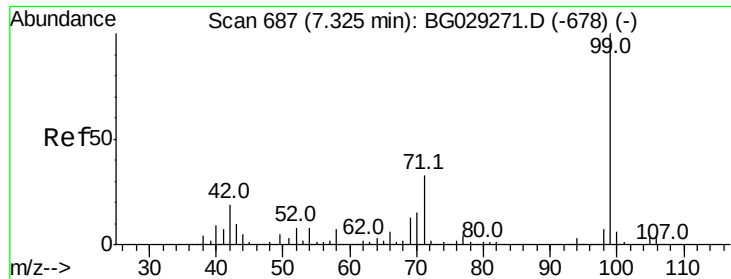

#7

Phenol-d6

Concen: 109.914 ng

RT: 7.31 min Scan# 685

Delta R.T. -0.01 min

Lab File: BG030660.D

Acq: 2 Nov 2017 13:44

Instrument :

BNA_G

ClientSampleId :

COMP-1


Tot Ion: 99 Resp: 579306

Ion Ratio Lower Upper




99 100

42 18.5 14.1 21.1

71 33.3 26.1 39.1

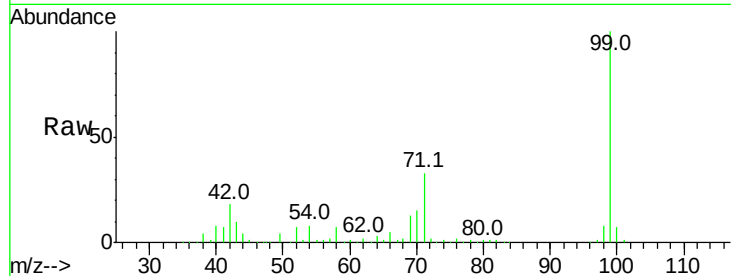

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

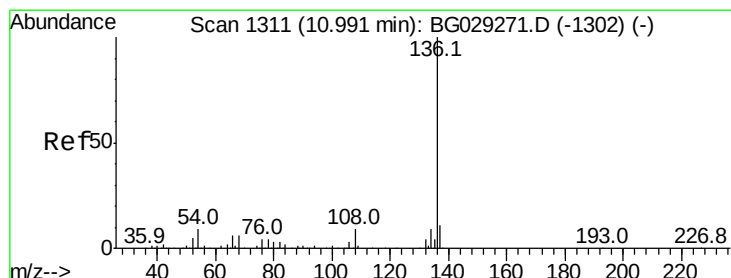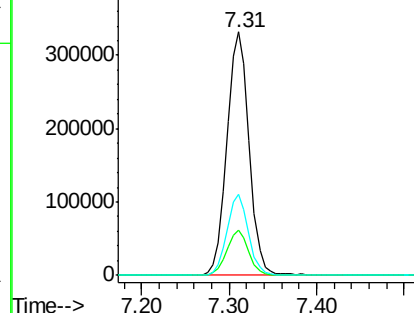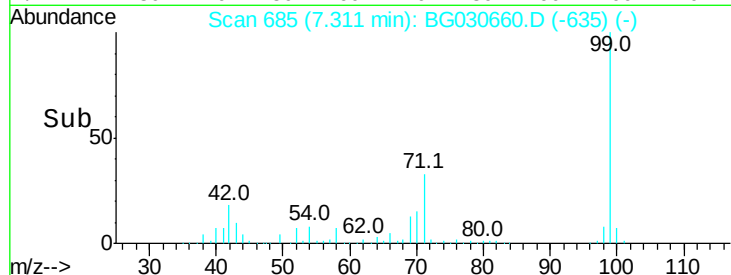

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.97 min Scan# 1307

Delta R.T. -0.01 min

Lab File: BG030660.D

Acq: 2 Nov 2017 13:44

Tgt Ion: 136 Resp: 282903


Ion Ratio Lower Upper

136 100



137 10.5 9.2 13.8


54 7.3 10.3 15.5#

68 5.9 4.5 6.7

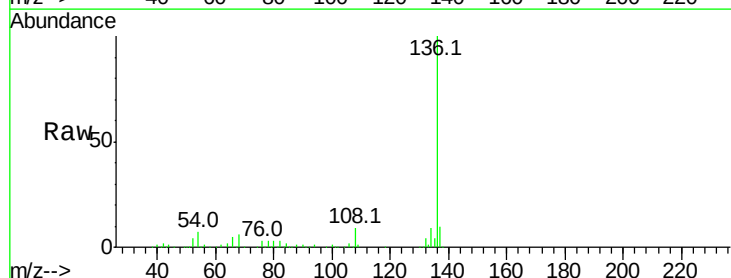

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



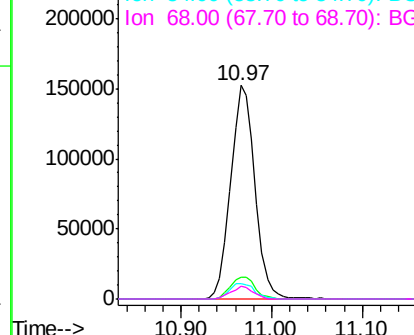
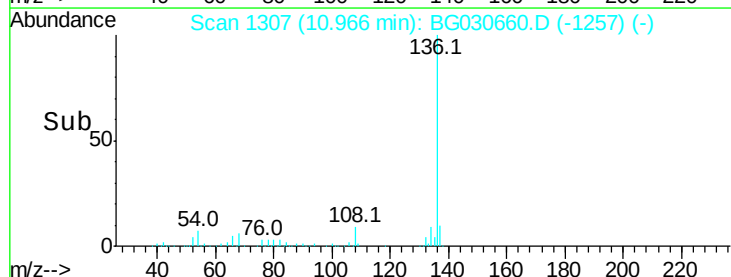


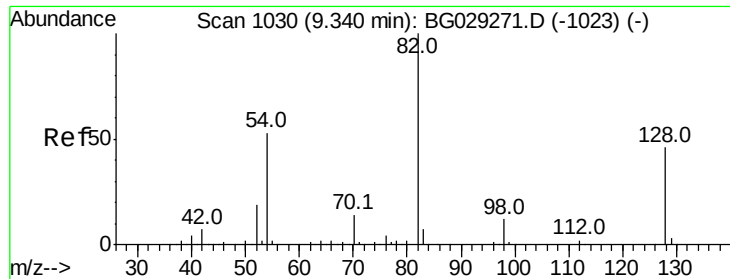

#23
Nitrobenzene-d5
Concen: 88.810 ng
RT: 9.32 min Scan# 1027
Delta R.T. -0.01 min
Lab File: BG030660.D
Acq: 2 Nov 2017 13:44




Instrument :
BNA_G
ClientSampleId :
COMP-1


Tot Ion: 82 Resp: 395370
Ion Ratio Lower Upper
82 100
128 49.5 29.7 44.5#
54 50.8 43.1 64.7

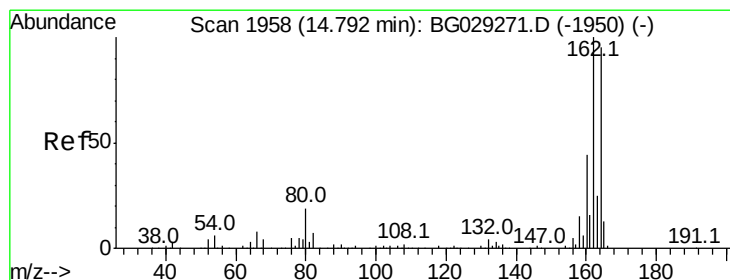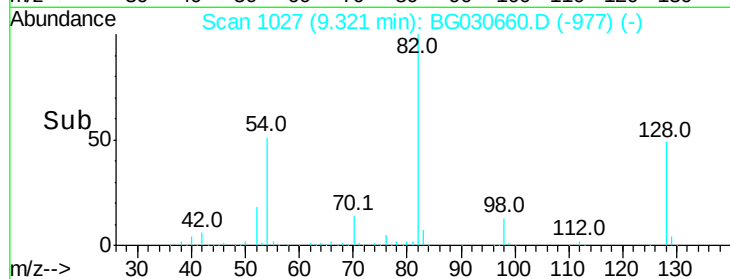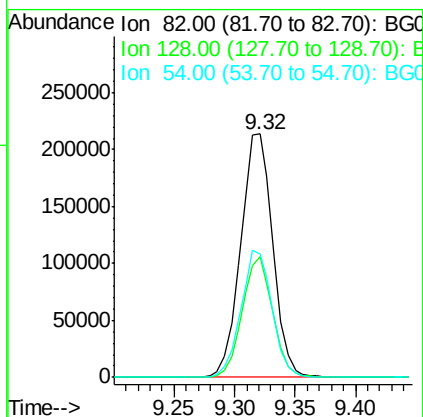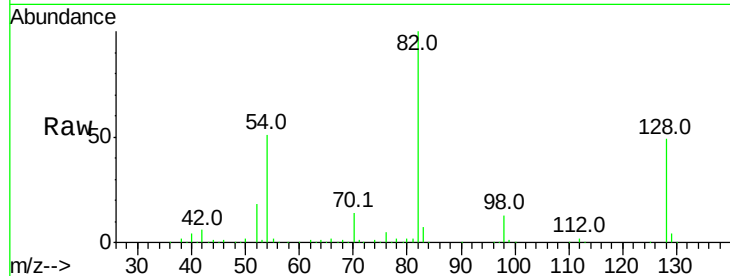

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.77 min Scan# 1954
Delta R.T. -0.01 min
Lab File: BG030660.D
Acq: 2 Nov 2017 13:44

Tgt Ion: 164 Resp: 198945
Ion Ratio Lower Upper
164 100
162 103.8 78.8 118.2
160 45.4 35.4 53.0

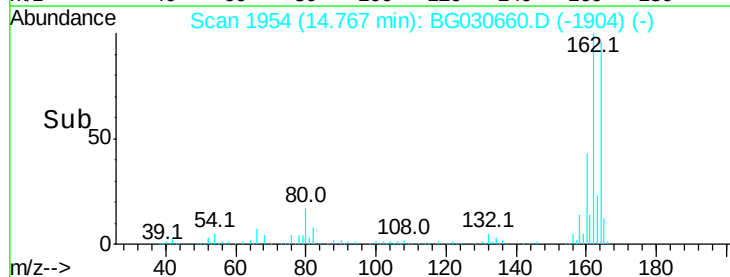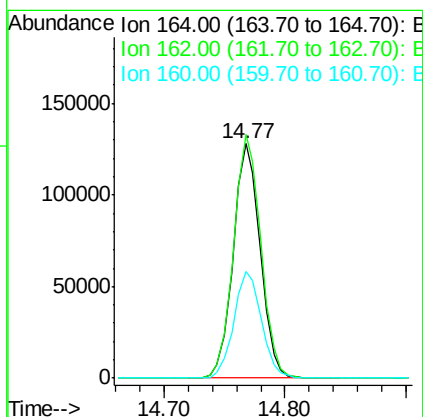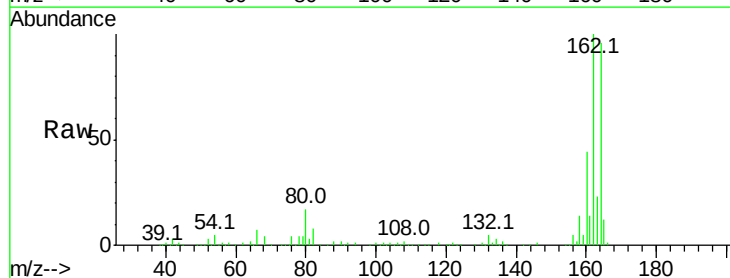


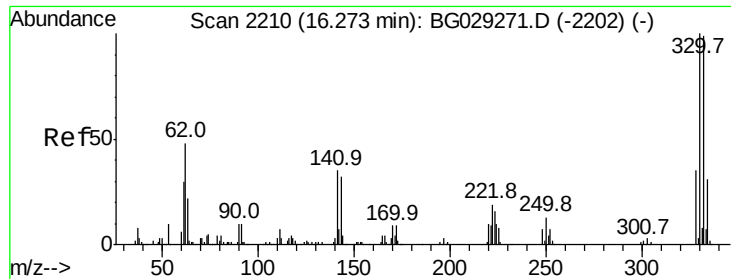




#41
 2,4,6-Tribromophenol
 Concen: 151.502 ng
 RT: 16.25 min Scan# 2207
 Delta R.T. -0.01 min
 Lab File: BG030660.D
 Acq: 2 Nov 2017 13:44

Instrument :
 BNA_G
 ClientSampleId :
 COMP-1

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.3	77.0	115.6
141	32.4	25.2	37.8

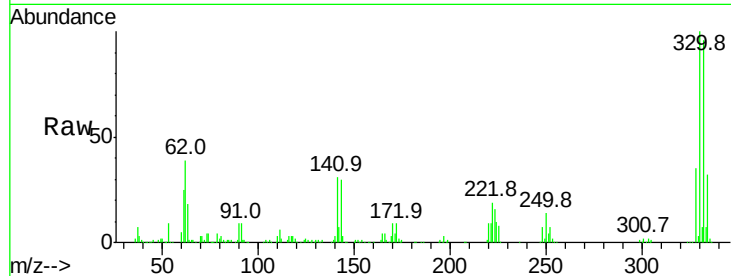


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

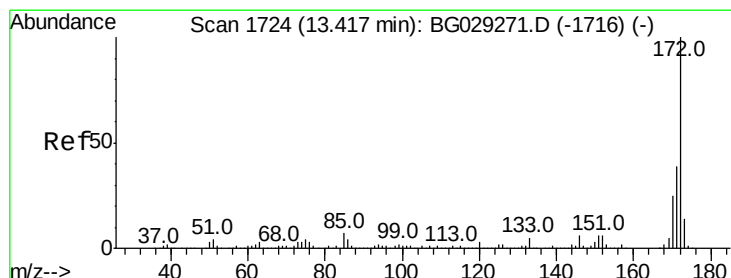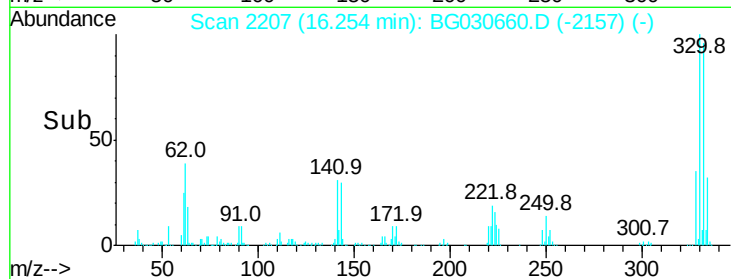
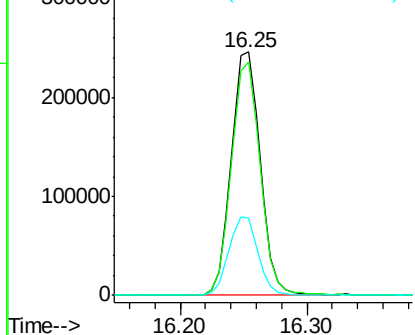



#44
 2-Fluorobiphenyl
 Concen: 81.615 ng
 RT: 13.39 min Scan# 1720
 Delta R.T. -0.01 min
 Lab File: BG030660.D
 Acq: 2 Nov 2017 13:44

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.8	30.0	45.0
170	24.8	19.5	29.3

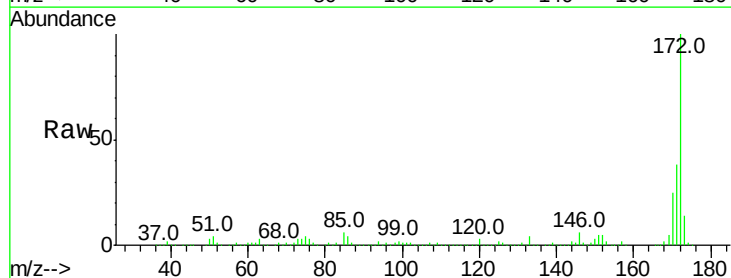

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



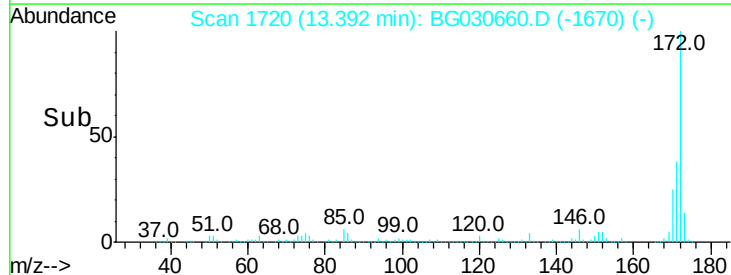
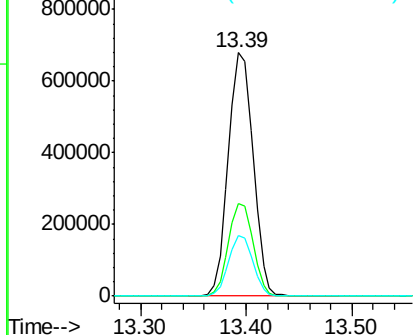


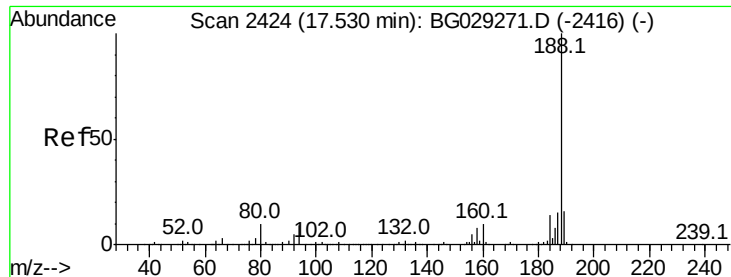

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.51 min Scan# 2420
Delta R.T. -0.01 min
Lab File: BG030660.D
Acq: 2 Nov 2017 13:44




Instrument :
BNA_G
ClientSampleId :
COMP-1


Tot Ion:188 Resp: 509851
Ion Ratio Lower Upper
188 100
94 8.3 6.9 10.3
80 8.8 7.7 11.5

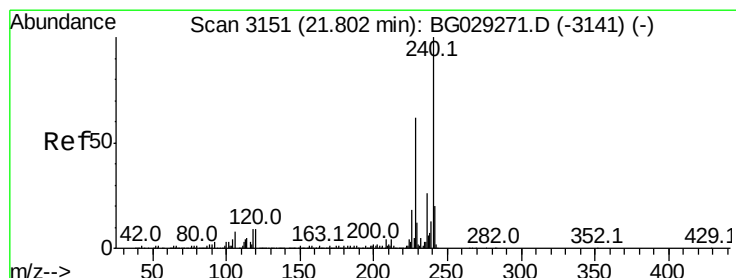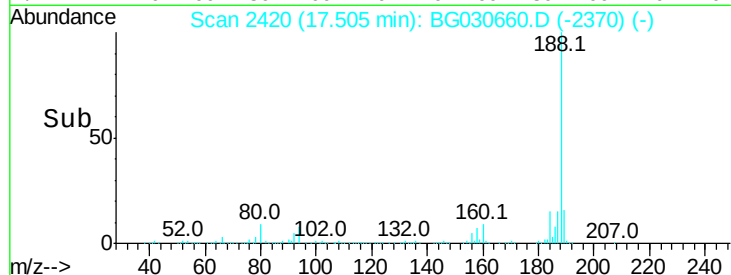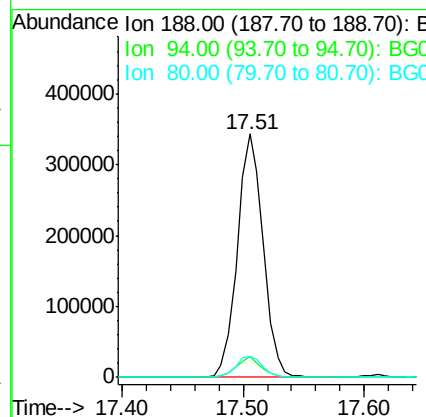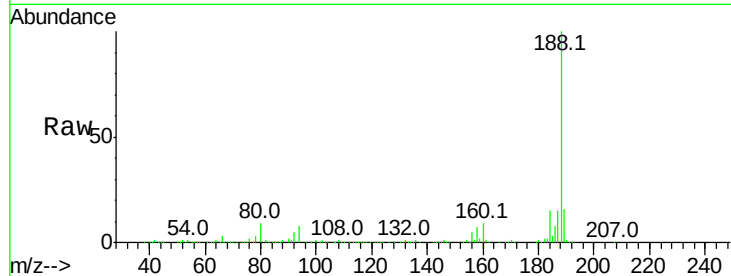

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.78 min Scan# 3147
Delta R.T. -0.01 min
Lab File: BG030660.D
Acq: 2 Nov 2017 13:44

Tgt Ion:240 Resp: 571545
Ion Ratio Lower Upper
240 100
120 8.7 6.8 10.2
236 27.4 20.9 31.3

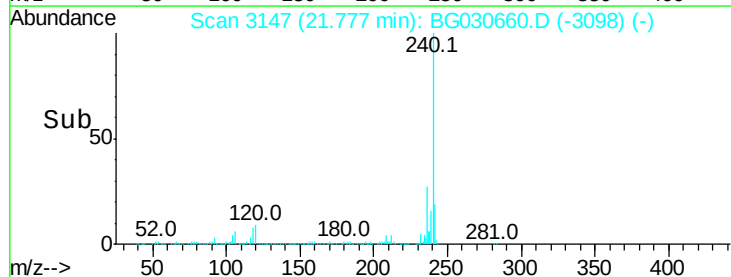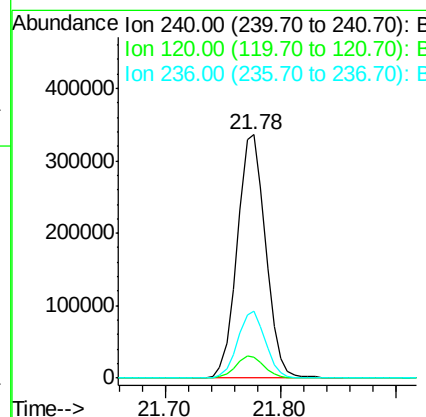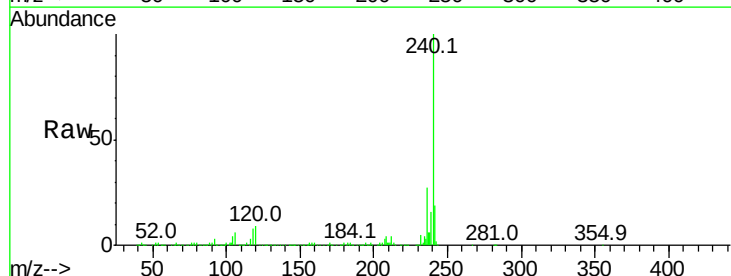

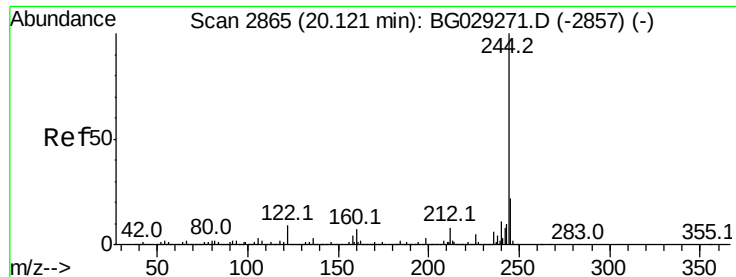

#78

Terphenyl-d14

Concen: 82.627 ng

RT: 20.10 min Scan# 2861

Delta R.T. -0.01 min

Lab File: BG030660.D

Acq: 2 Nov 2017 13:44

Instrument :


BNA_G

ClientSampleId :

COMP-1

Tot Ion:244 Resp: 2075877




Ion	Ratio	Lower	Upper
244	100		
212	8.6	5.8	8.8
122	9.9	7.0	10.4

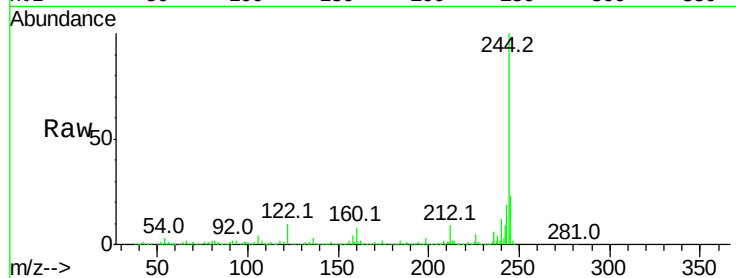

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

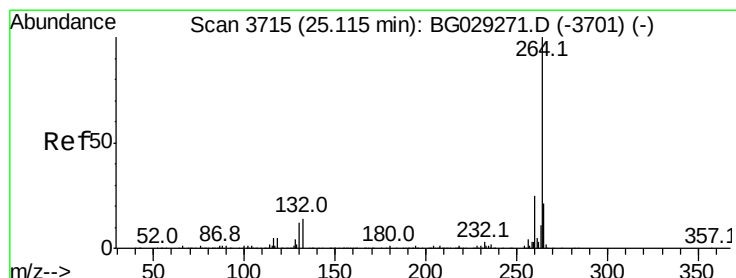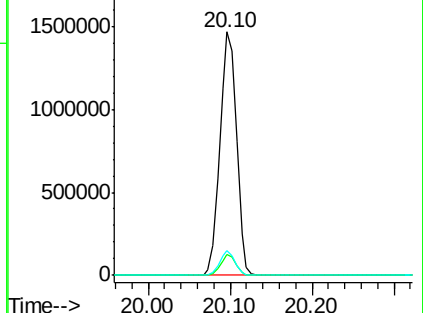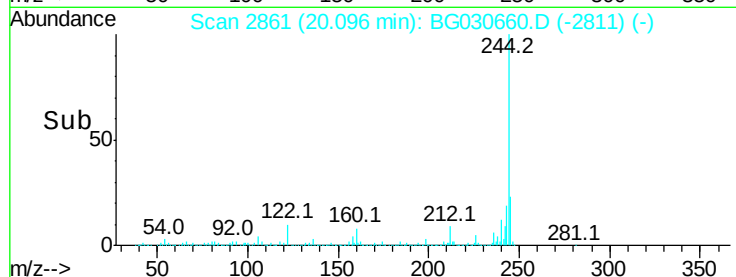

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.07 min Scan# 3708


Delta R.T. -0.02 min

Lab File: BG030660.D

Acq: 2 Nov 2017 13:44

Tgt Ion:264 Resp: 579639

Ion	Ratio	Lower	Upper
264	100		
260	23.4	17.4	26.0
265	22.1	17.7	26.5

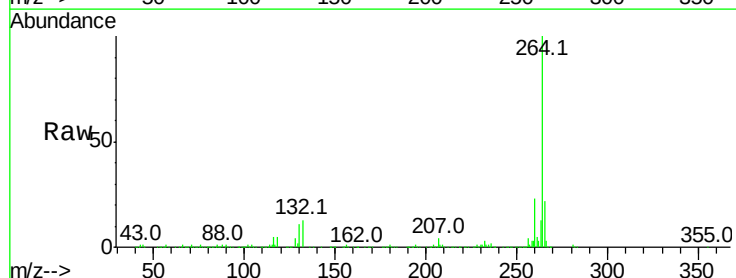

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

