

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110217\
 Data File : BG030679.D
 Acq On : 3 Nov 2017 1:40
 Operator : SJ/JU
 Sample : I6280-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EPE-110-1(35-37)

Quant Time: Nov 03 02:26:07 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 17:41:24 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	63763	20.00	ng	0.00
21) Naphthalene-d8	10.97	136	295221	20.00	ng	0.00
38) Acenaphthene-d10	14.77	164	205676	20.00	ng	0.00
63) Phenanthrene-d10	17.51	188	509739	20.00	ng	0.00
75) Chrysene-d12	21.78	240	575037	20.00	ng	-0.01
86) Perylene-d12	25.08	264	592022	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.71	112	713527	186.94	ng	0.00
7) Phenol-d6	7.31	99	977152	182.39	ng	0.00
23) Nitrobenzene-d5	9.32	82	580182	124.89	ng	0.00
41) 2,4,6-Tribromophenol	16.25	330	562181	211.71	ng	0.00
44) 2-Fluorobiphenyl	13.40	172	1615116	115.17	ng	0.00
78) Terphenyl-d14	20.10	244	2534830	100.28	ng	0.00
Target Compounds						
10) Phenol	7.34	94	19403	3.359	ng	96
49) Dimethylphthalate	14.21	163	128812	8.027	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110217\
Data File : BG030679.D
Acq On : 3 Nov 2017 1:40
Operator : SJ/JU
Sample : I6280-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EPE-110-1(35-37)

Quant Time: Nov 03 02:26:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

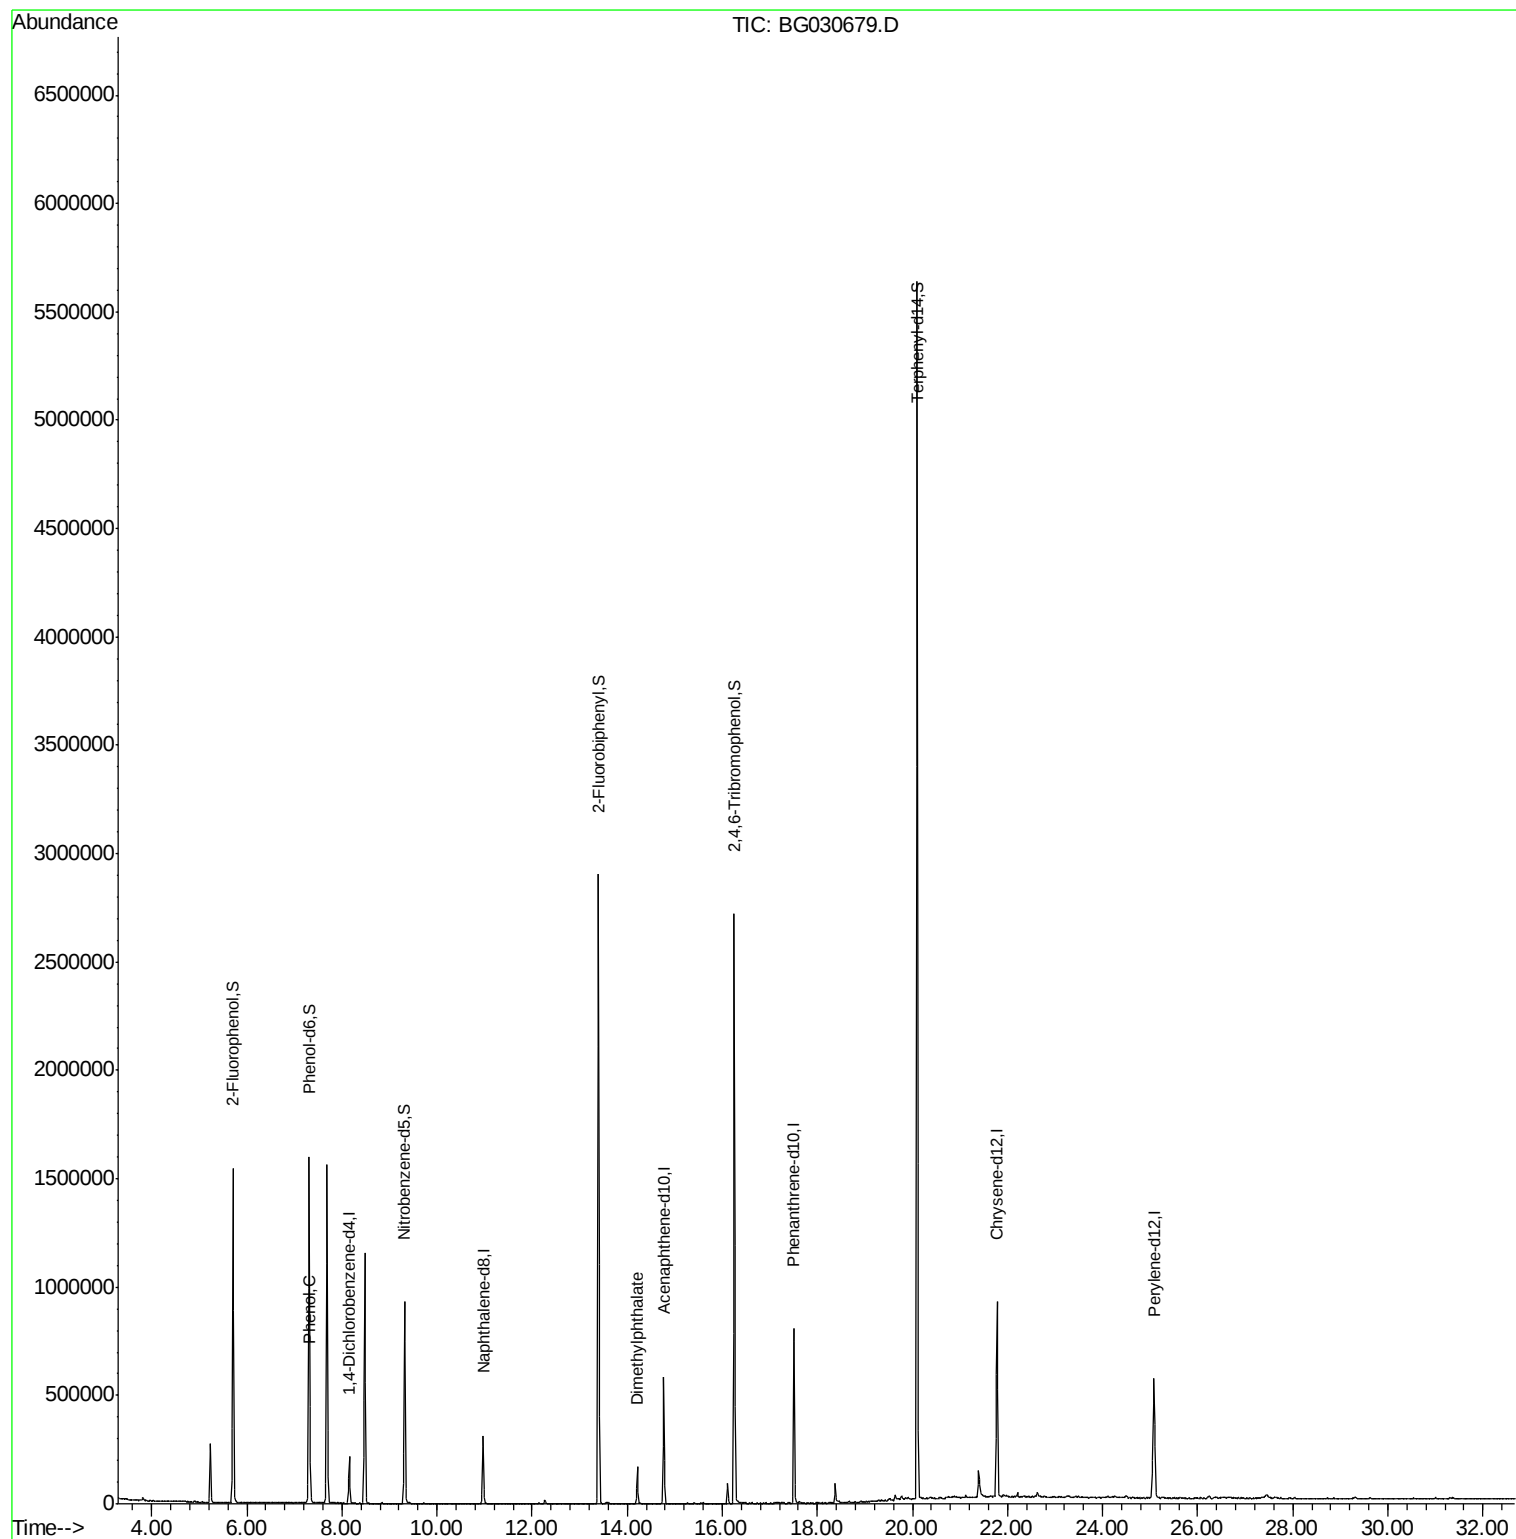

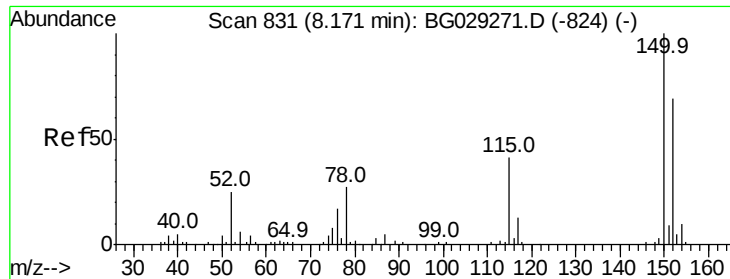


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.15 min Scan# 828
Delta R.T. -0.01 min
Lab File: BG030679.D
Acq: 3 Nov 2017 1:40

Instrument :
BNA_G
ClientSampleId :
EPE-110-1(35-37)

Tot Ion:152 Resp: 63763
Ion Ratio Lower Upper
152 100
150 152.6 126.6 189.8
115 56.3 53.0 79.4

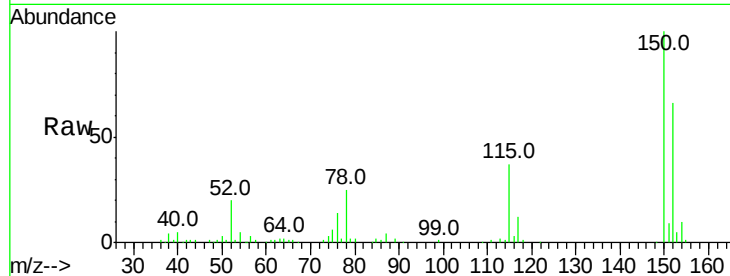


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

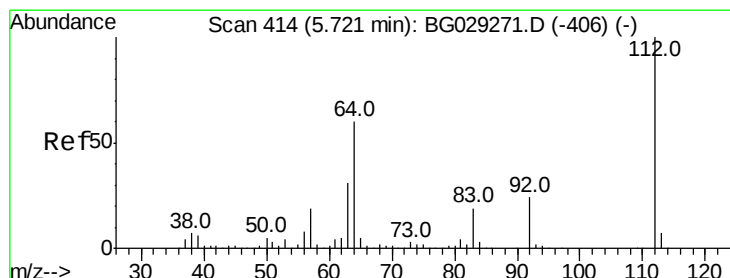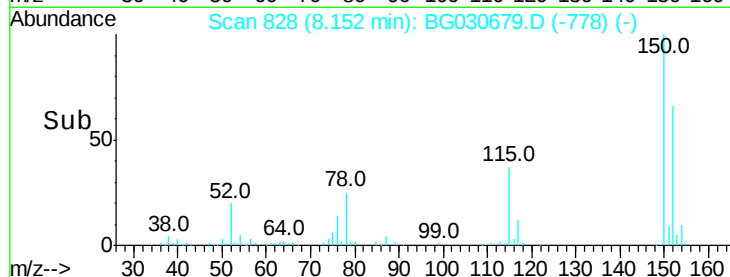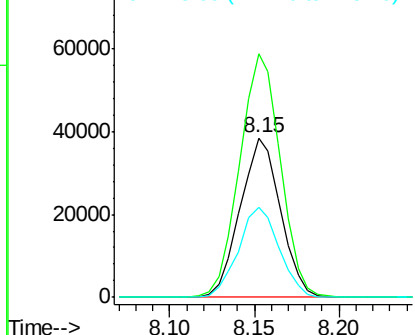



#5


2-Fluorophenol
Concen: 186.940 ng
RT: 5.71 min Scan# 412
Delta R.T. -0.01 min
Lab File: BG030679.D
Acq: 3 Nov 2017 1:40

Tgt Ion:112 Resp: 713527
Ion Ratio Lower Upper
112 100
64 59.2 56.3 84.5
63 30.9 30.1 45.1

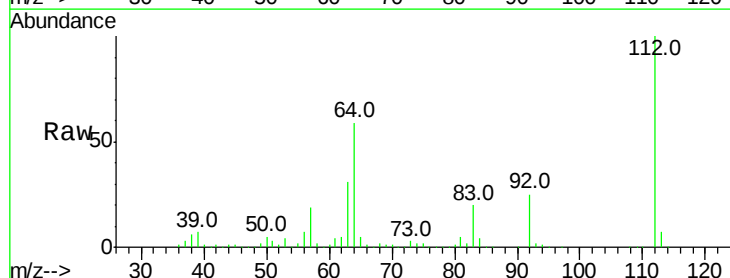

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

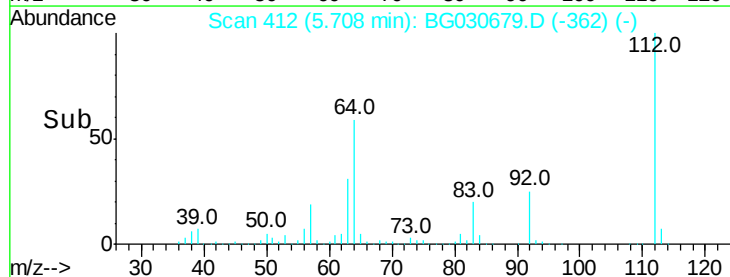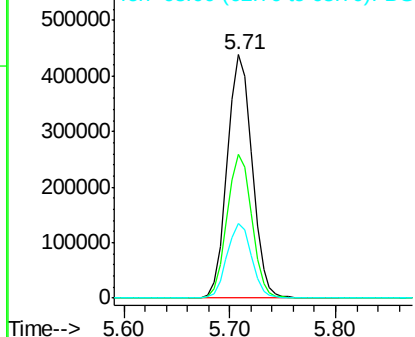

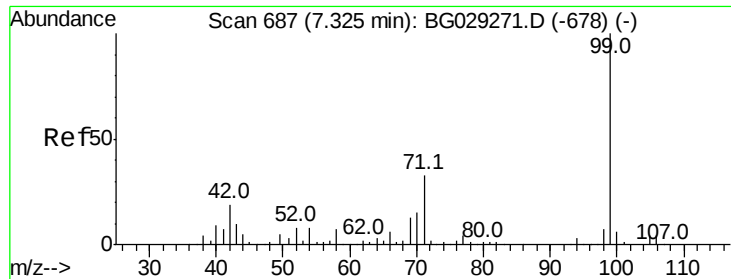

#7

Phenol-d6

Concen: 182.387 ng

RT: 7.31 min Scan# 685

Delta R.T. -0.01 min

Lab File: BG030679.D

Acq: 3 Nov 2017 1:40

Instrument :

BNA_G

ClientSampleId :

EPE-110-1(35-37)


Tot Ion: 99 Resp: 977152

Ion Ratio Lower Upper




99 100

42 18.8 14.1 21.1

71 33.9 26.1 39.1

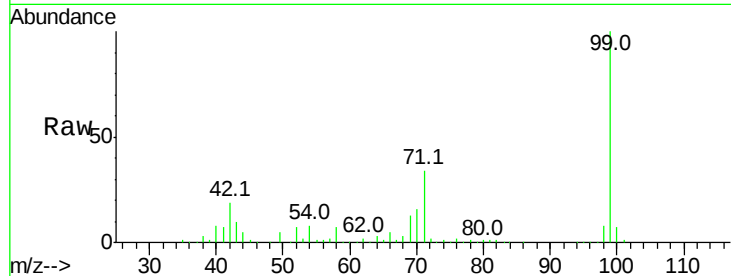

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

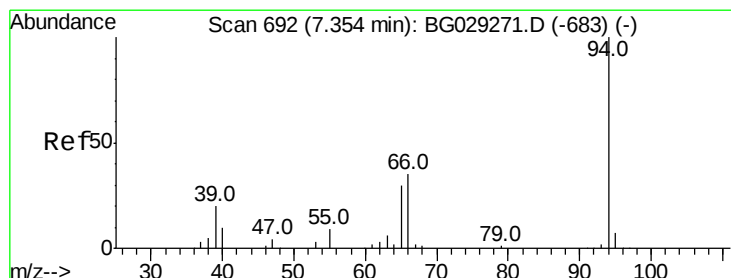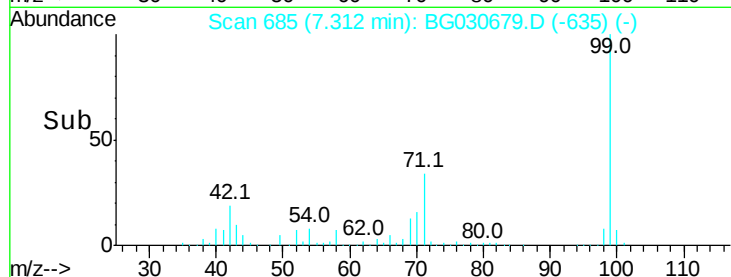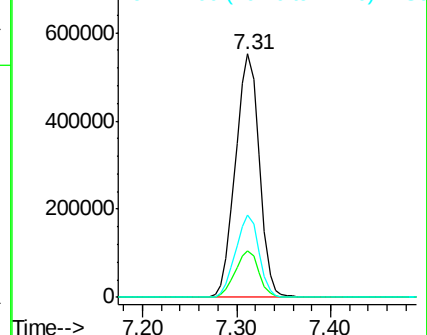

#10

Phenol

Concen: 3.359 ng

RT: 7.34 min Scan# 689

Delta R.T. -0.01 min

Lab File: BG030679.D

Acq: 3 Nov 2017 1:40


Tgt Ion: 94 Resp: 19403

Ion Ratio Lower Upper



94 100


65 31.8 11.9 51.9

66 46.9 22.2 62.2

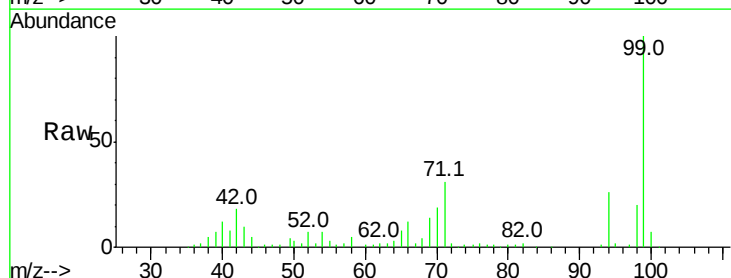

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



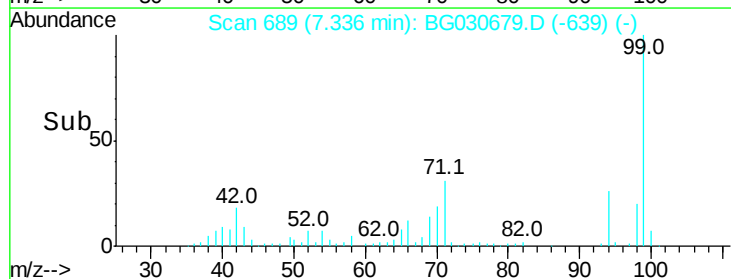
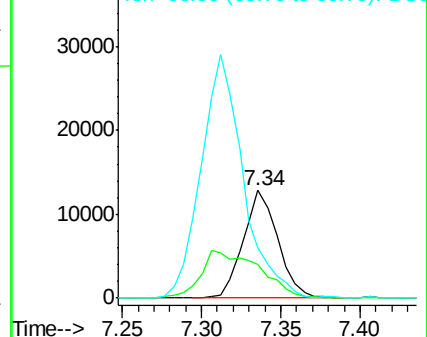


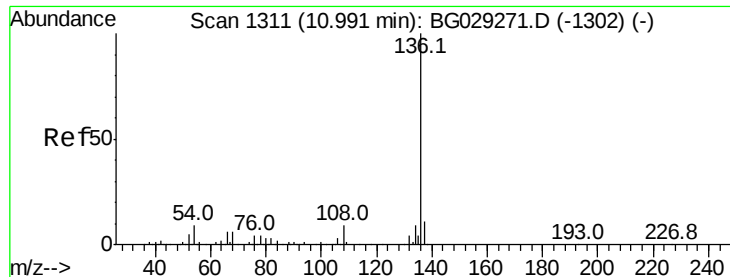

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.97 min Scan# 1307
Delta R.T. -0.01 min
Lab File: BG030679.D
Acq: 3 Nov 2017 1:40




Instrument :
BNA_G
ClientSampleId :
EPE-110-1(35-37)


Tot Ion:	136	Resp:	295221
Ion	Ratio	Lower	Upper
136	100		
137	10.8	9.2	13.8
54	7.8	10.3	15.5#
68	6.2	4.5	6.7

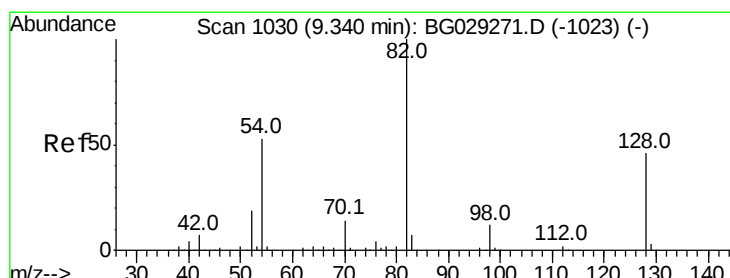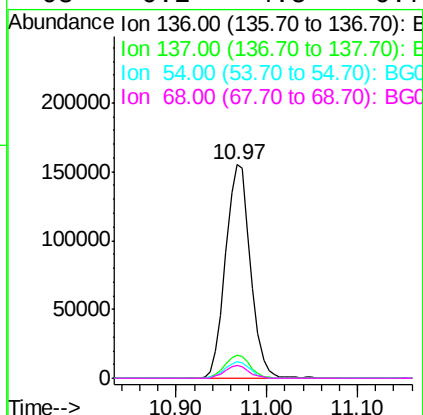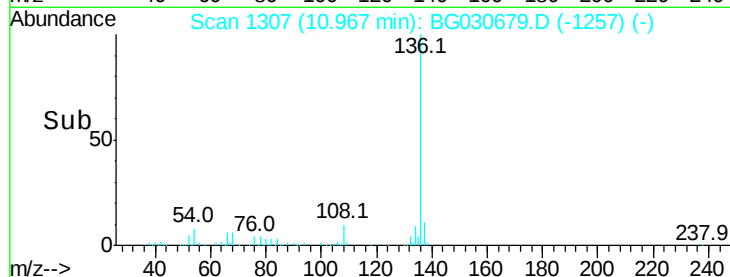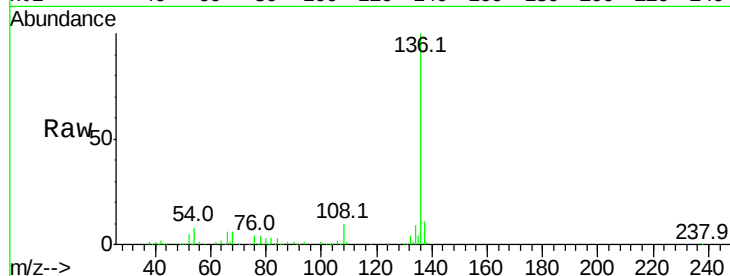

#23
Nitrobenzene-d5
Concen: 124.886 ng
RT: 9.32 min Scan# 1027
Delta R.T. -0.01 min
Lab File: BG030679.D
Acq: 3 Nov 2017 1:40

Tgt Ion:	82	Resp:	580182
Ion	Ratio	Lower	Upper
82	100		
128	46.7	29.7	44.5#
54	50.4	43.1	64.7

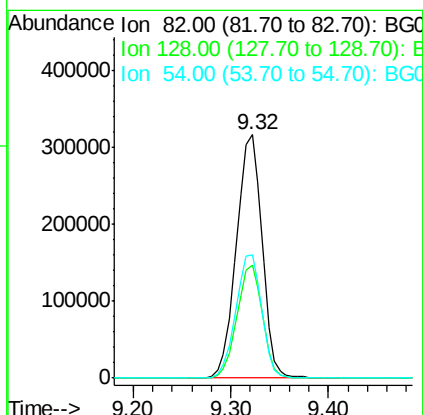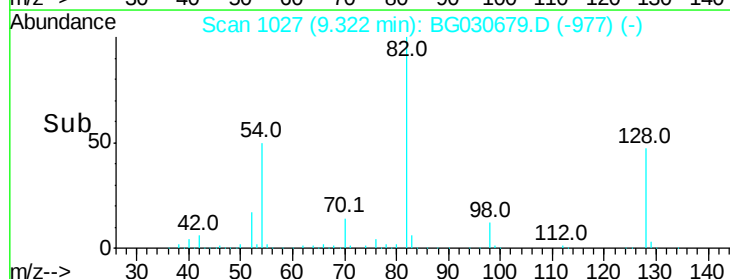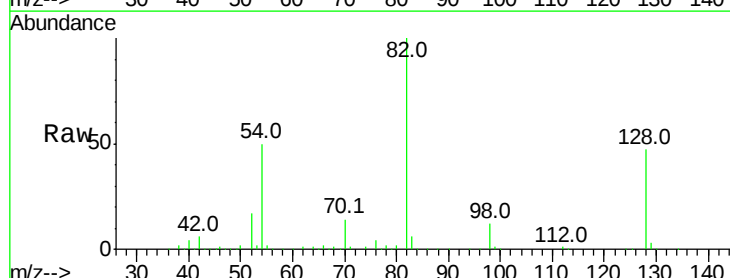

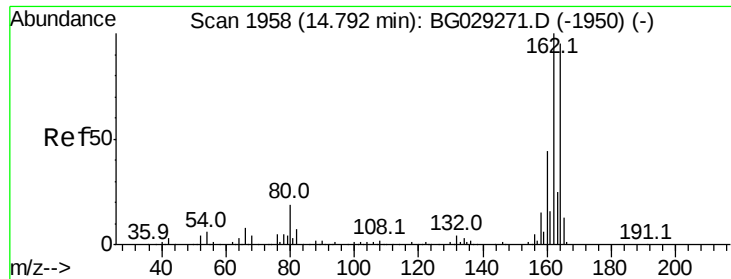

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.77 min Scan# 1954

Delta R.T. -0.01 min

Lab File: BG030679.D

Acq: 3 Nov 2017 1:40

Instrument :

BNA_G

ClientSampleId :

EPE-110-1(35-37)


Tot Ion:164 Resp: 205676

Ion Ratio Lower Upper

164 100

162 104.7 78.8 118.2




160 44.5 35.4 53.0

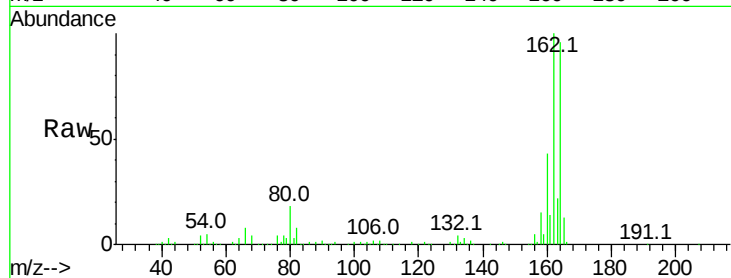

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

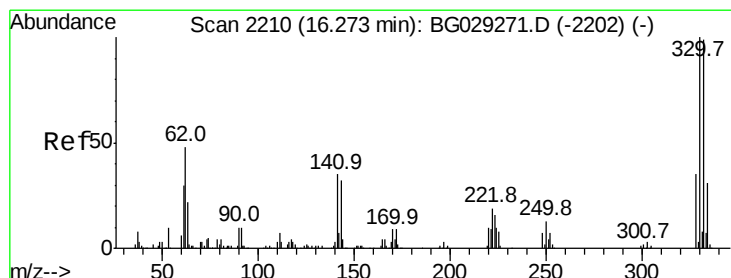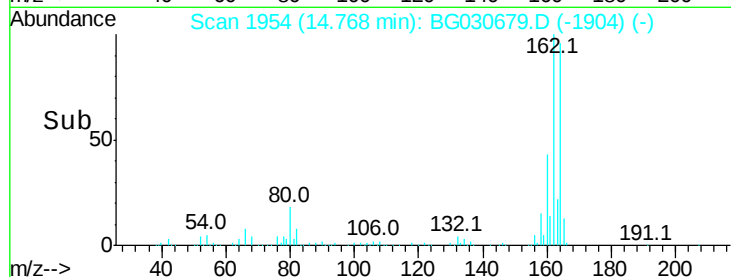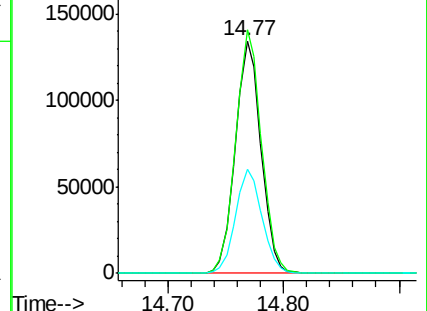

#41

2,4,6-Tribromophenol

Concen: 211.705 ng

RT: 16.25 min Scan# 2207

Delta R.T. -0.01 min

Lab File: BG030679.D

Acq: 3 Nov 2017 1:40


Tgt Ion:330 Resp: 562181

Ion Ratio Lower Upper

330 100

332 95.8 77.0 115.6



141 33.0 25.2 37.8

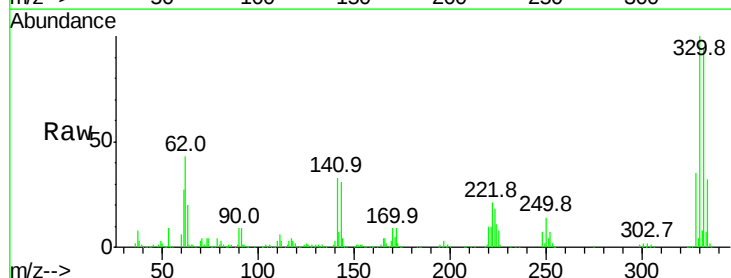


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



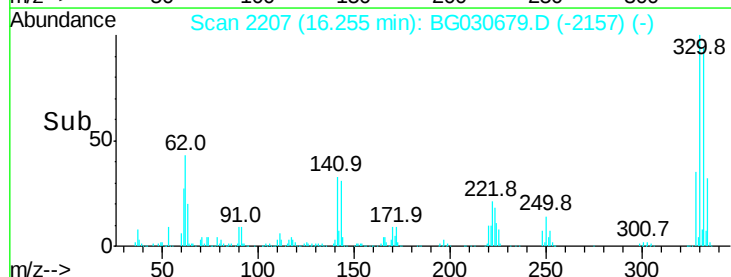
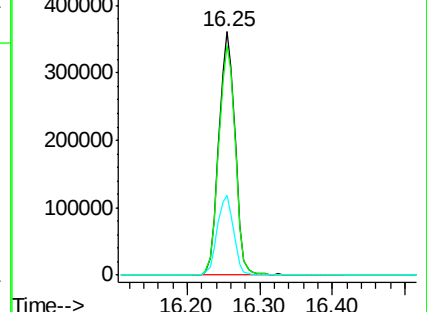


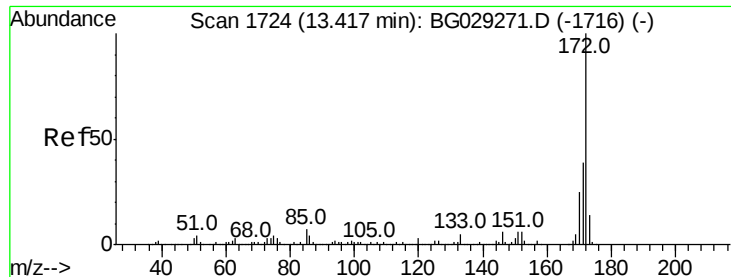

#44
2-Fluorobiphenyl
Concen: 115.172 ng
RT: 13.40 min Scan# 1721
Delta R.T. 0.00 min
Lab File: BG030679.D
Acq: 3 Nov 2017 1:40




Instrument :
BNA_G
ClientSampleId :
EPE-110-1(35-37)


Tot Ion:172 Resp: 1615116
Ion Ratio Lower Upper
172 100
171 38.8 30.0 45.0
170 25.2 19.5 29.3

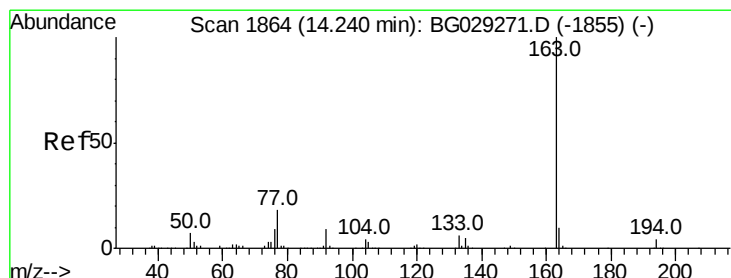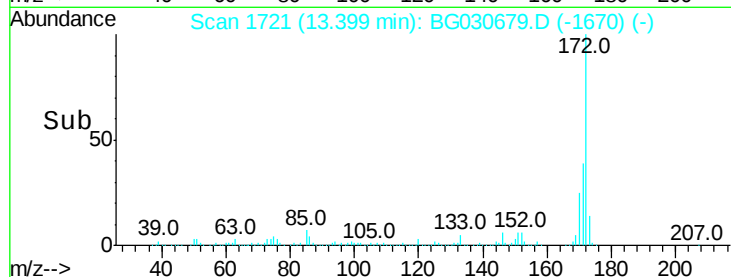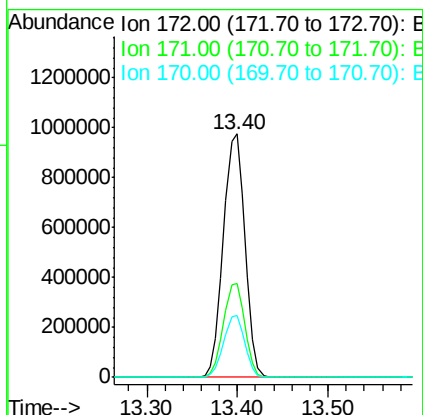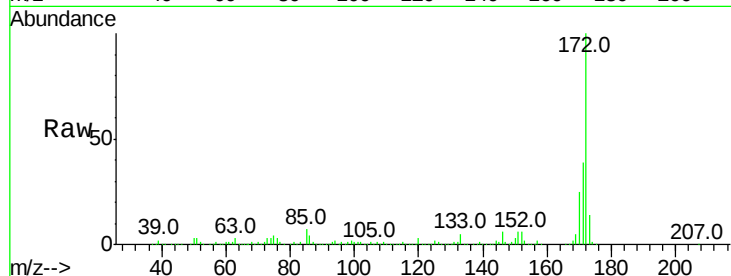

#49
Dimethylphthalate
Concen: 8.027 ng
RT: 14.21 min Scan# 1859
Delta R.T. -0.01 min
Lab File: BG030679.D
Acq: 3 Nov 2017 1:40

Tgt Ion:163 Resp: 128812
Ion Ratio Lower Upper
163 100
194 4.3 3.4 5.2
164 10.3 8.2 12.4

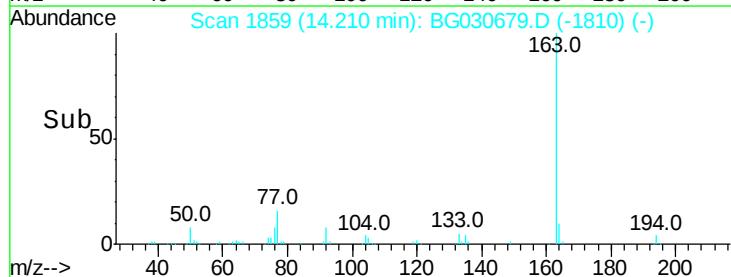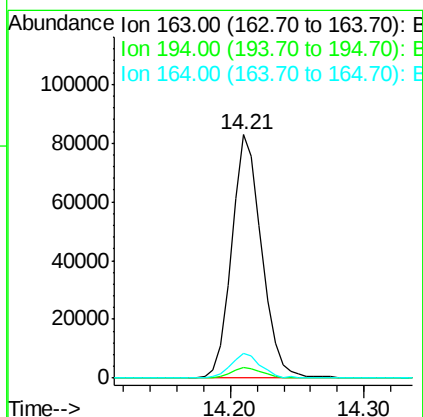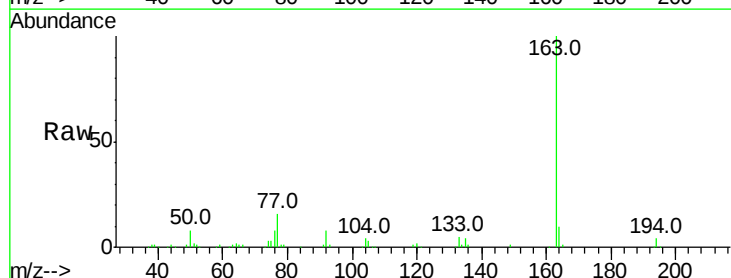

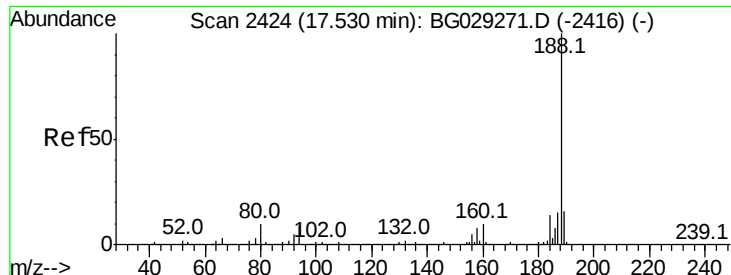

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.51 min Scan# 2420

Delta R.T. -0.01 min

Lab File: BG030679.D

Acq: 3 Nov 2017 1:40

Instrument :

BNA_G

ClientSampleId :

EPE-110-1(35-37)


Tot Ion:188 Resp: 509739

Ion Ratio Lower Upper

188 100

94 8.3 6.9 10.3




80 9.3 7.7 11.5

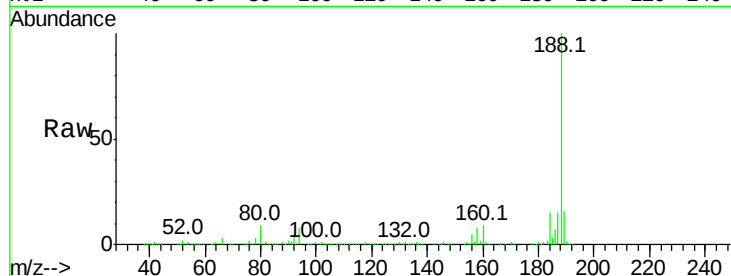

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

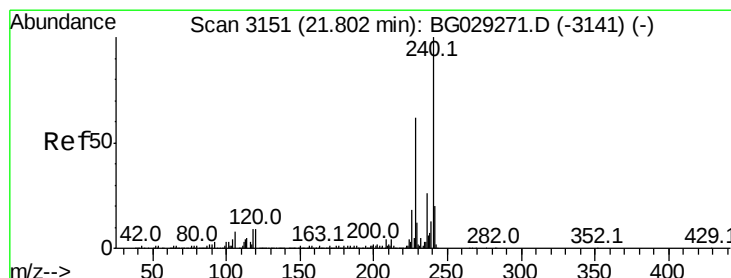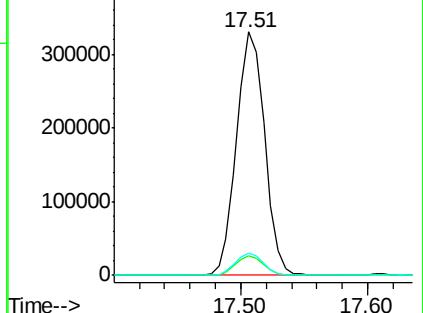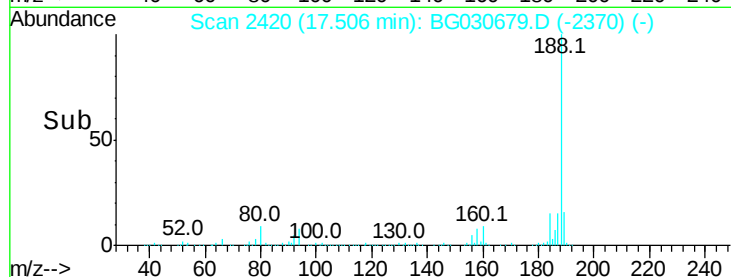

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.78 min Scan# 3147

Delta R.T. -0.01 min

Lab File: BG030679.D

Acq: 3 Nov 2017 1:40


Tgt Ion:240 Resp: 575037

Ion Ratio Lower Upper

240 100

120 8.6 6.8 10.2



236 27.0 20.9 31.3

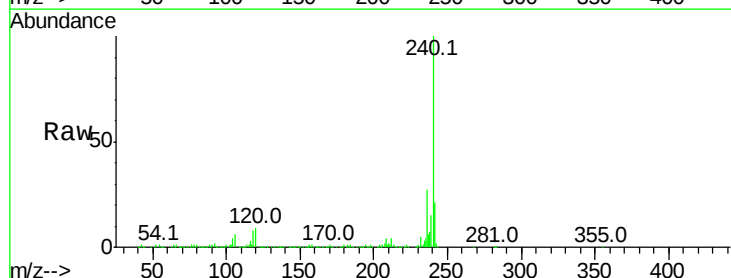


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



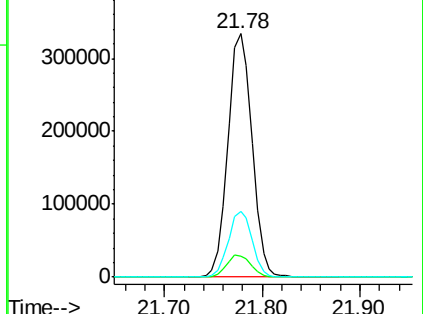
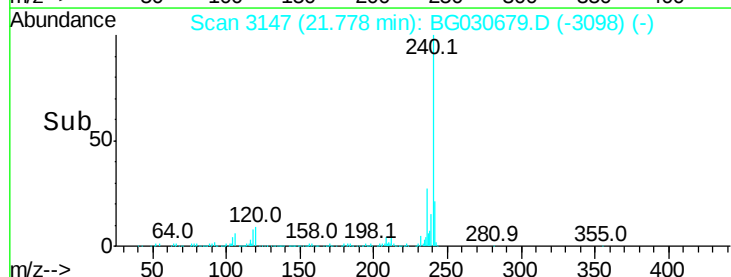


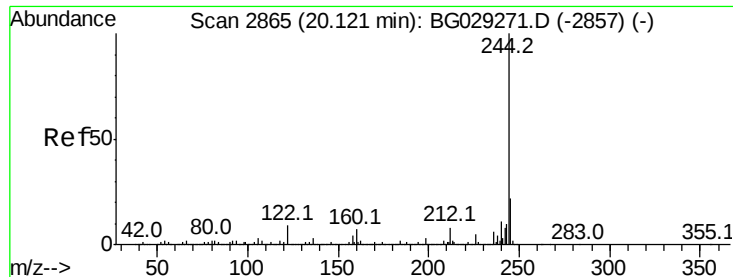

#78
 Terphenyl-d14
 Concen: 100.282 ng
 RT: 20.10 min Scan# 2862
 Delta R.T. 0.00 min
 Lab File: BG030679.D
 Acq: 3 Nov 2017 1:40

Instrument :
 BNA_G
 ClientSampleId :
 EPE-110-1(35-37)

Tot Ion:244 Resp: 2534830
 Ion Ratio Lower Upper
 244 100
 212 9.7 5.8 8.8#
 122 10.4 7.0 10.4

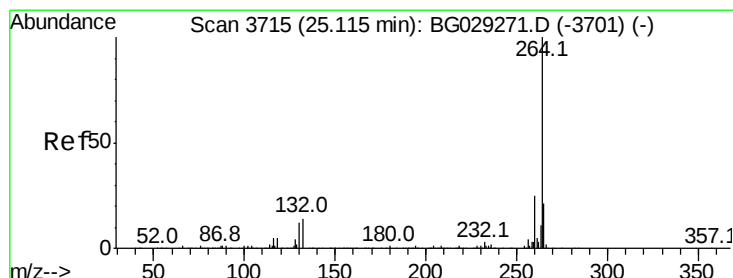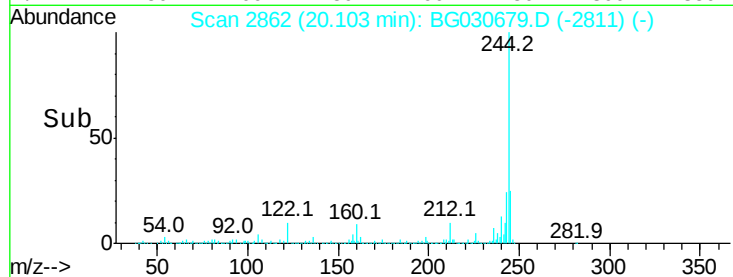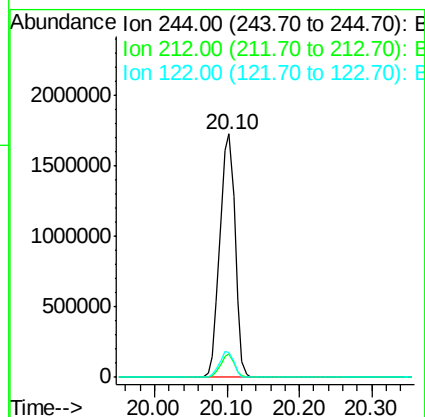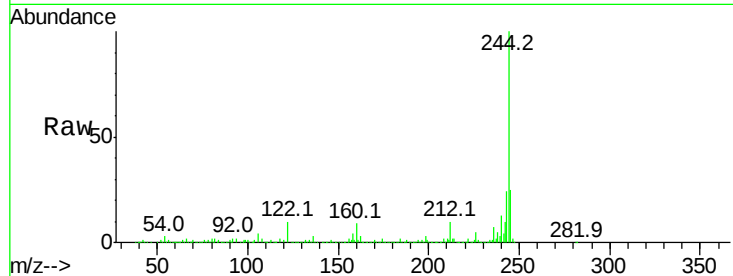

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.08 min Scan# 3709
 Delta R.T. -0.02 min
 Lab File: BG030679.D
 Acq: 3 Nov 2017 1:40

Tgt Ion:264 Resp: 592022
 Ion Ratio Lower Upper
 264 100
 260 24.6 17.4 26.0
 265 21.4 17.7 26.5

