


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110217\
 Data File : BG030663.D
 Acq On : 2 Nov 2017 15:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 01 17:41:24 2017

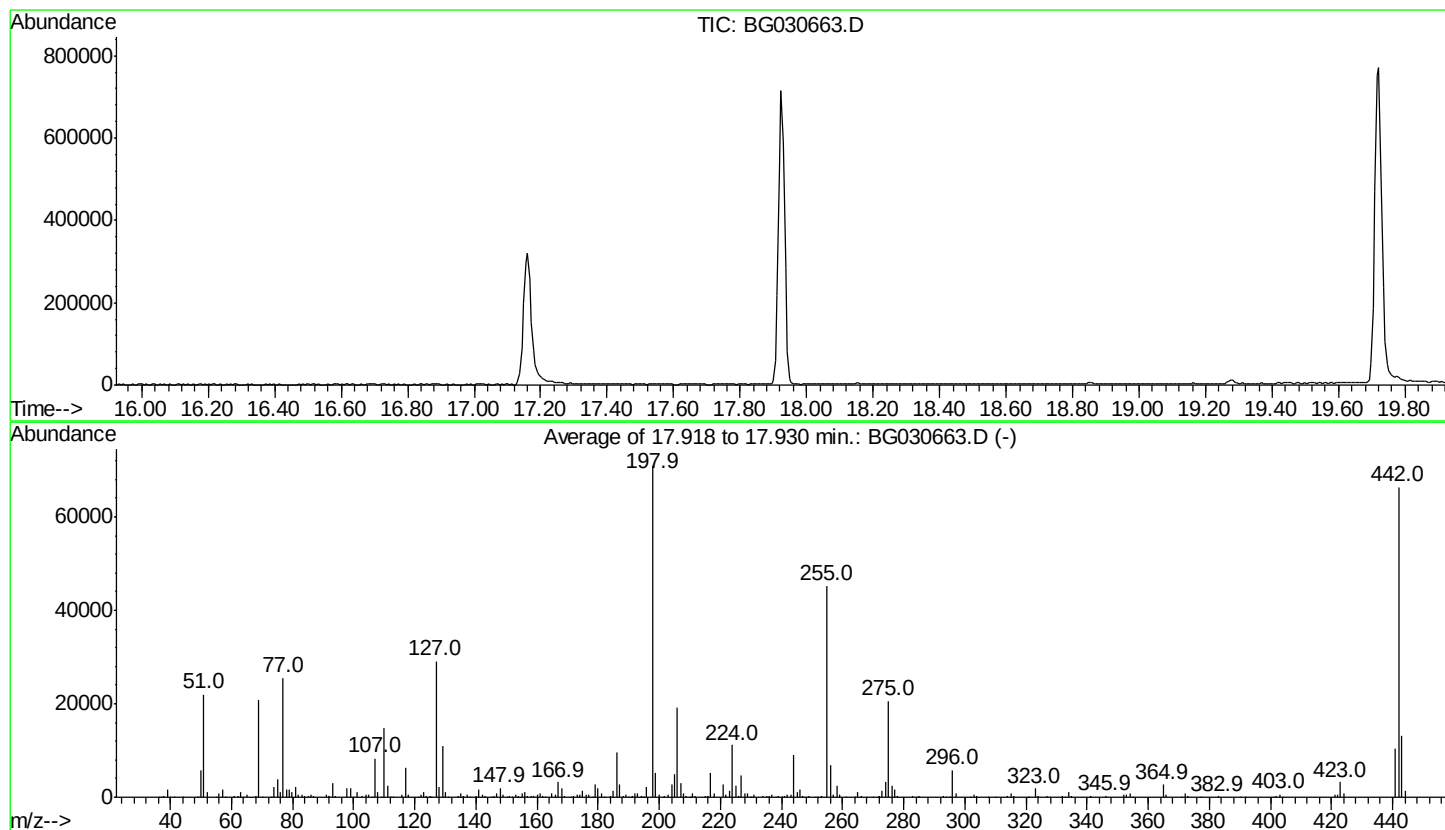

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	21968	PASS
68	69	0.00	2	1.6	345	PASS
69	198	0.00	100	29.5	20917	PASS
70	69	0.00	2	0.6	132	PASS
127	198	10	80	41.0	29085	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70949	PASS
199	198	5	9	7.4	5255	PASS
275	198	10	60	29.1	20656	PASS
365	198	1	100	3.8	2729	PASS
441	442	0.01	24	15.6	10387	PASS
442	198	50	100	93.6	66378	PASS
443	442	15	24	19.7	13059	PASS