


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110217\
 Data File : BG030682.D
 Acq On : 3 Nov 2017 3:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 01 17:41:24 2017

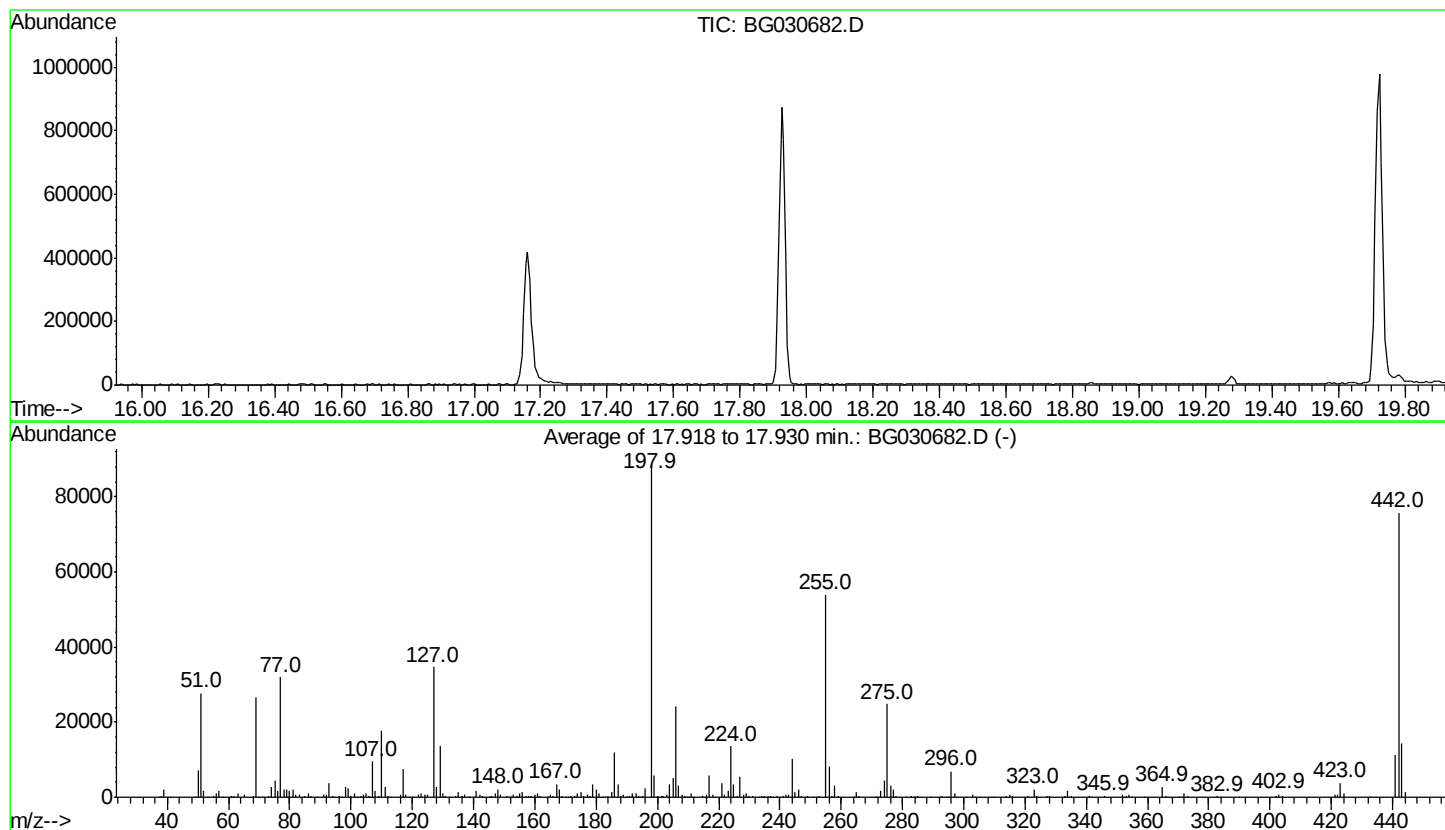

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	27640	PASS
68	69	0.00	2	0.8	208	PASS
69	198	0.00	100	30.1	26581	PASS
70	69	0.00	2	0.5	136	PASS
127	198	10	80	39.2	34624	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88304	PASS
199	198	5	9	6.5	5730	PASS
275	198	10	60	28.1	24800	PASS
365	198	1	100	3.3	2881	PASS
441	442	0.01	24	15.1	11431	PASS
442	198	50	100	85.9	75816	PASS
443	442	15	24	18.8	14268	PASS