

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110221\
 Data File : BG050804.D
 Acq On : 1 Nov 2021 20:08
 Operator : CG/JU
 Sample : SSTD02056
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020407

Quant Time: Nov 02 00:52:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 00:48:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.231	152	42522	20.000	ng/u1	0.00
20) Naphthalene-d8	11.057	136	205062	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.859	164	142624	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.602	188	322086	20.000	ng/u1	0.00
79) Chrysene-d12	21.903	240	255570	20.000	ng/u1	0.00
88) Perylene-d12	25.305	264	216170	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.589	96	7110	6.588	ng/uL	0.00
4) Pyridine-d5	4.018	84	52827	15.457	ng/u1	0.00
7) Phenol-d5	7.379	99	63313	16.023	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.544	67	41293	16.243	ng/u1	0.00
11) 2-Chlorophenol-d4	7.761	132	44232	15.936	ng/u1	0.00
15) 4-Methylphenol-d8	8.930	113	49767	16.312	ng/u1	0.00
21) Nitrobenzene-d5	9.406	128	24255	15.496	ng/u1	0.00
24) 2-Nitrophenol-d4	10.129	143	27396	15.521	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.675	165	45005	14.519	ng/u1	0.00
31) 4-Chloroaniline-d4	11.192	131	67933	14.933	ng/u1	0.00
46) Dimethylphthalate-d6	14.248	166	149052	14.798	ng/u1	0.00
49) Acenaphthylene-d8	14.553	160	184304	14.733	ng/u1	0.00
54) 4-Nitrophenol-d4	15.041	143	25117	13.778	ng/u1	0.00
60) Fluorene-d10	15.846	176	130641	15.092	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.963	200	25199	13.369	ng/u1	0.00
73) Anthracene-d10	17.702	188	206316	14.940	ng/u1	0.00
81) Pyrene-d10	19.976	212	237361	16.297	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.070	264	189078	17.000	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.625	88	9133	6.822	ng/uL	100
5) Pyridine	4.036	79	55773	15.694	ng/u1	100
6) Benzaldehyde	7.367	77	48979	24.842	ng/u1	100
8) Phenol	7.403	94	64789	15.718	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.643	93	49514	15.922	ng/u1	100
12) 2-Chlorophenol	7.796	128	44952	16.113	ng/u1	100
13) 2-Methylphenol	8.666	108	47967	15.717	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.760	45	77495	15.784	ng/u1	100
16) Acetophenone	9.059	105	79115	16.558	ng/u1	100
17) N-Nitroso-di-n-propyla...	9.036	70	48401	16.748	ng/u1	100
18) 4-Methylphenol	8.995	108	51019	15.850	ng/u1	100
19) Hexachloroethane	9.324	117	18874	15.678	ng/u1	100
22) Nitrobenzene	9.447	77	65880	14.482	ng/u1	100
23) Isophorone	9.970	82	128607	14.872	ng/u1	100
25) 2-Nitrophenol	10.164	139	27779	15.103	ng/u1	100
26) 2,4-Dimethylphenol	10.211	107	59423	14.778	ng/u1	100
27) Bis(2-Chloroethoxy)met...	10.446	93	68501	14.610	ng/u1	100
29) 2,4-Dichlorophenol	10.699	162	45213	15.097	ng/u1	100
30) Naphthalene	11.110	128	155370	14.853	ng/u1	100
32) 4-Chloroaniline	11.216	127	66653	14.588	ng/u1	100
33) Hexachlorobutadiene	11.380	225	28447	14.016	ng/u1	100
34) Caprolactam	11.968	113	11383	9.157	ng/u1	100
35) 4-Chloro-3-methylphenol	12.314	107	55185	14.801	ng/u1	100
36) 2-Methylnaphthalene	12.696	142	103465	14.789	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110221\
 Data File : BG050804.D
 Acq On : 1 Nov 2021 20:08
 Operator : CG/JU
 Sample : SSTD02056
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020407

Quant Time: Nov 02 00:52:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 00:48:48 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.914	142	109674	15.520	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	13.061	216	56468	14.252	ng/ul	100
40) Hexachlorocyclopentadiene	13.031	237	23975	11.258	ng/ul	100
41) 2,4,6-Trichlorophenol	13.296	196	37968	14.558	ng/ul	100
42) 2,4,5-Trichlorophenol	13.372	196	40368	14.666	ng/ul	100
43) 1,1'-Biphenyl	13.695	154	144574	14.630	ng/ul	100
44) 2-Chloronaphthalene	13.742	162	109957	14.368	ng/ul	100
45) 2-Nitroaniline	13.942	65	43699	14.317	ng/ul	100
47) Dimethylphthalate	14.294	163	148092	14.642	ng/ul	100
48) 2,6-Dinitrotoluene	14.430	165	30650	14.706	ng/ul	100
50) Acenaphthylene	14.582	152	185857	14.533	ng/ul	100
51) 3-Nitroaniline	14.759	138	34054	16.908	ng/ul	100
52) Acenaphthene	14.923	153	120067	14.371	ng/ul	100
53) 2,4-Dinitrophenol	14.970	184	14791	12.724	ng/ul	100
55) 4-Nitrophenol	15.058	109	24222	13.818	ng/ul	100
56) Dibenzofuran	15.252	168	174091	14.737	ng/ul	100
57) 2,4-Dinitrotoluene	15.211	165	44709	14.951	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.475	232	31993	14.912	ng/ul	100
59) Diethylphthalate	15.652	149	159169	14.731	ng/ul	100
61) Fluorene	15.899	166	138727	14.795	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.887	204	72193	14.598	ng/ul	100
63) 4-Nitroaniline	15.916	138	35041	18.586	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.975	198	24758	13.598	ng/ul	100
67) N-Nitrosodiphenylamine	16.098	169	122515	14.315	ng/ul	100
68) 4-Bromophenyl-phenylether	16.780	248	42988	14.166	ng/ul	100
69) Hexachlorobenzene	16.903	284	44557	14.377	ng/ul	100
70) Atrazine	17.038	200	52411	14.305	ng/ul	100
71) Pentachlorophenol	17.250	266	16317	10.331	ng/ul	100
72) Phenanthrene	17.644	178	232601	14.446	ng/ul	100
74) Anthracene	17.738	178	237302	14.775	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.666	216	59731	13.870	ng/uL	100
76) Pentachlorobenzene	15.170	250	55922	14.060	ng/uL	100
77) Carbazole	18.002	167	217669	14.595	ng/ul	100
78) Di-n-butylphthalate	18.537	149	280955	14.916	ng/ul	100
80) Fluoranthene	19.641	202	281565	15.169	ng/ul	100
82) Pyrene	20.005	202	279007	15.371	ng/ul	100
83) Butylbenzylphthalate	20.869	149	114416	14.869	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.786	252	92108	16.248	ng/ul	100
85) Benzo(a)anthracene	21.880	228	248653	15.341	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.750	149	163644	14.944	ng/ul	100
87) Chrysene	21.950	228	235238	15.243	ng/ul	100
89) Di-n-octyl phthalate	23.020	149	277653	17.642	ng/ul	100
90) Benzo(b)fluoranthene	24.212	252	240325	17.418	ng/ul	100
91) Benzo(k)fluoranthene	24.289	252	229061	17.813	ng/ul	100
93) Benzo(a)pyrene	25.146	252	233125	17.627	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	29.218	276	260207	17.805	ng/ul	100
95) Dibenzo(a,h)anthracene	29.283	278	220203	17.519	ng/ul	100
96) Benzo(g,h,i)perylene	30.446	276	216498	17.733	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110221\
 Data File : BG050804.D
 Acq On : 1 Nov 2021 20:08
 Operator : CG/JU
 Sample : SSTD02056
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020407

Quant Time: Nov 02 00:52:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 00:48:48 2021
 Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 6.822 ng/uL
RT: 3.625 min Scan# 21
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion	Ratio	Lower	Upper
88	100		
43	34.0	27.2	40.8
58	72.7	58.2	87.2



#5
Pyridine
Concen: 15.694 ng/uL
RT: 4.036 min Scan# 93
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion	Ratio	Lower	Upper
79	100		
52	81.4	65.1	97.7
51	37.0	29.6	44.4









#6
Benzaldehyde
Concen: 24.842 ng/ul
RT: 7.367 min Scan# 660
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion: 77 Resp: 48979
Ion Ratio Lower Upper
77 100
105 87.2 69.8 104.6
106 83.9 67.1 100.7



#8
Phenol
Concen: 15.718 ng/ul
RT: 7.403 min Scan# 666
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion: 94 Resp: 64789
Ion Ratio Lower Upper
94 100
65 32.8 26.2 39.4
66 40.3 32.2 48.4









#10
Bis(2-Chloroethyl)ether
Concen: 15.922 ng/ul
RT: 7.643 min Scan# 707
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:	93	Resp:	49514
Ion	Ratio	Lower	Upper
93	100		
63	85.3	68.2	102.4
95	34.6	27.7	41.5



#12
2-Chlorophenol
Concen: 16.113 ng/ul
RT: 7.796 min Scan# 733
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:	128	Resp:	44952
Ion	Ratio	Lower	Upper
128	100		
64	59.0	47.2	70.8
130	32.1	25.7	38.5









#13
2-Methylphenol
Concen: 15.717 ng/ul
RT: 8.666 min Scan# 881
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:108 Resp: 47967
Ion Ratio Lower Upper
108 100
107 90.2 72.2 108.2



#14
2,2'-oxybis(1-Chloropropane)
Concen: 15.784 ng/ul
RT: 8.760 min Scan# 897
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion: 45 Resp: 77495
Ion Ratio Lower Upper
45 100
77 15.1 12.1 18.1
79 10.6 8.5 12.7









#16
Acetophenone
Concen: 16.558 ng/ul
RT: 9.059 min Scan# 948
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:105 Resp: 79115
Ion Ratio Lower Upper
105 100
77 84.2 67.4 101.0
51 28.5 22.8 34.2



#17
N-Nitroso-di-n-propylamine
Concen: 16.748 ng/ul
RT: 9.036 min Scan# 944
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion: 70 Resp: 48401
Ion Ratio Lower Upper
70 100
42 59.5 47.6 71.4
101 7.6 6.1 9.1
130 15.2 12.2 18.2









#18
4-Methylphenol
Concen: 15.850 ng/ul
RT: 8.995 min Scan# 910
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:108 Resp: 51019
Ion Ratio Lower Upper
108 100
107 122.2 97.8 146.6



#19
Hexachloroethane
Concen: 15.678 ng/ul
RT: 9.324 min Scan# 993
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:117 Resp: 18874
Ion Ratio Lower Upper
117 100
201 107.7 86.2 129.2
199 64.8 51.8 77.8



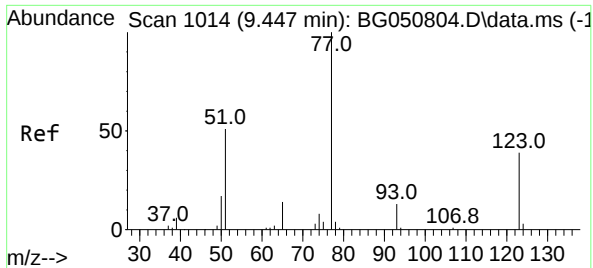

#22

Nitrobenzene

Concen: 14.482 ng/ul

RT: 9.447 min Scan# 1103

Delta R.T. 0.000 min

Lab File: BG050804.D

Acq: 1 Nov 2021 20:08

Instrument :

BNA_G

ClientSampleId :

SSTD020407





Tgt Ion: 77 Resp: 65880

Ion Ratio Lower Upper

77 100

123 38.8 31.0 46.6

65 13.5 10.8 16.2



#23

Isophorone

Concen: 14.872 ng/ul

RT: 9.970 min Scan# 1103

Delta R.T. 0.000 min

Lab File: BG050804.D

Acq: 1 Nov 2021 20:08




Tgt Ion: 82 Resp: 128607


Ion Ratio Lower Upper

82 100

95 6.9 5.5 8.3

138 15.5 12.4 18.6









#25
2-Nitrophenol
Concen: 15.103 ng/ul
RT: 10.164 min Scan# 1136
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:139 Resp: 27779
Ion Ratio Lower Upper
139 100
65 58.4 46.7 70.1
109 36.3 29.0 43.6



#26
2,4-Dimethylphenol
Concen: 14.778 ng/ul
RT: 10.211 min Scan# 1144
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:107 Resp: 59423
Ion Ratio Lower Upper
107 100
121 48.9 39.1 58.7
122 80.4 64.3 96.5





#27

Bis(2-Chloroethoxy)methane

Concen: 14.610 ng/ul

RT: 10.446 min Scan# 1184

Delta R.T. 0.000 min

Lab File: BG050804.D

Acq: 1 Nov 2021 20:08

Instrument :

BNA_G

ClientSampleId :

SSTD020407





Tgt Ion: 93 Resp: 68501

Ion Ratio Lower Upper

93 100

95 33.5 26.8 40.2

123 9.5 7.6 11.4



#29

2,4-Dichlorophenol

Concen: 15.097 ng/ul

RT: 10.699 min Scan# 1227

Delta R.T. 0.000 min

Lab File: BG050804.D

Acq: 1 Nov 2021 20:08




Tgt Ion:162 Resp: 45213


Ion Ratio Lower Upper

162 100

164 65.3 52.2 78.4

98 38.6 30.9 46.3









#30
Naphthalene
Concen: 14.853 ng/ul
RT: 11.110 min Scan# 1297
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:128 Resp: 155370
Ion Ratio Lower Upper
128 100
129 10.6 8.5 12.7
127 13.4 10.7 16.1



#32
4-Chloroaniline
Concen: 14.588 ng/ul
RT: 11.216 min Scan# 1315
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:127 Resp: 66653
Ion Ratio Lower Upper
127 100
129 32.3 25.8 38.8









#33
Hexachlorobutadiene
Concen: 14.016 ng/ul
RT: 11.380 min Scan# 11
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:225 Resp: 28447
Ion Ratio Lower Upper
225 100
223 67.1 53.7 80.5
227 63.6 50.9 76.3



#34
Caprolactam
Concen: 9.157 ng/ul
RT: 11.968 min Scan# 1443
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:113 Resp: 11383
Ion Ratio Lower Upper
113 100
55 179.9 143.9 215.9
56 130.0 104.0 156.0









#35
 4-Chloro-3-methylphenol
 Concen: 14.801 ng/ul
 RT: 12.314 min Scan# 1502
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020407


Tgt Ion:	107	Resp:	55185
Ion	Ratio	Lower	Upper
107	100		
144	23.2	18.6	27.8
142	72.2	57.8	86.6



#36
 2-Methylnaphthalene
 Concen: 14.789 ng/ul
 RT: 12.696 min Scan# 1567
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08

Tgt Ion:	142	Resp:	103465
Ion	Ratio	Lower	Upper
142	100		
141	88.9	71.1	106.7





#37

1-Methylnaphthalene

Concen: 15.520 ng/ul

RT: 12.914 min Scan# 1

Delta R.T. 0.000 min

Lab File: BG050804.D

Acq: 1 Nov 2021 20:08

Instrument :

BNA_G

ClientSampleId :

SSTD020407





Tgt Ion:142 Resp: 109674

Ion Ratio Lower Upper

142 100

141 91.2 73.0 109.4

116 4.5 3.6 5.4



#39

1,2,4,5-Tetrachlorobenzene

Concen: 14.252 ng/ul

RT: 13.061 min Scan# 1629

Delta R.T. 0.000 min

Lab File: BG050804.D

Acq: 1 Nov 2021 20:08

Tgt Ion:216 Resp: 56468




Ion Ratio Lower Upper


216 100

214 79.1 63.3 94.9

179 20.6 16.5 24.7

108 17.0 13.6 20.4









#40
Hexachlorocyclopentadiene
Concen: 11.258 ng/ul
RT: 13.031 min Scan# 1624
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:237 Resp: 23975
Ion Ratio Lower Upper
237 100
235 58.0 46.4 69.6
272 12.0 9.6 14.4



#41
2,4,6-Trichlorophenol
Concen: 14.558 ng/ul
RT: 13.296 min Scan# 1669
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:196 Resp: 37968
Ion Ratio Lower Upper
196 100
198 98.1 78.5 117.7
200 31.9 25.5 38.3









#42
2,4,5-Trichlorophenol
Concen: 14.666 ng/ul
RT: 13.372 min Scan# 1
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:196 Resp: 40368
Ion Ratio Lower Upper
196 100
198 90.3 72.2 108.4
200 28.9 23.1 34.7



#43
1,1'-Biphenyl
Concen: 14.630 ng/ul
RT: 13.695 min Scan# 1737
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:154 Resp: 144574
Ion Ratio Lower Upper
154 100
153 42.5 34.0 51.0
76 14.9 11.9 17.9









#44
2-Chloronaphthalene
Concen: 14.368 ng/ul
RT: 13.742 min Scan# 1745
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:162 Resp: 109957
Ion Ratio Lower Upper
162 100
164 34.0 27.2 40.8
127 41.7 33.4 50.0



#45
2-Nitroaniline
Concen: 14.317 ng/ul
RT: 13.942 min Scan# 1779
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion: 65 Resp: 43699
Ion Ratio Lower Upper
65 100
92 64.7 51.8 77.6
138 88.2 70.6 105.8









#47
Dimethylphthalate
Concen: 14.642 ng/ul
RT: 14.294 min Scan# 1839
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:163 Resp: 148092
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 10.1 8.1 12.1



#48
2,6-Dinitrotoluene
Concen: 14.706 ng/ul
RT: 14.430 min Scan# 1862
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:165 Resp: 30650
Ion Ratio Lower Upper
165 100
89 66.3 53.0 79.6
121 22.6 18.1 27.1









#50
Acenaphthylene
Concen: 14.533 ng/ul
RT: 14.582 min Scan# 1888
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:152 Resp: 185857
Ion Ratio Lower Upper
152 100
151 20.8 16.6 25.0
153 14.3 11.4 17.2



#51
3-Nitroaniline
Concen: 16.908 ng/ul
RT: 14.759 min Scan# 1918
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:138 Resp: 34054
Ion Ratio Lower Upper
138 100
108 13.0 10.4 15.6
92 132.7 106.2 159.2









#52
Acenaphthene
Concen: 14.371 ng/ul
RT: 14.923 min Scan# 1946
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:153 Resp: 120067
Ion Ratio Lower Upper
153 100
152 47.2 37.8 56.6
154 85.7 68.6 102.8



#53
2,4-Dinitrophenol
Concen: 12.724 ng/ul
RT: 14.970 min Scan# 1954
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:184 Resp: 14791
Ion Ratio Lower Upper
184 100
63 68.1 54.5 81.7
154 62.0 49.6 74.4









#55
4-Nitrophenol
Concen: 13.818 ng/ul
RT: 15.058 min Scan# 1969
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:109 Resp: 24222
Ion Ratio Lower Upper
109 100
139 108.5 86.8 130.2
65 135.9 108.7 163.1



#56
Dibenzofuran
Concen: 14.737 ng/ul
RT: 15.252 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:168 Resp: 174091
Ion Ratio Lower Upper
168 100
139 40.0 32.0 48.0









#57
2,4-Dinitrotoluene
Concen: 14.951 ng/ul
RT: 15.211 min Scan# 1995
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:165 Resp: 44709
Ion Ratio Lower Upper
165 100
63 53.8 43.0 64.6
182 2.5 2.0 3.0



#58
2,3,4,6-Tetrachlorophenol
Concen: 14.912 ng/ul
RT: 15.475 min Scan# 2040
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:232 Resp: 31993
Ion Ratio Lower Upper
232 100
131 46.8 37.4 56.2
130 2.9 2.3 3.5
166 30.5 24.4 36.6









#59
Diethylphthalate
Concen: 14.731 ng/ul
RT: 15.652 min Scan# 2070
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:149 Resp: 159169
Ion Ratio Lower Upper
149 100
177 20.4 16.3 24.5
150 12.9 10.3 15.5



#61
Fluorene
Concen: 14.795 ng/ul
RT: 15.899 min Scan# 2112
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:166 Resp: 138727
Ion Ratio Lower Upper
166 100
165 97.9 78.3 117.5
167 13.2 10.6 15.8









#62
4-Chlorophenyl-phenylether
Concen: 14.598 ng/ul
RT: 15.887 min Scan# 2110
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:204 Resp: 72193
Ion Ratio Lower Upper
204 100
206 33.3 26.6 40.0
141 57.3 45.8 68.8



#63
4-Nitroaniline
Concen: 18.586 ng/ul
RT: 15.916 min Scan# 2115
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:138 Resp: 35041
Ion Ratio Lower Upper
138 100
92 54.2 43.4 65.0
108 94.6 75.7 113.5









#66
 4,6-Dinitro-2-methylphenol
 Concen: 13.598 ng/ul
 RT: 15.975 min Scan# 2125
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08




Instrument :
 BNA_G
 ClientSampleId :
 SST020407


Tgt Ion:198 Resp: 24758
 Ion Ratio Lower Upper
 198 100
 182 4.6 3.7 5.5
 77 32.0 25.6 38.4



#67
 N-Nitrosodiphenylamine
 Concen: 14.315 ng/ul
 RT: 16.098 min Scan# 2146
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08

Tgt Ion:169 Resp: 122515
 Ion Ratio Lower Upper
 169 100
 168 73.6 58.9 88.3
 167 38.1 30.5 45.7









#68
4-Bromophenyl-phenylether
Concen: 14.166 ng/ul
RT: 16.780 min Scan# 21
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:248 Resp: 42988
Ion Ratio Lower Upper
248 100
250 98.3 78.6 118.0
141 79.6 63.7 95.5



#69
Hexachlorobenzene
Concen: 14.377 ng/ul
RT: 16.903 min Scan# 2283
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:284 Resp: 44557
Ion Ratio Lower Upper
284 100
142 40.4 32.3 48.5
249 35.0 28.0 42.0









#70
 Atrazine
 Concen: 14.305 ng/ul
 RT: 17.038 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08




Instrument :
 BNA_G
 ClientSampleId :
 SST020407


Tgt Ion:200 Resp: 52411
 Ion Ratio Lower Upper
 200 100
 173 25.5 20.4 30.6
 215 46.5 37.2 55.8



#71
 Pentachlorophenol
 Concen: 10.331 ng/ul
 RT: 17.250 min Scan# 2342
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08

Tgt Ion:266 Resp: 16317
 Ion Ratio Lower Upper
 266 100
 264 70.4 56.3 84.5
 268 66.5 53.2 79.8









#72
Phenanthrene
Concen: 14.446 ng/ul
RT: 17.644 min Scan# 2409
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:178 Resp: 232601
Ion Ratio Lower Upper
178 100
179 16.3 13.0 19.6
176 19.9 15.9 23.9



#74
Anthracene
Concen: 14.775 ng/ul
RT: 17.738 min Scan# 2425
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:178 Resp: 237302
Ion Ratio Lower Upper
178 100
179 15.3 12.2 18.4
176 19.3 15.4 23.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 13.870 ng/uL
RT: 13.666 min Scan# 1
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:216 Resp: 59731
Ion Ratio Lower Upper
216 100
214 75.6 60.5 90.7
218 49.1 39.3 58.9



#76
Pentachlorobenzene
Concen: 14.060 ng/uL
RT: 15.170 min Scan# 1988
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:250 Resp: 55922
Ion Ratio Lower Upper
250 100
248 64.8 51.8 77.8
252 62.9 50.3 75.5









#77
 Carbazole
 Concen: 14.595 ng/ul
 RT: 18.002 min Scan# 2470
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020407

Tgt Ion:167 Resp: 217669




Ion	Ratio	Lower	Upper
167	100		
166	22.4	17.9	26.9
139	13.0	10.4	15.6




#78
 Di-n-butylphthalate
 Concen: 14.916 ng/ul
 RT: 18.537 min Scan# 2561
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08

Tgt Ion:149 Resp: 280955

Ion	Ratio	Lower	Upper
149	100		
150	9.4	7.5	11.3
104	6.3	5.0	7.6









#80
Fluoranthene
Concen: 15.169 ng/ul
RT: 19.641 min Scan# 2749
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:202 Resp: 281565
Ion Ratio Lower Upper
202 100
101 10.3 8.2 12.4
100 9.0 7.2 10.8



#82
Pyrene
Concen: 15.371 ng/ul
RT: 20.005 min Scan# 2811
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:202 Resp: 279007
Ion Ratio Lower Upper
202 100
101 13.3 10.6 16.0
100 11.3 9.0 13.6









#83
Butylbenzylphthalate
Concen: 14.869 ng/ul
RT: 20.869 min Scan# 2958
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:149 Resp: 114416
Ion Ratio Lower Upper
149 100
91 79.9 63.9 95.9
206 19.3 15.4 23.2



#84
3,3'-Dichlorobenzidine
Concen: 16.248 ng/ul
RT: 21.786 min Scan# 3114
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:252 Resp: 92108
Ion Ratio Lower Upper
252 100
254 64.2 51.4 77.0
126 9.5 7.6 11.4









#85
Benzo(a)anthracene
Concen: 15.341 ng/ul
RT: 21.880 min Scan# 3130
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:228 Resp: 248653
Ion Ratio Lower Upper
228 100
229 19.0 15.2 22.8
226 27.6 22.1 33.1



#86
Bis(2-ethylhexyl)phthalate
Concen: 14.944 ng/ul
RT: 21.750 min Scan# 3108
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:149 Resp: 163644
Ion Ratio Lower Upper
149 100
167 26.0 20.8 31.2
279 3.6 2.9 4.3









#87
Chrysene
Concen: 15.243 ng/ul
RT: 21.950 min Scan# 3142
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:228 Resp: 235238
Ion Ratio Lower Upper
228 100
226 30.0 24.0 36.0
229 19.9 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 17.642 ng/ul
RT: 23.020 min Scan# 3324
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:149 Resp: 277653









#90
Benzo(b)fluoranthene
Concen: 17.418 ng/ul
RT: 24.212 min Scan# 3527
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:252 Resp: 240325
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 10.1 8.1 12.1



#91
Benzo(k)fluoranthene
Concen: 17.813 ng/ul
RT: 24.289 min Scan# 3540
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:252 Resp: 229061
Ion Ratio Lower Upper
252 100
253 21.3 17.0 25.6
125 9.1 7.3 10.9









#93
Benzo(a)pyrene
Concen: 17.627 ng/ul
RT: 25.146 min Scan# 3686
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08




Instrument :
BNA_G
ClientSampleId :
SSTD020407


Tgt Ion:252 Resp: 233125
Ion Ratio Lower Upper
252 100
253 22.5 18.0 27.0
125 10.0 8.0 12.0



#94
Indeno(1,2,3-cd)pyrene
Concen: 17.805 ng/ul
RT: 29.218 min Scan# 4379
Delta R.T. 0.000 min
Lab File: BG050804.D
Acq: 1 Nov 2021 20:08

Tgt Ion:276 Resp: 260207
Ion Ratio Lower Upper
276 100
138 18.6 14.9 22.3
277 23.9 19.1 28.7









#95
 Dibenzo(a,h)anthracene
 Concen: 17.519 ng/ul
 RT: 29.283 min Scan# 4390
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08

Instrument :
 BNA_G
 ClientSampleId :
 SST020407

Tgt Ion:278 Resp: 220203
 Ion Ratio Lower Upper
 278 100
 139 15.0 12.0 18.0
 279 23.9 19.1 28.7



#96
 Benzo(g,h,i)perylene
 Concen: 17.733 ng/ul
 RT: 30.446 min Scan# 4588
 Delta R.T. 0.000 min
 Lab File: BG050804.D
 Acq: 1 Nov 2021 20:08

Tgt Ion:276 Resp: 216498
 Ion Ratio Lower Upper
 276 100
 138 18.5 14.8 22.2
 277 22.7 18.2 27.2

