

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110221\
 Data File : BG050808.D
 Acq On : 1 Nov 2021 22:53
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SICV411

Quant Time: Nov 02 03:06:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 02:58:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.234	152	45435	20.000	ng/u1	0.00
20) Naphthalene-d8	11.061	136	216261	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.856	164	148498	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.600	188	335890	20.000	ng/u1	0.00
79) Chrysene-d12	21.901	240	264935	20.000	ng/u1	0.00
88) Perylene-d12	25.303	264	223842	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.593	96	8371	6.430	ng/uL	0.00
4) Pyridine-d5	4.016	84	57606	14.846	ng/u1	0.00
7) Phenol-d5	7.371	99	66553	14.435	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.547	67	43230	14.604	ng/u1	0.00
11) 2-Chlorophenol-d4	7.759	132	47788	14.936	ng/u1	0.00
15) 4-Methylphenol-d8	8.934	113	52341	14.525	ng/u1	0.00
21) Nitrobenzene-d5	9.404	128	25482	14.394	ng/u1	0.00
24) 2-Nitrophenol-d4	10.132	143	28204	14.197	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.673	165	48702	14.449	ng/u1	0.00
31) 4-Chloroaniline-d4	11.190	131	69448	14.078	ng/u1	0.00
46) Dimethylphthalate-d6	14.251	166	154852	14.006	ng/u1	0.00
49) Acenaphthylene-d8	14.551	160	193614	14.127	ng/u1	0.00
54) 4-Nitrophenol-d4	15.044	143	26659	13.412	ng/u1	0.00
60) Fluorene-d10	15.843	176	134926	13.867	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.961	200	26300	13.258	ng/u1	0.00
73) Anthracene-d10	17.700	188	212773	13.912	ng/u1	0.00
81) Pyrene-d10	19.974	212	247436	14.978	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.068	264	194544	16.534	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.622	88	9440	5.901	ng/uL	98
5) Pyridine	4.039	79	60696	14.743	ng/u1	92
6) Benzaldehyde	7.365	77	52134	17.300	ng/u1	99
8) Phenol	7.400	94	68510	14.566	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.641	93	51850	14.573	ng/u1	96
12) 2-Chlorophenol	7.794	128	48668	14.832	ng/u1	98
13) 2-Methylphenol	8.669	108	50700	14.515	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.752	45	83151	14.990	ng/u1	98
16) Acetophenone	9.057	105	84712	15.218	ng/u1	98
17) N-Nitroso-di-n-propyla...	9.034	70	50433	14.741	ng/u1#	97
18) 4-Methylphenol	8.998	108	56158	15.103	ng/u1	90
19) Hexachloroethane	9.321	117	20618	15.002	ng/u1	90
22) Nitrobenzene	9.445	77	70645	14.354	ng/u1	96
23) Isophorone	9.968	82	136437	14.232	ng/u1	98
25) 2-Nitrophenol	10.162	139	30019	14.931	ng/u1	94
26) 2,4-Dimethylphenol	10.209	107	63159	14.253	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.444	93	73999	14.257	ng/u1	99
29) 2,4-Dichlorophenol	10.702	162	46925	14.281	ng/u1	98
30) Naphthalene	11.108	128	163732	14.314	ng/u1	99
32) 4-Chloroaniline	11.213	127	70791	14.383	ng/u1	98
33) Hexachlorobutadiene	11.378	225	31249	14.154	ng/u1	96
34) Caprolactam	11.971	113	18552	13.910	ng/u1	95
35) 4-Chloro-3-methylphenol	12.318	107	59449	14.589	ng/u1	98
36) 2-Methylnaphthalene	12.700	142	110674	14.386	ng/u1	95

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110221\
 Data File : BG050808.D
 Acq On : 1 Nov 2021 22:53
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SICV411


Quant Time: Nov 02 03:06:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 02:58:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.917	142	112963	14.244	ng/ul	95
39) 1,2,4,5-Tetrachloroben...	13.058	216	60459	14.303	ng/ul	98
40) Hexachlorocyclopentadiene	13.029	237	23533	11.736	ng/ul	91
41) 2,4,6-Trichlorophenol	13.293	196	39916	14.106	ng/ul	94
42) 2,4,5-Trichlorophenol	13.370	196	40972	13.735	ng/ul	99
43) 1,1'-Biphenyl	13.693	154	148671	14.141	ng/ul	98
44) 2-Chloronaphthalene	13.740	162	115094	14.019	ng/ul	98
45) 2-Nitroaniline	13.940	65	45928	14.244	ng/ul	98
47) Dimethylphthalate	14.298	163	156551	14.186	ng/ul	100
48) 2,6-Dinitrotoluene	14.427	165	32367	13.939	ng/ul	99
50) Acenaphthylene	14.580	152	194761	14.211	ng/ul	97
51) 3-Nitroaniline	14.756	138	34985	14.734	ng/ul#	99
52) Acenaphthene	14.921	153	127403	14.191	ng/ul	98
53) 2,4-Dinitrophenol	14.968	184	15301	12.102	ng/ul	96
55) 4-Nitrophenol	15.056	109	24469	13.175	ng/ul	99
56) Dibenzofuran	15.256	168	181061	14.019	ng/ul	98
57) 2,4-Dinitrotoluene	15.215	165	46904	14.121	ng/ul#	95
58) 2,3,4,6-Tetrachlorophenol	15.473	232	32563	13.547	ng/ul	94
59) Diethylphthalate	15.649	149	165207	13.826	ng/ul	99
61) Fluorene	15.902	166	143215	13.927	ng/ul	94
62) 4-Chlorophenyl-phenyle...	15.884	204	75912	14.019	ng/ul	98
63) 4-Nitroaniline	15.920	138	35201	14.814	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.972	198	25492	13.196	ng/ul	100
67) N-Nitrosodiphenylamine	16.096	169	127186	14.053	ng/ul	98
68) 4-Bromophenyl-phenylether	16.777	248	46264	14.281	ng/ul	95
69) Hexachlorobenzene	16.901	284	46505	13.855	ng/ul	96
70) Atrazine	17.036	200	54115	13.961	ng/ul	99
71) Pentachlorophenol	17.247	266	16873	11.021	ng/ul	94
72) Phenanthrene	17.647	178	239536	13.892	ng/ul	98
74) Anthracene	17.735	178	242754	14.090	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.663	216	62722	14.318	ng/ul	99
76) Pentachlorobenzene	15.168	250	58027	14.110	ng/ul	99
77) Carbazole	18.005	167	225712	14.405	ng/ul	99
78) Di-n-butylphthalate	18.534	149	289445	14.034	ng/ul	99
80) Fluoranthene	19.645	202	294879	14.959	ng/ul	99
82) Pyrene	20.003	202	289154	15.045	ng/ul	99
83) Butylbenzylphthalate	20.867	149	122316	15.067	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.783	252	96303	15.293	ng/ul#	99
85) Benzo(a)anthracene	21.877	228	259832	14.887	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.748	149	170231	14.434	ng/ul	99
87) Chrysene	21.948	228	246875	14.735	ng/ul	99
89) Di-n-octyl phthalate	23.017	149	292526	17.252	ng/ul	100
90) Benzo(b)fluoranthene	24.210	252	247390	16.501	ng/ul	99
91) Benzo(k)fluoranthene	24.286	252	238223	16.699	ng/ul	99
93) Benzo(a)pyrene	25.138	252	240088	16.494	ng/ul#	97
94) Indeno(1,2,3-cd)pyrene	29.204	276	267271	16.482	ng/ul	98
95) Dibenzo(a,h)anthracene	29.280	278	223879	16.300	ng/ul	98
96) Benzo(g,h,i)perylene	30.438	276	222365	16.475	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 02 03:06:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110221.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 02 02:58:24 2021
Response via : Initial Calibration









#2
 1,4-Dioxane
 Concen: 5.901 ng/uL
 RT: 3.622 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53




Instrument :
 BNA_G
 ClientSampleId :
 SICV411


Tgt Ion: 88	Resp:	9440
Ion	Ratio	Lower Upper
88	100	
43	32.2	27.2 40.8
58	71.1	58.2 87.2

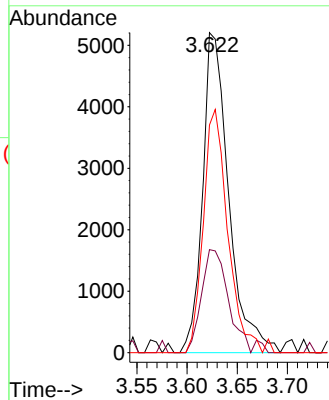

#5
 Pyridine
 Concen: 14.743 ng/uL
 RT: 4.039 min Scan# 94
 Delta R.T. 0.003 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53

Tgt Ion: 79	Resp:	60696
Ion	Ratio	Lower Upper
79	100	
52	72.7	65.1 97.7
51	35.3	29.6 44.4


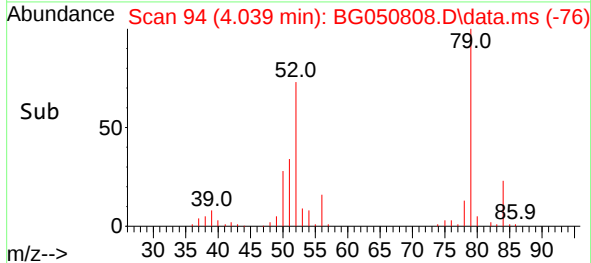
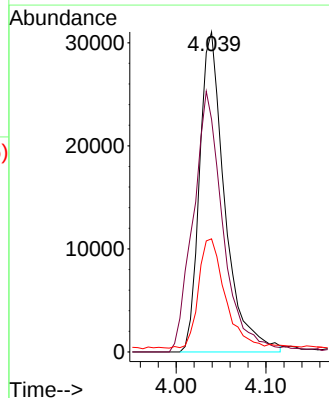





#6
Benzaldehyde
Concen: 17.300 ng/ul
RT: 7.365 min Scan# 660
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion: 77 Resp: 52134
Ion Ratio Lower Upper
77 100
105 88.5 69.8 104.6
106 84.2 67.1 100.7

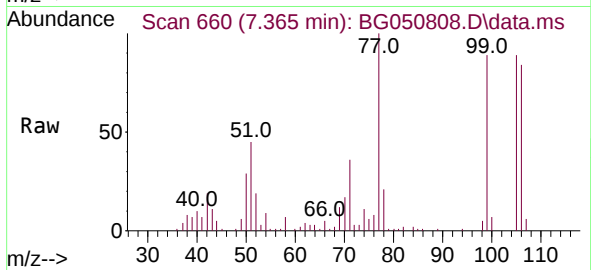

#8
Phenol
Concen: 14.566 ng/ul
RT: 7.400 min Scan# 666
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion: 94 Resp: 68510
Ion Ratio Lower Upper
94 100
65 33.0 26.2 39.4
66 38.7 32.2 48.4


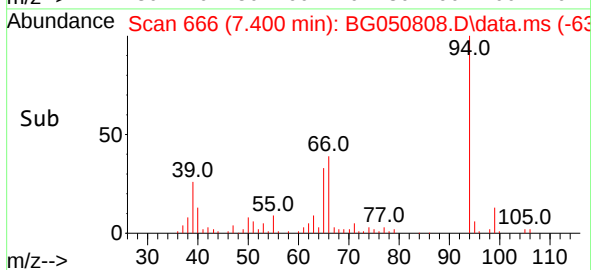






#10
 Bis(2-Chloroethyl)ether
 Concen: 14.573 ng/ul
 RT: 7.641 min Scan# 707
 Delta R.T. -0.002 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53




Instrument :
 BNA_G
 ClientSampleId :
 SICV411


Tgt Ion:	93	Resp:	51850
Ion	Ratio	Lower	Upper
93	100		
63	90.8	68.2	102.4
95	34.7	27.7	41.5



#12
 2-Chlorophenol
 Concen: 14.832 ng/ul
 RT: 7.794 min Scan# 733
 Delta R.T. -0.002 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53

Tgt Ion:	128	Resp:	48668
Ion	Ratio	Lower	Upper
128	100		
64	57.4	47.2	70.8
130	33.3	25.7	38.5



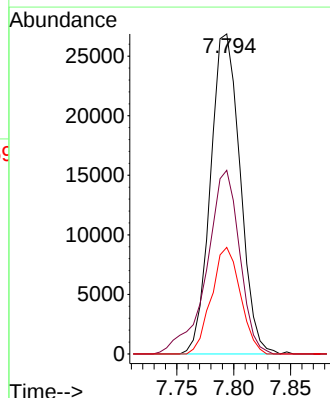





#13
2-Methylphenol
Concen: 14.515 ng/ul
RT: 8.669 min Scan# 881
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:108 Resp: 50700
Ion Ratio Lower Upper
108 100
107 88.7 72.2 108.2



#14
2,2'-oxybis(1-Chloropropane)
Concen: 14.990 ng/ul
RT: 8.752 min Scan# 896
Delta R.T. -0.008 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion: 45 Resp: 83151
Ion Ratio Lower Upper
45 100
77 15.0 12.1 18.1
79 9.1 8.5 12.7









#16
Acetophenone
Concen: 15.218 ng/ul
RT: 9.057 min Scan# 948
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:105 Resp: 84712
Ion Ratio Lower Upper
105 100
77 86.3 67.4 101.0
51 29.6 22.8 34.2



#17
N-Nitroso-di-n-propylamine
Concen: 14.741 ng/ul
RT: 9.034 min Scan# 944
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion: 70 Resp: 50433
Ion Ratio Lower Upper
70 100
42 60.9 47.6 71.4
101 8.0 6.1 9.1
130 18.9 12.2 18.2



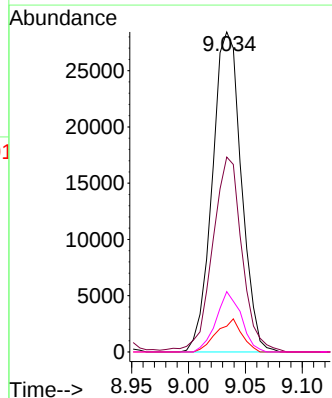





#18
4-Methylphenol
Concen: 15.103 ng/ul
RT: 8.998 min Scan# 911
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:108 Resp: 56158
Ion Ratio Lower Upper
108 100
107 110.8 97.8 146.6



#19
Hexachloroethane
Concen: 15.002 ng/ul
RT: 9.321 min Scan# 993
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:117 Resp: 20618
Ion Ratio Lower Upper
117 100
201 93.8 86.2 129.2
199 62.0 51.8 77.8


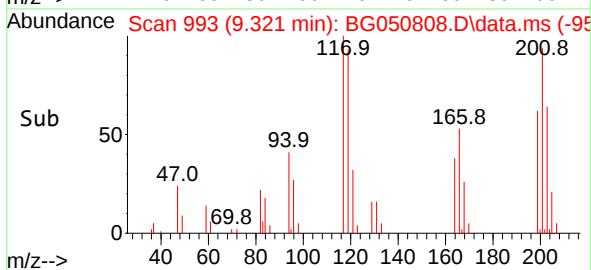




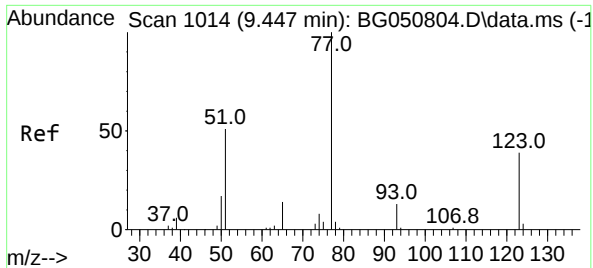

#22
Nitrobenzene
Concen: 14.354 ng/ul
RT: 9.445 min Scan# 1014
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion: 77 Resp: 70645
Ion Ratio Lower Upper
77 100
123 36.4 31.0 46.6
65 12.2 10.8 16.2

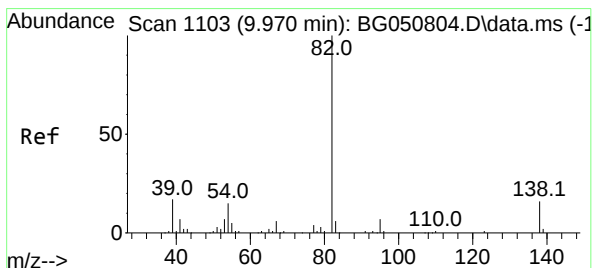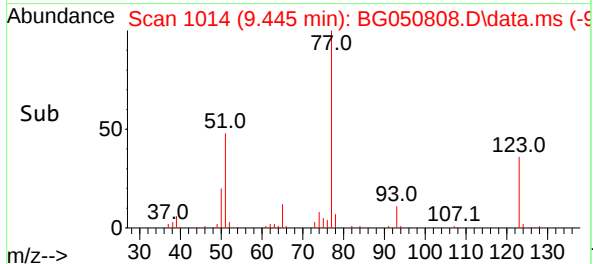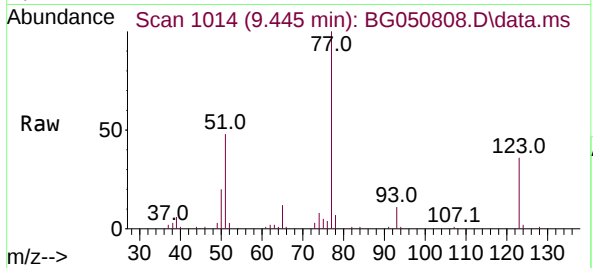

#23
Isophorone
Concen: 14.232 ng/ul
RT: 9.968 min Scan# 1103
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion: 82 Resp: 136437
Ion Ratio Lower Upper
82 100
95 6.9 5.5 8.3
138 14.4 12.4 18.6


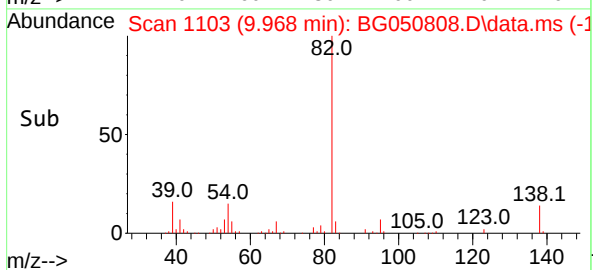

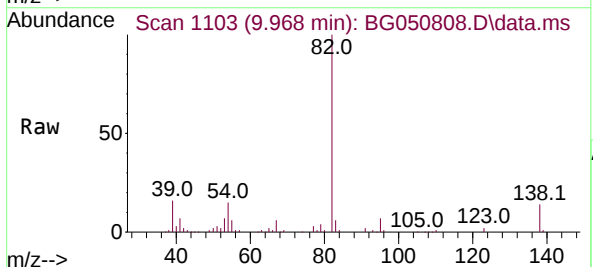




#25
2-Nitrophenol
Concen: 14.931 ng/ul
RT: 10.162 min Scan# 1136
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion	Ratio	Lower	Upper
139	100		
65	61.4	46.7	70.1
109	31.4	29.0	43.6



#26
2,4-Dimethylphenol
Concen: 14.253 ng/ul
RT: 10.209 min Scan# 1144
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion	Ratio	Lower	Upper
107	100		
121	48.3	39.1	58.7
122	78.5	64.3	96.5





#27

Bis(2-Chloroethoxy)methane

Concen: 14.257 ng/ul

RT: 10.444 min Scan# 1184

Delta R.T. -0.002 min

Lab File: BG050808.D

Acq: 1 Nov 2021 22:53

Instrument :

BNA_G

ClientSampleId :

SICV411





Tgt Ion: 93 Resp: 73999

Ion Ratio Lower Upper

93 100

95 32.7 26.8 40.2

123 9.8 7.6 11.4

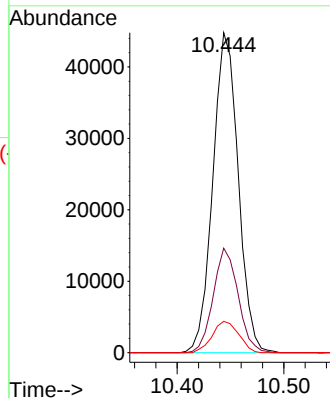

#29

2,4-Dichlorophenol

Concen: 14.281 ng/ul

RT: 10.702 min Scan# 1228

Delta R.T. 0.003 min

Lab File: BG050808.D

Acq: 1 Nov 2021 22:53




Tgt Ion:162 Resp: 46925


Ion Ratio Lower Upper

162 100

164 66.4 52.2 78.4

98 37.0 30.9 46.3


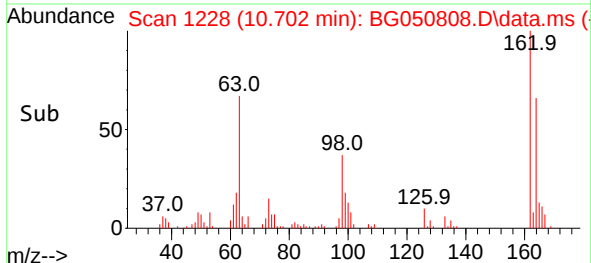
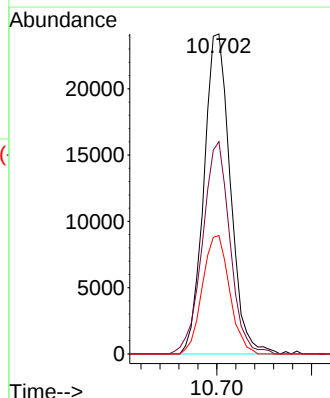





#30
Naphthalene
Concen: 14.314 ng/ul
RT: 11.108 min Scan# 1297
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:128 Resp: 163732
Ion Ratio Lower Upper
128 100
129 11.2 8.5 12.7
127 13.9 10.7 16.1



#32
4-Chloroaniline
Concen: 14.383 ng/ul
RT: 11.213 min Scan# 1315
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:127 Resp: 70791
Ion Ratio Lower Upper
127 100
129 31.1 25.8 38.8









#33
Hexachlorobutadiene
Concen: 14.154 ng/ul
RT: 11.378 min Scan# 11
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:225 Resp: 31249
Ion Ratio Lower Upper
225 100
223 60.6 53.7 80.5
227 63.2 50.9 76.3



#34
Caprolactam
Concen: 13.910 ng/ul
RT: 11.971 min Scan# 1444
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:113 Resp: 18552
Ion Ratio Lower Upper
113 100
55 178.1 143.9 215.9
56 142.2 104.0 156.0









#35
4-Chloro-3-methylphenol
Concen: 14.589 ng/ul
RT: 12.318 min Scan# 1503
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:107 Resp: 59449
Ion Ratio Lower Upper
107 100
144 23.3 18.6 27.8
142 70.4 57.8 86.6

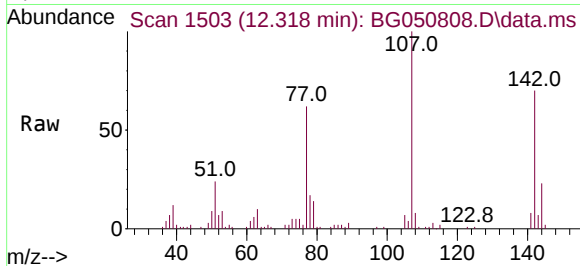

#36
2-Methylnaphthalene
Concen: 14.386 ng/ul
RT: 12.700 min Scan# 1568
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:142 Resp: 110674
Ion Ratio Lower Upper
142 100
141 93.7 71.1 106.7

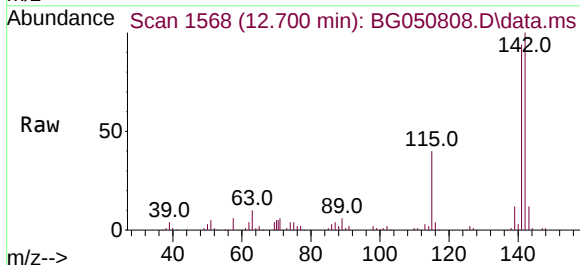



#37

1-Methylnaphthalene

Concen: 14.244 ng/ul

RT: 12.917 min Scan# 1

Delta R.T. 0.003 min

Lab File: BG050808.D

Acq: 1 Nov 2021 22:53

Instrument :

BNA_G

ClientSampleId :

SICV411





Tgt Ion:142 Resp: 112963

Ion Ratio Lower Upper

142 100

141 96.6 73.0 109.4

116 4.8 3.6 5.4

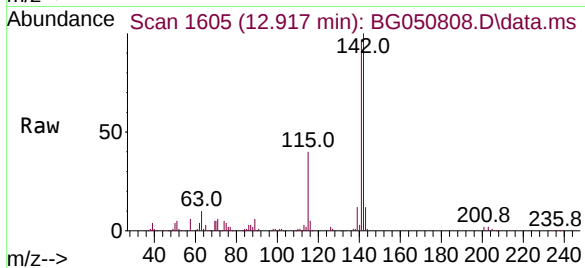

#39

1,2,4,5-Tetrachlorobenzene

Concen: 14.303 ng/ul

RT: 13.058 min Scan# 1629

Delta R.T. -0.002 min

Lab File: BG050808.D

Acq: 1 Nov 2021 22:53

Tgt Ion:216 Resp: 60459




Ion Ratio Lower Upper


216 100

214 76.5 63.3 94.9

179 20.5 16.5 24.7


108 18.2 13.6 20.4

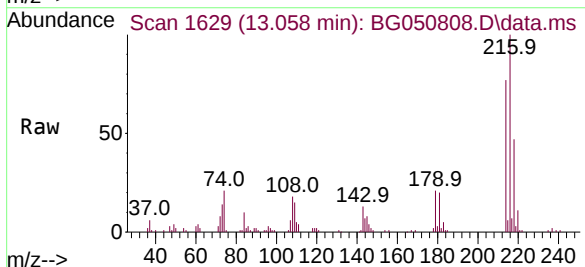






#40
Hexachlorocyclopentadiene
Concen: 11.736 ng/ul
RT: 13.029 min Scan# 1624
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53


Instrument :
BNA_G
ClientSampleId :
SICV411





Tgt Ion:237 Resp: 23533
Ion Ratio Lower Upper
237 100
235 65.9 46.4 69.6
272 12.4 9.6 14.4




#41
2,4,6-Trichlorophenol
Concen: 14.106 ng/ul
RT: 13.293 min Scan# 1669
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53



Tgt Ion:196 Resp: 39916
Ion Ratio Lower Upper
196 100
198 91.9 78.5 117.7
200 30.0 25.5 38.3



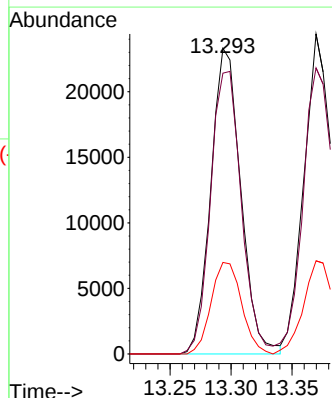





#42
2,4,5-Trichlorophenol
Concen: 13.735 ng/ul
RT: 13.370 min Scan# 1
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:196 Resp: 40972
Ion Ratio Lower Upper
196 100
198 89.4 72.2 108.4
200 29.1 23.1 34.7



#43
1,1'-Biphenyl
Concen: 14.141 ng/ul
RT: 13.693 min Scan# 1737
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:154 Resp: 148671
Ion Ratio Lower Upper
154 100
153 41.0 34.0 51.0
76 14.8 11.9 17.9


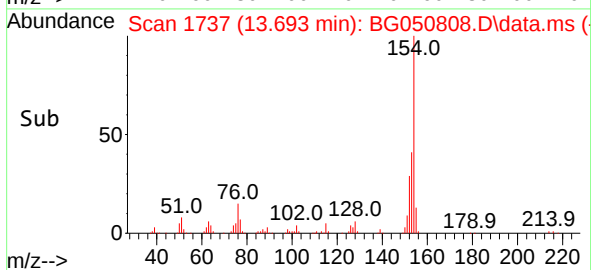






#44
2-Chloronaphthalene
Concen: 14.019 ng/ul
RT: 13.740 min Scan# 1745
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:162	Resp:	115094	
Ion	Ratio	Lower	Upper
162	100		
164	32.6	27.2	40.8
127	40.2	33.4	50.0



#45
2-Nitroaniline
Concen: 14.244 ng/ul
RT: 13.940 min Scan# 1779
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion: 65	Resp:	45928	
Ion Ratio	Lower	Upper	
65 100			
92 67.4	51.8	77.6	
138 89.3	70.6	105.8	









#47
Dimethylphthalate
Concen: 14.186 ng/ul
RT: 14.298 min Scan# 1839
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:163 Resp: 156551
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 10.2 8.1 12.1



#48
2,6-Dinitrotoluene
Concen: 13.939 ng/ul
RT: 14.427 min Scan# 1862
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:165 Resp: 32367
Ion Ratio Lower Upper
165 100
89 65.8 53.0 79.6
121 22.8 18.1 27.1









#50
Acenaphthylene
Concen: 14.211 ng/ul
RT: 14.580 min Scan# 1888
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:152 Resp: 194761
Ion Ratio Lower Upper
152 100
151 19.8 16.6 25.0
153 12.8 11.4 17.2



#51
3-Nitroaniline
Concen: 14.734 ng/ul
RT: 14.756 min Scan# 1918
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:138 Resp: 34985
Ion Ratio Lower Upper
138 100
108 10.2 10.4 15.6#
92 132.3 106.2 159.2









#52
Acenaphthene
Concen: 14.191 ng/ul
RT: 14.921 min Scan# 1946
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:153 Resp: 127403
Ion Ratio Lower Upper
153 100
152 48.1 37.8 56.6
154 87.6 68.6 102.8

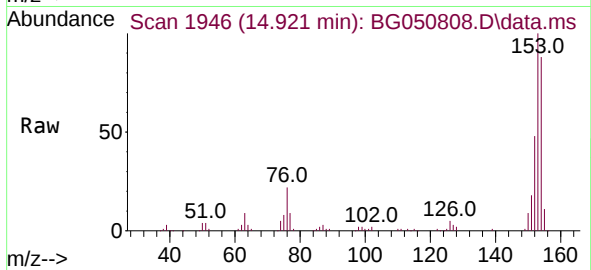

#53
2,4-Dinitrophenol
Concen: 12.102 ng/ul
RT: 14.968 min Scan# 1954
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:184 Resp: 15301
Ion Ratio Lower Upper
184 100
63 71.7 54.5 81.7
154 59.2 49.6 74.4









#55
4-Nitrophenol
Concen: 13.175 ng/ul
RT: 15.056 min Scan# 1969
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:109 Resp: 24469
Ion Ratio Lower Upper
109 100
139 111.3 86.8 130.2
65 136.0 108.7 163.1

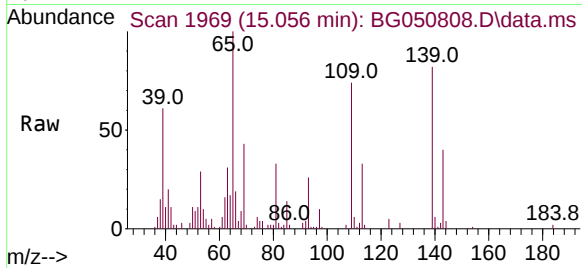

#56
Dibenzofuran
Concen: 14.019 ng/ul
RT: 15.256 min Scan# 2003
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:168 Resp: 181061
Ion Ratio Lower Upper
168 100
139 38.7 32.0 48.0




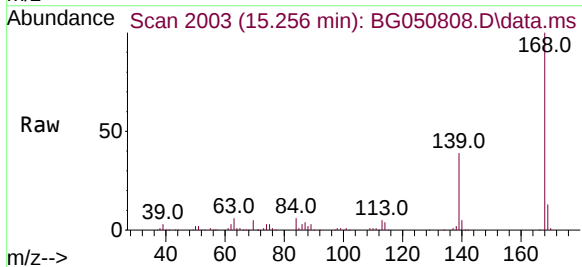




#57
2,4-Dinitrotoluene
Concen: 14.121 ng/ul
RT: 15.215 min Scan# 1996
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:165 Resp: 46904
Ion Ratio Lower Upper
165 100
63 50.4 43.0 64.6
182 3.2 2.0 3.0#



#58
2,3,4,6-Tetrachlorophenol
Concen: 13.547 ng/ul
RT: 15.473 min Scan# 2040
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:232 Resp: 32563
Ion Ratio Lower Upper
232 100
131 50.7 37.4 56.2
130 2.8 2.3 3.5
166 34.1 24.4 36.6









#59
Diethylphthalate
Concen: 13.826 ng/ul
RT: 15.649 min Scan# 2070
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:149 Resp: 165207
Ion Ratio Lower Upper
149 100
177 21.2 16.3 24.5
150 12.7 10.3 15.5



#61
Fluorene
Concen: 13.927 ng/ul
RT: 15.902 min Scan# 2113
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:166 Resp: 143215
Ion Ratio Lower Upper
166 100
165 104.2 78.3 117.5
167 14.2 10.6 15.8









#62
4-Chlorophenyl-phenylether
Concen: 14.019 ng/ul
RT: 15.884 min Scan# 2110
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:204 Resp: 75912
Ion Ratio Lower Upper
204 100
206 33.7 26.6 40.0
141 59.1 45.8 68.8



#63
4-Nitroaniline
Concen: 14.814 ng/ul
RT: 15.920 min Scan# 2116
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:138 Resp: 35201
Ion Ratio Lower Upper
138 100
92 55.7 43.4 65.0
108 89.4 75.7 113.5









#66
 4,6-Dinitro-2-methylphenol
 Concen: 13.196 ng/ul
 RT: 15.972 min Scan# 2125
 Delta R.T. -0.002 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53




Instrument :
 BNA_G
 ClientSampleId :
 SICV411


Tgt Ion:198 Resp: 25492
 Ion Ratio Lower Upper
 198 100
 182 4.6 3.7 5.5
 77 32.1 25.6 38.4



#67
 N-Nitrosodiphenylamine
 Concen: 14.053 ng/ul
 RT: 16.096 min Scan# 2146
 Delta R.T. -0.002 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53

Tgt Ion:169 Resp: 127186
 Ion Ratio Lower Upper
 169 100
 168 72.1 58.9 88.3
 167 40.3 30.5 45.7









#68
4-Bromophenyl-phenylether
Concen: 14.281 ng/ul
RT: 16.777 min Scan# 21
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:248 Resp: 46264
Ion Ratio Lower Upper
248 100
250 91.9 78.6 118.0
141 82.2 63.7 95.5

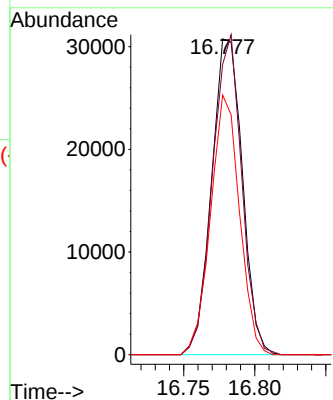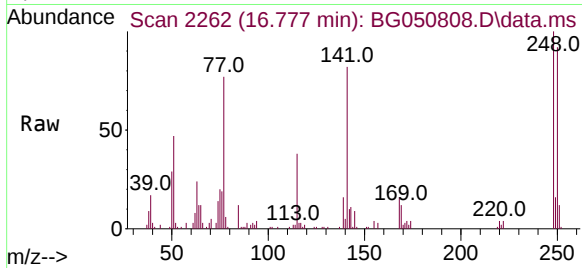

#69
Hexachlorobenzene
Concen: 13.855 ng/ul
RT: 16.901 min Scan# 2283
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:284 Resp: 46505
Ion Ratio Lower Upper
284 100
142 44.7 32.3 48.5
249 35.2 28.0 42.0

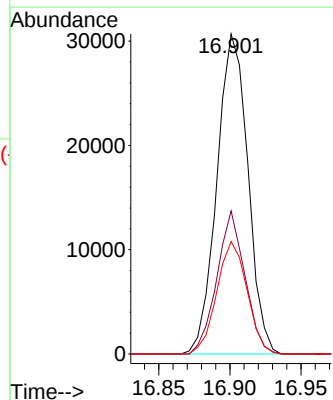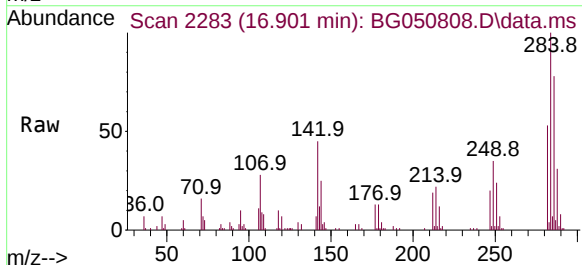



#70

Atrazine

Concen: 13.961 ng/ul

RT: 17.036 min Scan# 21

Delta R.T. -0.002 min

Lab File: BG050808.D

Acq: 1 Nov 2021 22:53

Instrument :

BNA_G

ClientSampleId :

SICV411





Tgt Ion:200 Resp: 54115

Ion Ratio Lower Upper

200 100

173 27.0 20.4 30.6

215 46.3 37.2 55.8

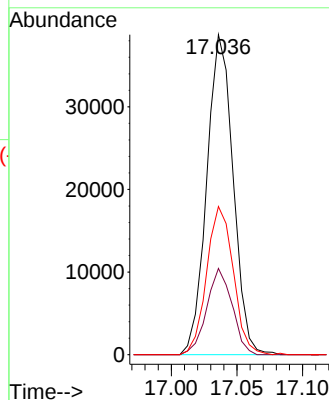

#71

Pentachlorophenol

Concen: 11.021 ng/ul

RT: 17.247 min Scan# 2342

Delta R.T. -0.002 min

Lab File: BG050808.D

Acq: 1 Nov 2021 22:53




Tgt Ion:266 Resp: 16873


Ion Ratio Lower Upper

266 100

264 67.8 56.3 84.5

268 58.7 53.2 79.8



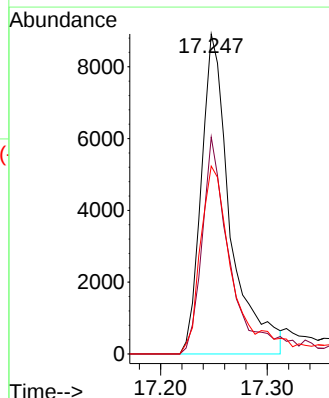





#72
Phenanthrene
Concen: 13.892 ng/ul
RT: 17.647 min Scan# 2409
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:178 Resp: 239536
Ion Ratio Lower Upper
178 100
179 15.2 13.0 19.6
176 19.5 15.9 23.9



#74
Anthracene
Concen: 14.090 ng/ul
RT: 17.735 min Scan# 2425
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:178 Resp: 242754
Ion Ratio Lower Upper
178 100
179 15.3 12.2 18.4
176 19.5 15.4 23.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 14.318 ng/uL
RT: 13.663 min Scan# 1732
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:216 Resp: 62722
Ion Ratio Lower Upper
216 100
214 77.6 60.5 90.7
218 49.0 39.3 58.9



#76
Pentachlorobenzene
Concen: 14.110 ng/uL
RT: 15.168 min Scan# 1988
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:250 Resp: 58027
Ion Ratio Lower Upper
250 100
248 64.3 51.8 77.8
252 64.1 50.3 75.5









#77
 Carbazole
 Concen: 14.405 ng/ul
 RT: 18.005 min Scan# 2470
 Delta R.T. 0.003 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53




Instrument :
 BNA_G
 ClientSampleId :
 SICV411


Tgt Ion:167 Resp: 225712
 Ion Ratio Lower Upper
 167 100
 166 21.9 17.9 26.9
 139 13.4 10.4 15.6

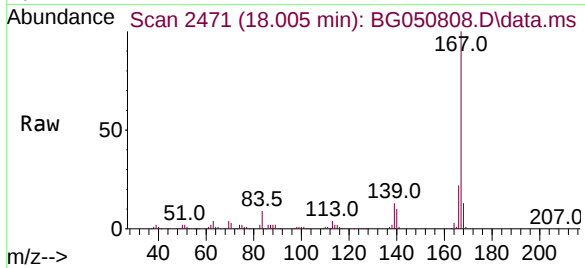

#78
 Di-n-butylphthalate
 Concen: 14.034 ng/ul
 RT: 18.534 min Scan# 2561
 Delta R.T. -0.002 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53

Tgt Ion:149 Resp: 289445
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.5 11.3
 104 6.0 5.0 7.6




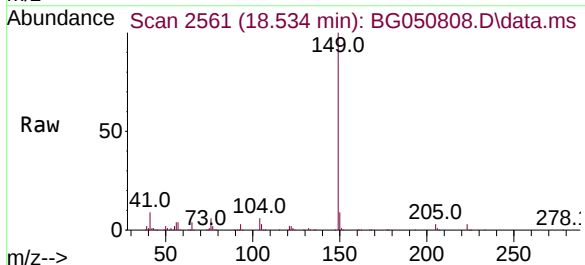


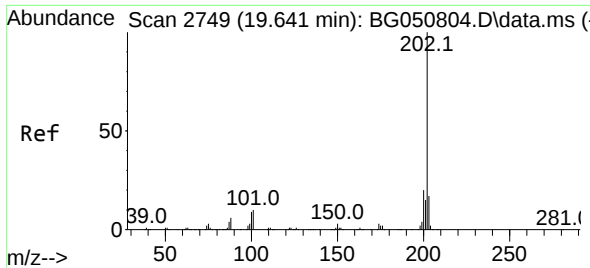

#80
Fluoranthene
Concen: 14.959 ng/ul
RT: 19.645 min Scan# 2749
Delta R.T. 0.003 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:202 Resp: 294879
Ion Ratio Lower Upper
202 100
101 11.0 8.2 12.4
100 8.8 7.2 10.8

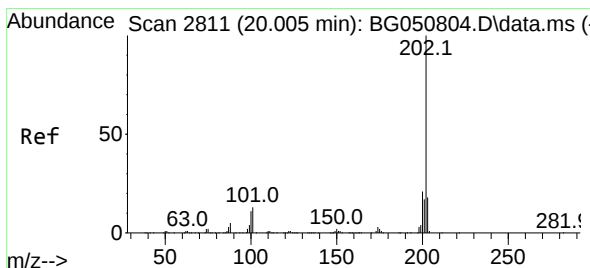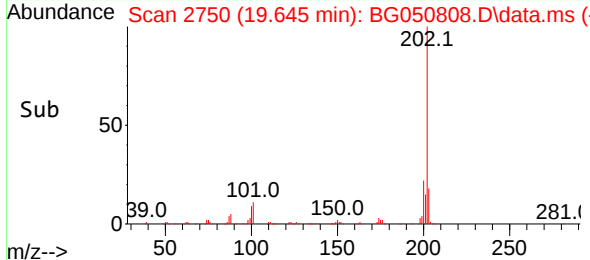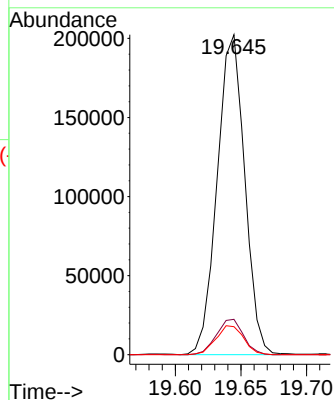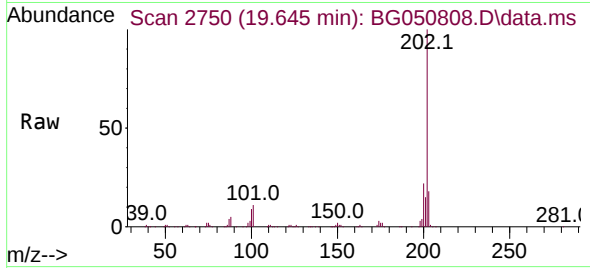

#82
Pyrene
Concen: 15.045 ng/ul
RT: 20.003 min Scan# 2811
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:202 Resp: 289154
Ion Ratio Lower Upper
202 100
101 12.9 10.6 16.0
100 11.0 9.0 13.6


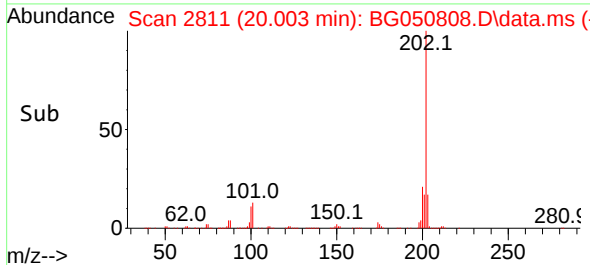
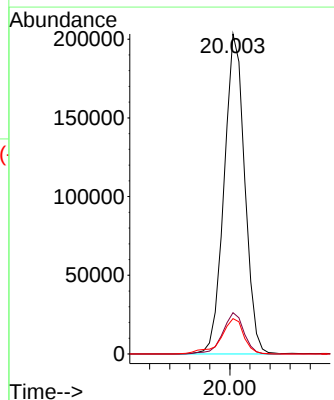
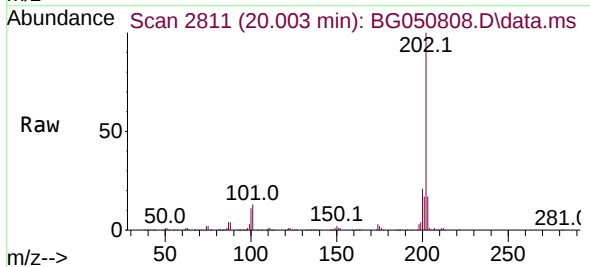




#83
Butylbenzylphthalate
Concen: 15.067 ng/ul
RT: 20.867 min Scan# 2958
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:149 Resp: 122316
Ion Ratio Lower Upper
149 100
91 82.1 63.9 95.9
206 19.2 15.4 23.2



#84
3,3'-Dichlorobenzidine
Concen: 15.293 ng/ul
RT: 21.783 min Scan# 3114
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:252 Resp: 96303
Ion Ratio Lower Upper
252 100
254 63.5 51.4 77.0
126 11.5 7.6 11.4#


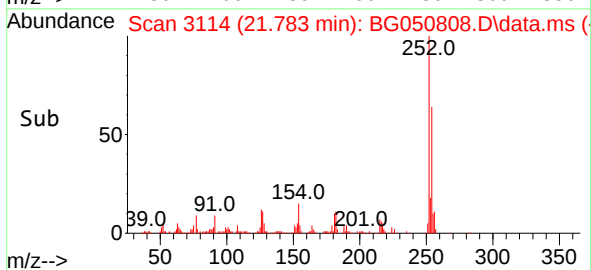






#85
 Benzo(a)anthracene
 Concen: 14.887 ng/ul
 RT: 21.877 min Scan# 3130
 Delta R.T. -0.002 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53




Instrument :
 BNA_G
 ClientSampleId :
 SICV411


Tgt Ion:228 Resp: 259832
 Ion Ratio Lower Upper
 228 100
 229 20.1 15.2 22.8
 226 26.8 22.1 33.1

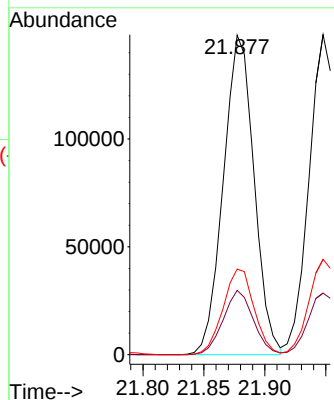

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 14.434 ng/ul
 RT: 21.748 min Scan# 3108
 Delta R.T. -0.002 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53

Tgt Ion:149 Resp: 170231
 Ion Ratio Lower Upper
 149 100
 167 26.4 20.8 31.2
 279 3.3 2.9 4.3



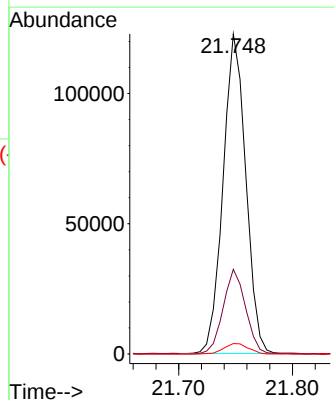





#87
Chrysene
Concen: 14.735 ng/ul
RT: 21.948 min Scan# 3142
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:228 Resp: 246875
Ion Ratio Lower Upper
228 100
226 29.8 24.0 36.0
229 19.2 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 17.252 ng/ul
RT: 23.017 min Scan# 3324
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:149 Resp: 292526


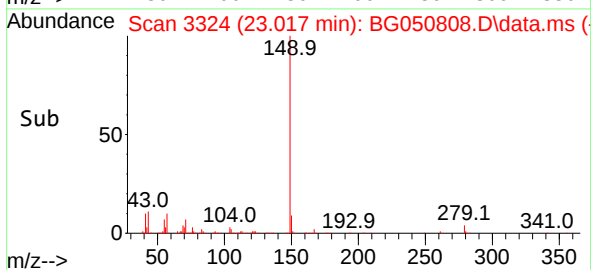






#90
Benzo(b)fluoranthene
Concen: 16.501 ng/ul
RT: 24.210 min Scan# 3527
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:252 Resp: 247390
Ion Ratio Lower Upper
252 100
253 22.8 17.8 26.8
125 10.9 8.1 12.1

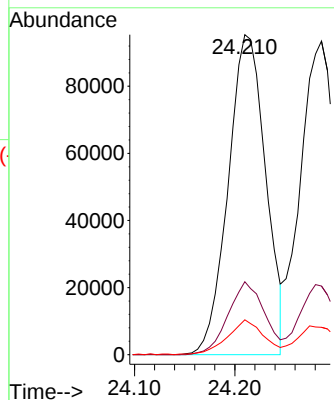

#91
Benzo(k)fluoranthene
Concen: 16.699 ng/ul
RT: 24.286 min Scan# 3540
Delta R.T. -0.002 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:252 Resp: 238223
Ion Ratio Lower Upper
252 100
253 21.9 17.0 25.6
125 8.8 7.3 10.9


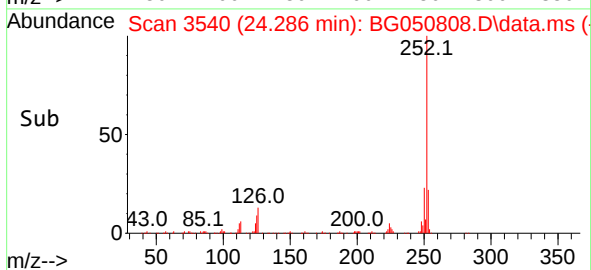
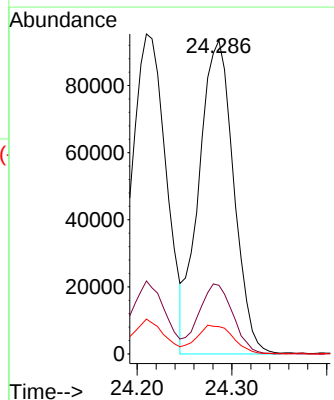





#93
Benzo(a)pyrene
Concen: 16.494 ng/ul
RT: 25.138 min Scan# 3
Delta R.T. -0.008 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53




Instrument :
BNA_G
ClientSampleId :
SICV411


Tgt Ion:252 Resp: 240088
Ion Ratio Lower Upper
252 100
253 21.7 18.0 27.0
125 12.1 8.0 12.0#



#94
Indeno(1,2,3-cd)pyrene
Concen: 16.482 ng/ul
RT: 29.204 min Scan# 4377
Delta R.T. -0.014 min
Lab File: BG050808.D
Acq: 1 Nov 2021 22:53

Tgt Ion:276 Resp: 267271
Ion Ratio Lower Upper
276 100
138 20.1 14.9 22.3
277 24.3 19.1 28.7


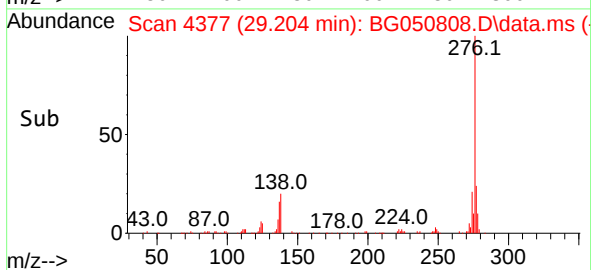






#95
 Dibenzo(a,h)anthracene
 Concen: 16.300 ng/ul
 RT: 29.280 min Scan# 41
 Delta R.T. -0.002 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53

Instrument :
 BNA_G
 ClientSampleId :
 SICV411

Tgt Ion:278 Resp: 223879
 Ion Ratio Lower Upper
 278 100
 139 13.9 12.0 18.0
 279 24.9 19.1 28.7



#96
 Benzo(g,h,i)perylene
 Concen: 16.475 ng/ul
 RT: 30.438 min Scan# 4587
 Delta R.T. -0.008 min
 Lab File: BG050808.D
 Acq: 1 Nov 2021 22:53

Tgt Ion:276 Resp: 222365
 Ion Ratio Lower Upper
 276 100
 138 20.5 14.8 22.2
 277 25.4 18.2 27.2

