

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110315\
 Data File : BG019451.D
 Acq On : 3 Nov 2015 14:23
 Operator : UM/NP
 Sample : PB86394BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK94

Quant Time: Nov 04 00:16:08 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 04 00:13:26 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	23941	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	100186	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	81976	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	253776	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	357738	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	339922	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	3879	7.76	ng/uL	0.00
5) Phenol-d5	7.33	99	81901	37.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.50	67	59054	42.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.71	132	53350	38.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	68091	38.90	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	28832	39.16	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	34340	39.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	69269	36.53	ng/ul	0.00
29) 4-Chloroaniline-d4	11.14	131	68761	35.85	ng/ul	0.00
44) Dimethylphthalate-d6	14.21	166	304651	45.07	ng/ul	0.00
47) Acenaphthylene-d8	14.51	160	297330	39.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.99	143	49950	46.52	ng/ul	0.00
58) Fluorene-d10	15.80	176	250881	40.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	59038	35.94	ng/ul	0.00
71) Anthracene-d10	17.65	188	465449	40.23	ng/ul	0.00
79) Pyrene-d10	19.92	212	601894	38.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.95	264	684364	40.12	ng/ul	0.00


Target Compounds						Qvalue
15) N-Nitroso-di-n-propylamine	8.88	70	2395	1.24	ng/ul#	1
21) Isophorone	10.08	82	5538	1.06	ng/ul#	77




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110315\
Data File : BG019451.D
Acq On : 3 Nov 2015 14:23
Operator : UM/NP
Sample : PB86394BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK94

Quant Time: Nov 04 00:16:08 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 04 00:13:26 2015
Response via : Initial Calibration




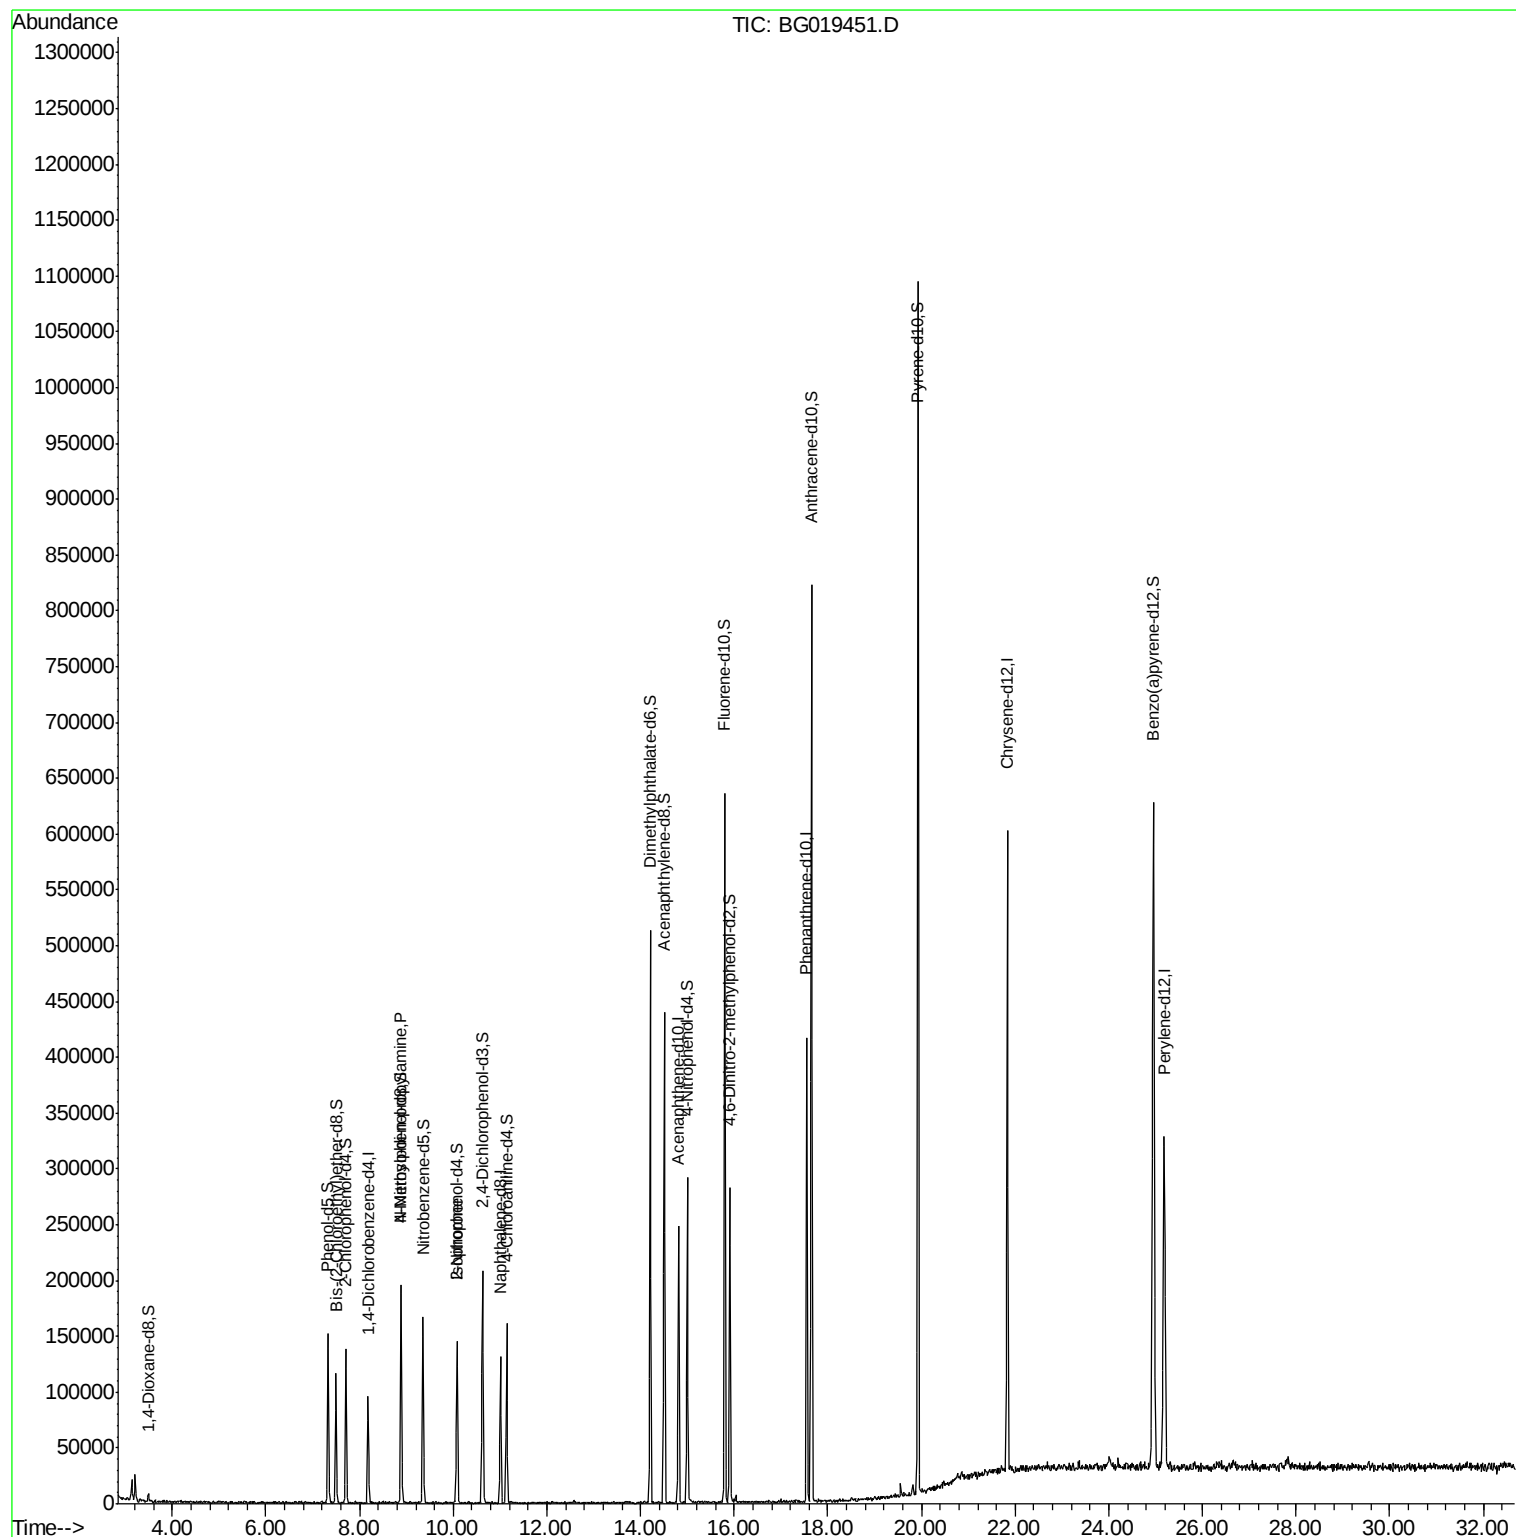


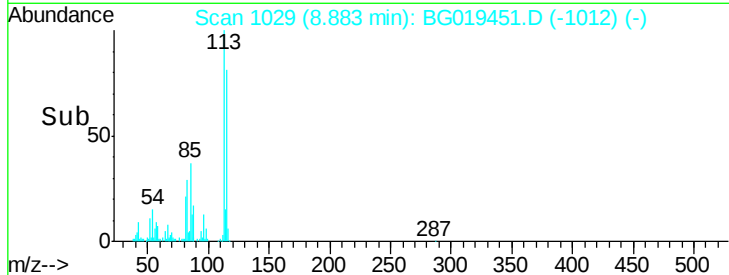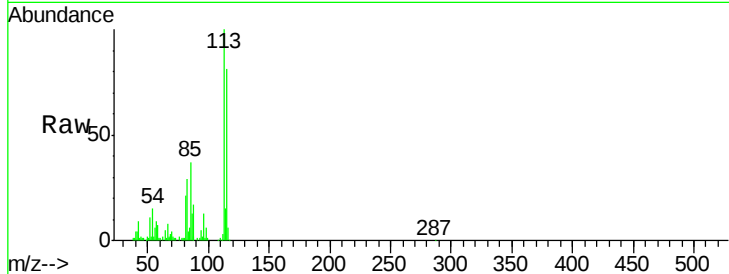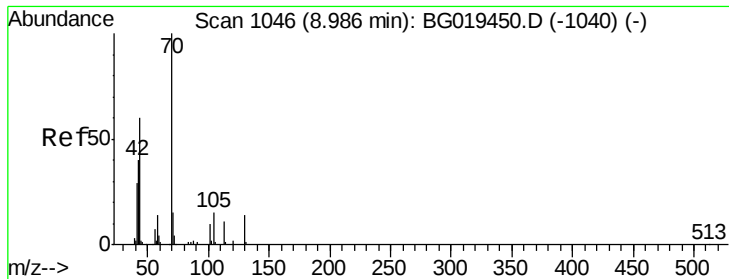

#15
N-Nitroso-di-n-propylamine
Concen: 1.24 ng/ul
RT: 8.88 min Scan# 1029
Delta R.T. -0.10 min
Lab File: BG019451.D
Acq: 3 Nov 2015 14:23

Instrument :
BNA_G
ClientSampleId :
SBLK94

Tgt Ion:	70	Resp:	2395
Ion	Ratio	Lower	Upper
70	100		
42	212.3	36.6	55.0#
101	0.0	5.8	8.8#
130	0.0	14.6	22.0#

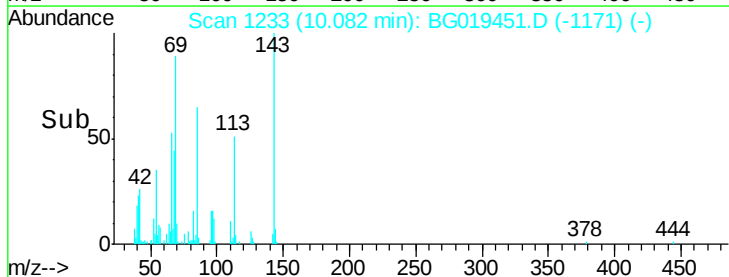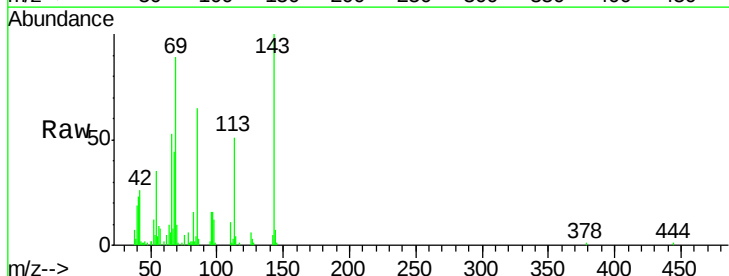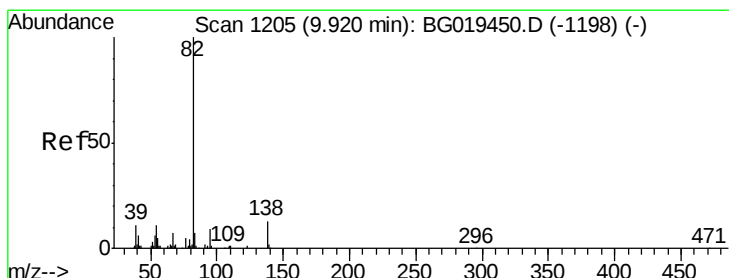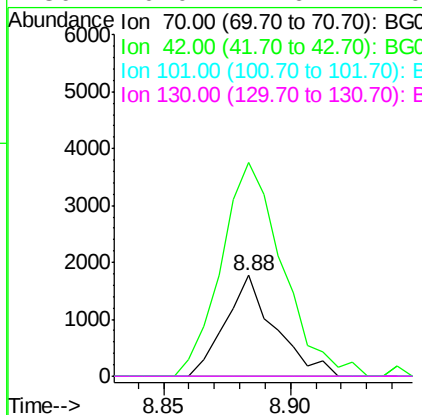

#21
Isophorone
Concen: 1.06 ng/ul
RT: 10.08 min Scan# 1233
Delta R.T. 0.16 min
Lab File: BG019451.D
Acq: 3 Nov 2015 14:23

Tgt Ion:	82	Resp:	5538
Ion	Ratio	Lower	Upper
82	100		
95	10.5	6.7	10.1#
138	0.0	10.8	16.2#

