

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110315\
 Data File : BG019453.D
 Acq On : 3 Nov 2015 15:39
 Operator : UM/NP
 Sample : G4202-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCY40

Quant Time: Nov 04 00:16:31 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 04 00:13:26 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	25603	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	105715	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	84762	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	251007	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	364057	20.00	ng/ul	0.00
86) Perylene-d12	25.19	264	338629	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	363	0.68	ng/uL	0.00
5) Phenol-d5	7.33	99	16594	7.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	53383	35.83	ng/ul	0.00
9) 2-Chlorophenol-d4	7.71	132	40469	27.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	32753	17.50	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	26965	34.71	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	32920	35.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	63975	31.97	ng/ul	0.00
29) 4-Chloroaniline-d4	11.13	131	378	0.19	ng/ul	0.00
44) Dimethylphthalate-d6	14.21	166	271907	38.91	ng/ul	0.00
47) Acenaphthylene-d8	14.51	160	287057	37.09	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	8195	7.38	ng/ul	0.00
58) Fluorene-d10	15.80	176	231773	35.85	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	56404	34.72	ng/ul	0.00
71) Anthracene-d10	17.65	188	408435	35.70	ng/ul	0.00
79) Pyrene-d10	19.92	212	524569	32.93	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.95	264	589191	34.67	ng/ul	0.00


Target Compounds					Qvalue
21) Isophorone	10.08	82	5758	1.05 ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110315\
Data File : BG019453.D
Acq On : 3 Nov 2015 15:39
Operator : UM/NP
Sample : G4202-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCY40

Quant Time: Nov 04 00:16:31 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 04 00:13:26 2015
Response via : Initial Calibration

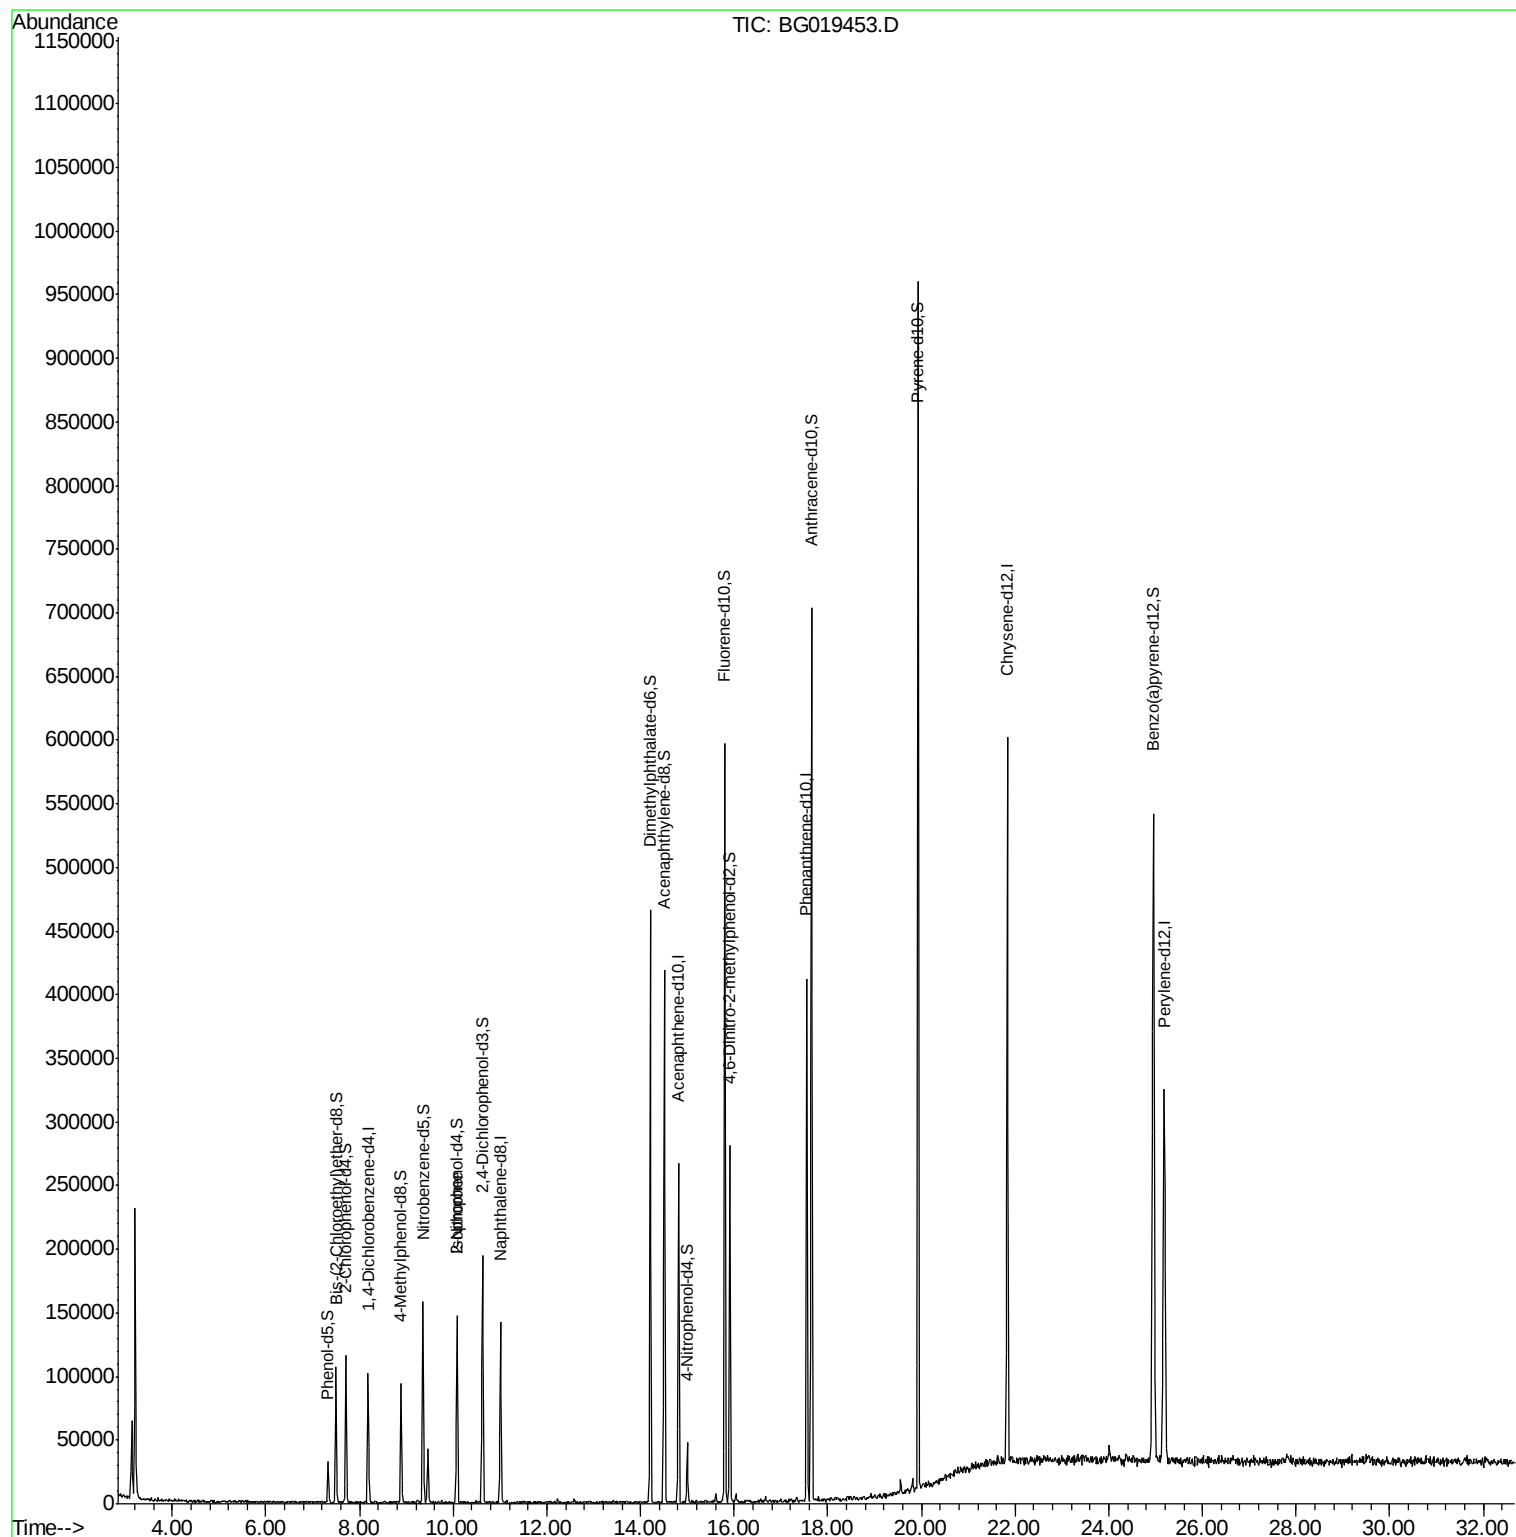

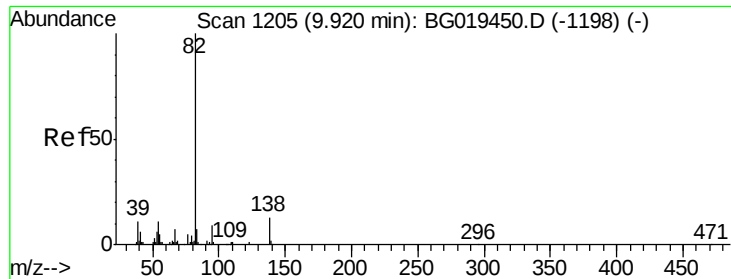

#21
Isophorone
Concen: 1.05 ng/ul
RT: 10.08 min Scan# 1232
Delta R.T. 0.16 min
Lab File: BG019453.D
Acq: 3 Nov 2015 15:39

Instrument :
BNA_G
ClientSampleId :
BCY40

Tgt Ion: 82 Resp: 5758
Ion Ratio Lower Upper
82 100
95 0.0 6.7 10.1#
138 0.0 10.8 16.2#

