

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110315\
 Data File : BG019458.D
 Acq On : 3 Nov 2015 18:50
 Operator : UM/NP
 Sample : G4202-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCY43

Quant Time: Nov 04 00:17:26 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 04 00:13:26 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	26672	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	108313	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	90615	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	267188	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	364565	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	349674	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.49	96	903	1.62	ng/uL	0.00
5) Phenol-d5	7.33	99	20751	8.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	62178	40.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.71	132	46257	30.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	38282	19.63	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	30674	38.53	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	35826	37.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	71699	34.97	ng/ul	0.00
29) 4-Chloroaniline-d4	11.15	131	3856	1.86	ng/ul	0.00
44) Dimethylphthalate-d6	14.21	166	307168	41.11	ng/ul	0.00
47) Acenaphthylene-d8	14.51	160	320491	38.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.99	143	10699	9.01	ng/ul	0.00
58) Fluorene-d10	15.80	176	272224	39.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.91	200	67597	39.09	ng/ul	0.00
71) Anthracene-d10	17.65	188	490157	40.24	ng/ul	0.00
79) Pyrene-d10	19.92	212	613699	38.47	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.95	264	691204	39.39	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
21) Isophorone	10.08	82	6013	1.07	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110315\
Data File : BG019458.D
Acq On : 3 Nov 2015 18:50
Operator : UM/NP
Sample : G4202-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCY43

Quant Time: Nov 04 00:17:26 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 04 00:13:26 2015
Response via : Initial Calibration

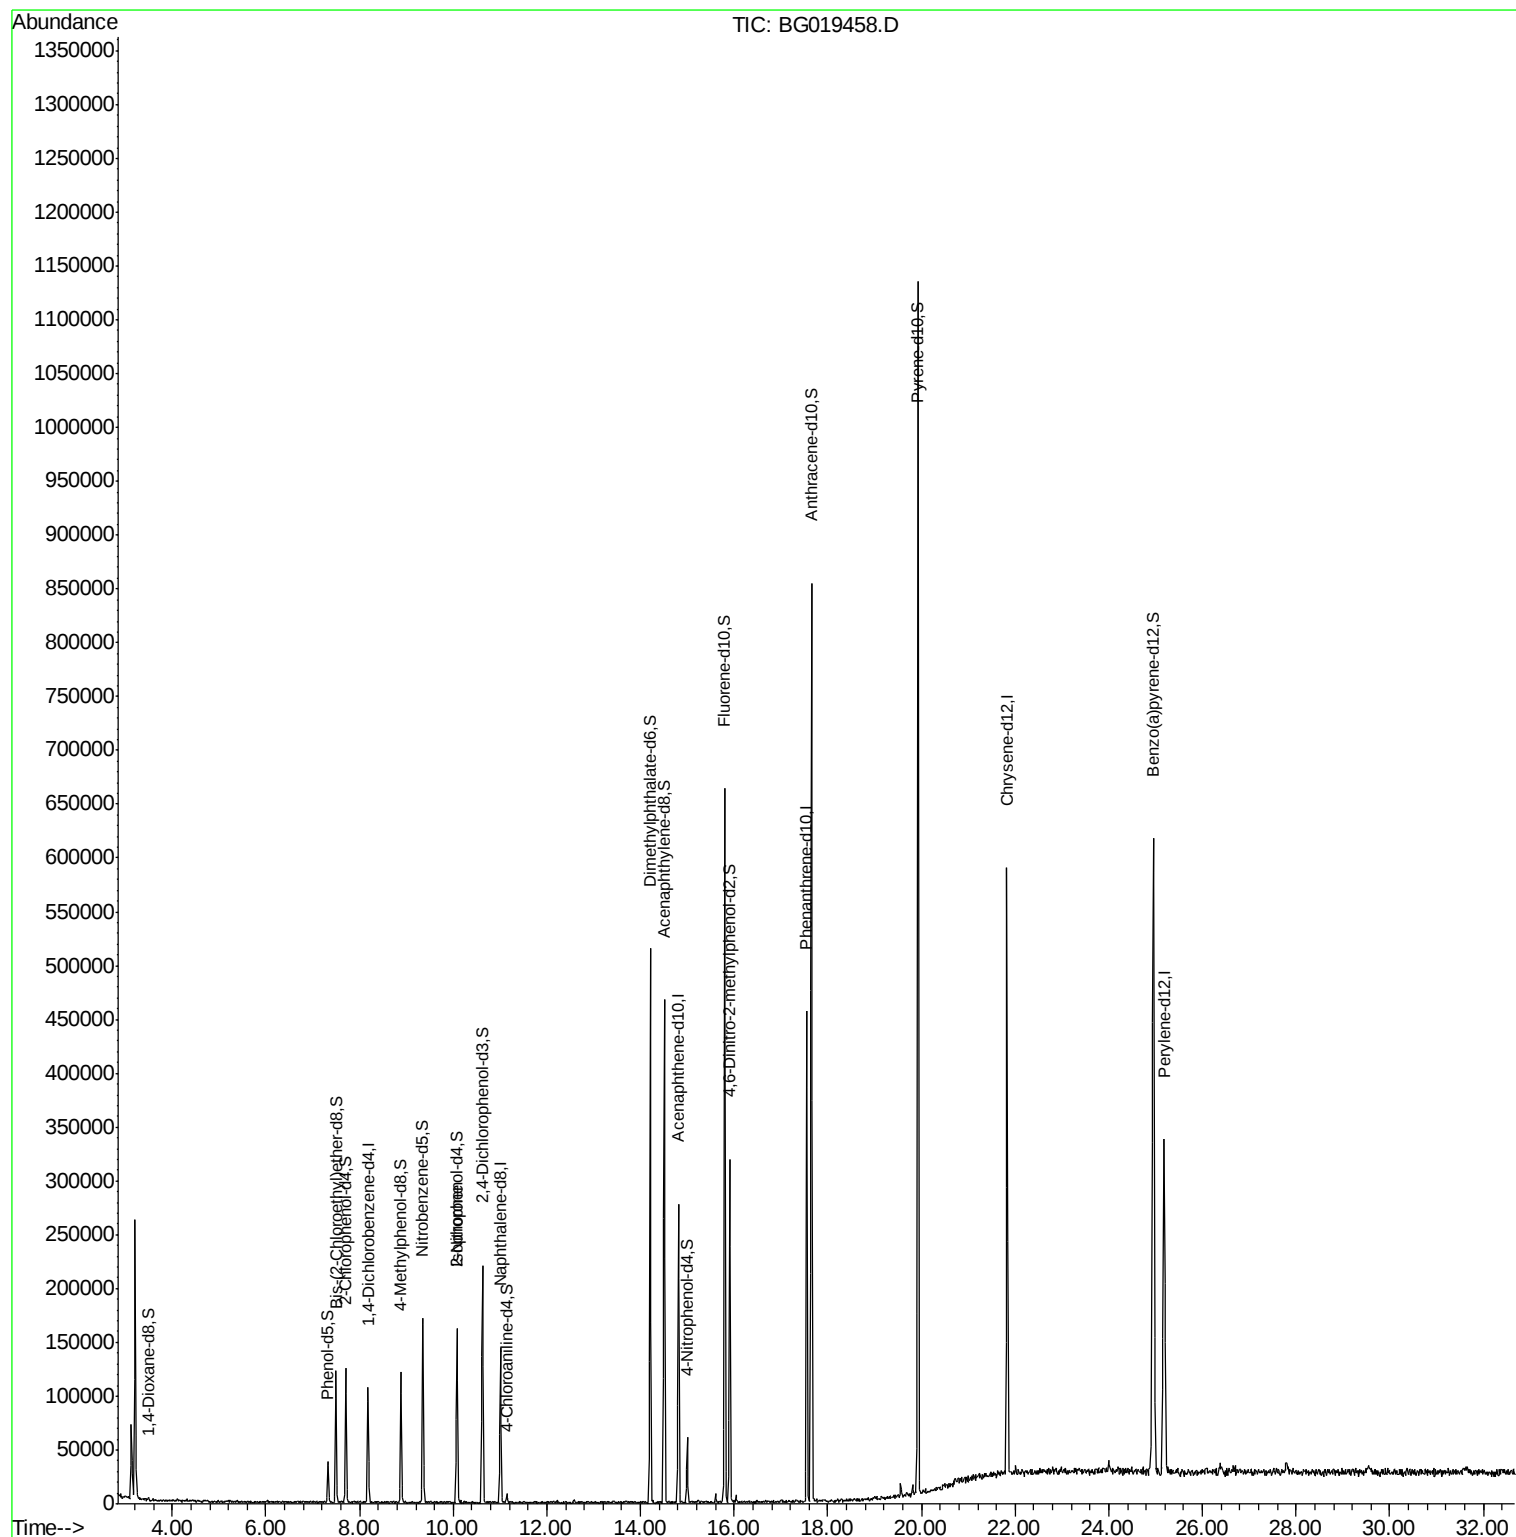

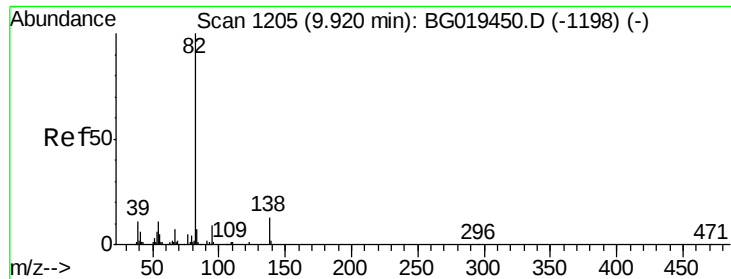

#21
Isophorone
Concen: 1.07 ng/ul
RT: 10.08 min Scan# 1233
Delta R.T. 0.16 min
Lab File: BG019458.D
Acq: 3 Nov 2015 18:50

Instrument :
BNA_G
ClientSampleId :
BCY43

Tgt Ion: 82 Resp: 6013
Ion Ratio Lower Upper
82 100
95 12.8 6.7 10.1#
138 0.0 10.8 16.2#

