

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110316\
 Data File : BG024669.D
 Acq On : 4 Nov 2016 5:28
 Operator : UM/SJ
 Sample : H5509-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-92-22.5-23.0

Quant Time: Nov 04 05:45:06 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	86284	20.00	ng	0.00
21) Naphthalene-d8	11.09	136	345545	20.00	ng	0.00
38) Acenaphthene-d10	14.88	164	274656	20.00	ng	0.00
63) Phenanthrene-d10	17.62	188	653033	20.00	ng	0.00
75) Chrysene-d12	21.91	240	895237	20.00	ng	-0.02
86) Perylene-d12	25.35	264	899831	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.80	112	806151	153.13	ng	0.00
7) Phenol-d6	7.40	99	1137873	157.57	ng	0.00
23) Nitrobenzene-d5	9.44	82	799320	105.32	ng	0.00
41) 2,4,6-Tribromophenol	16.37	330	638883	155.70	ng	0.00
44) 2-Fluorobiphenyl	13.51	172	1514036	91.62	ng	0.00
78) Terphenyl-d14	20.21	244	2684168	89.59	ng	0.00
Target Compounds						
10) Phenol	7.44	94	18321	2.46	ng	84
49) Dimethylphthalate	14.32	163	544583	27.93	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110316\
Data File : BG024669.D
Acq On : 4 Nov 2016 5:28
Operator : UM/SJ
Sample : H5509-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-92-22.5-23.0

Quant Time: Nov 04 05:45:06 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

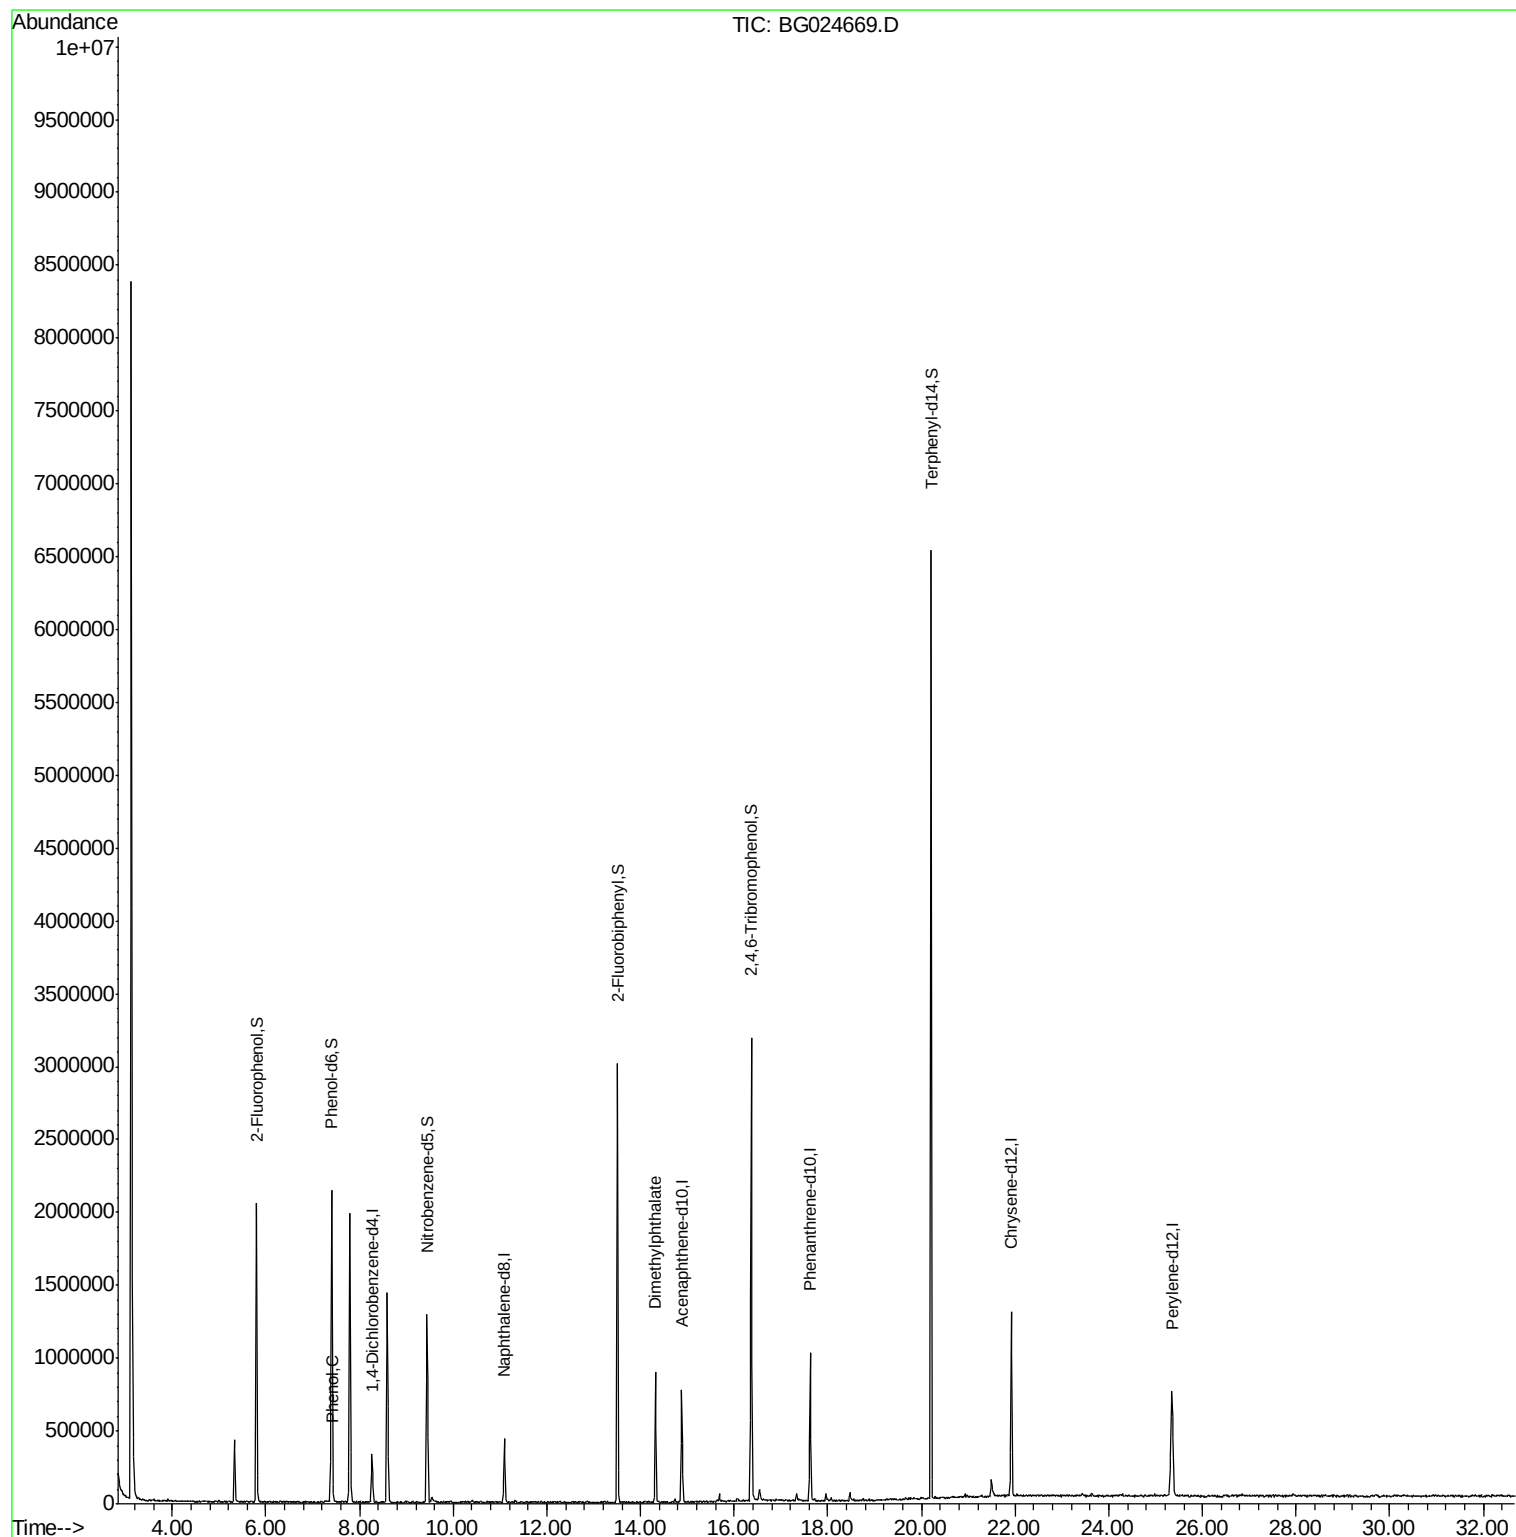

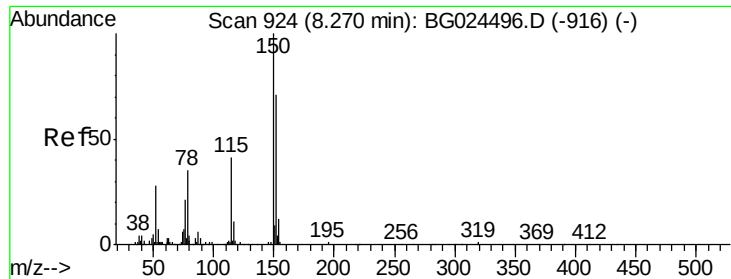


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.27 min Scan# 924
Delta R.T. -0.00 min
Lab File: BG024669.D
Acq: 4 Nov 2016 5:28

Instrument :
BNA_G
ClientSampleId :
SB-92-22.5-23.0

Tgt Ion:152 Resp: 86284
Ion Ratio Lower Upper
152 100
150 152.1 114.0 171.0
115 70.3 48.1 72.1

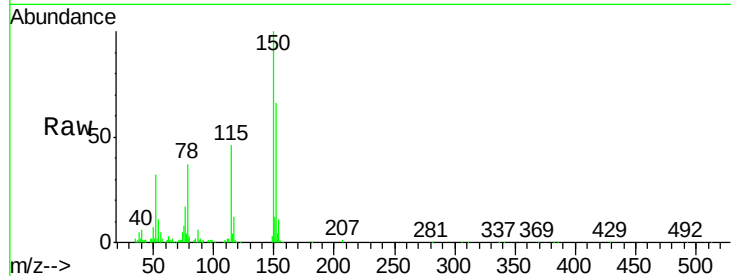


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

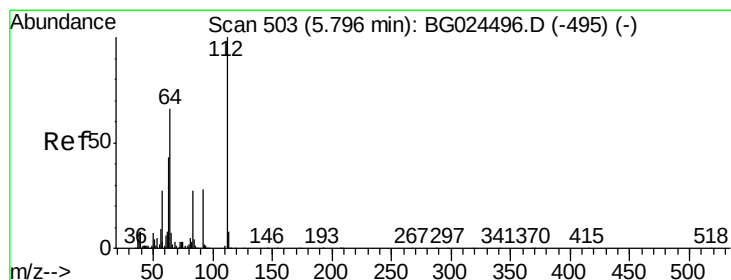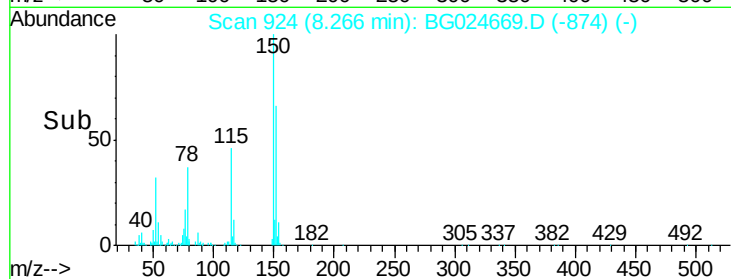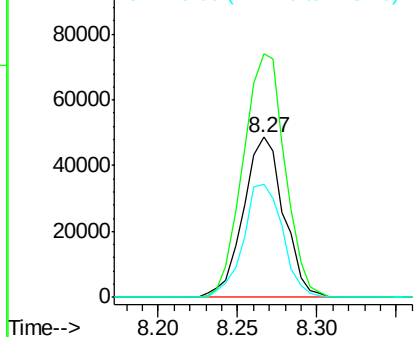



#5


2-Fluorophenol
Concen: 153.13 ng
RT: 5.80 min Scan# 504
Delta R.T. 0.00 min
Lab File: BG024669.D
Acq: 4 Nov 2016 5:28

Tgt Ion:112 Resp: 806151
Ion Ratio Lower Upper
112 100
64 69.3 61.8 92.6
63 42.4 37.2 55.8

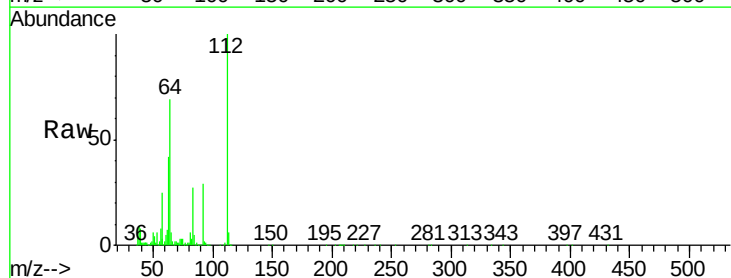

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

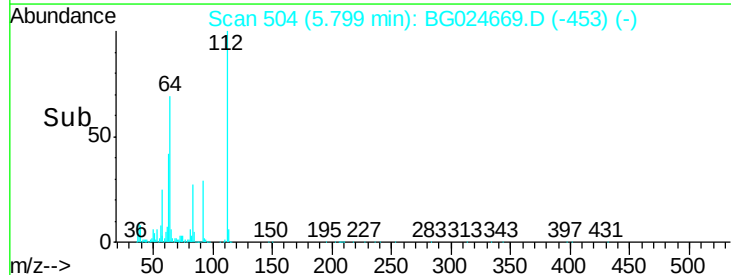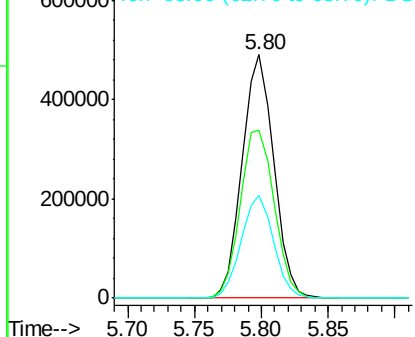

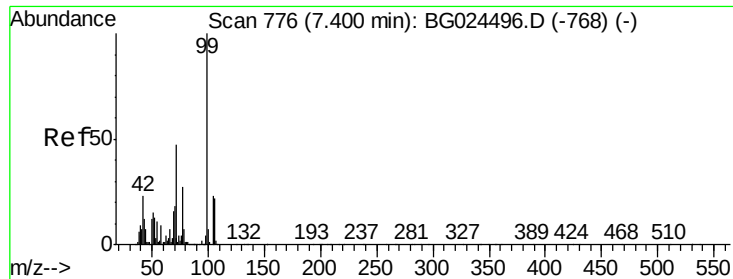

#7

Phenol-d6

Concen: 157.57 ng

RT: 7.40 min Scan# 777

Delta R.T. 0.00 min

Lab File: BG024669.D

Acq: 4 Nov 2016 5:28

Instrument :

BNA_G

ClientSampleId :

SB-92-22.5-23.0


Tgt Ion: 99 Resp: 1137873

Ion Ratio Lower Upper




99 100

42 22.2 20.5 30.7

71 47.0 37.6 56.4

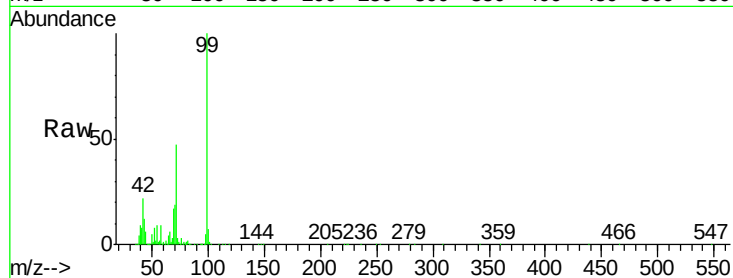

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

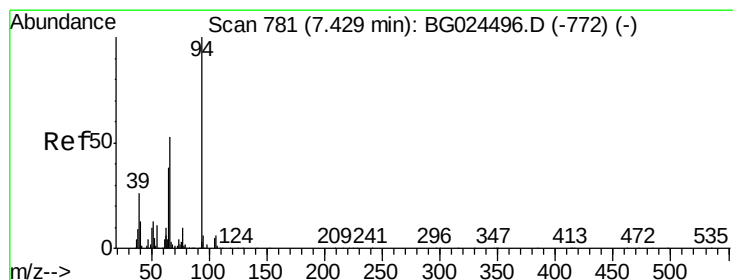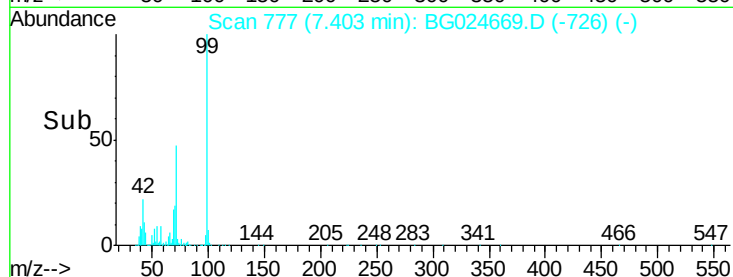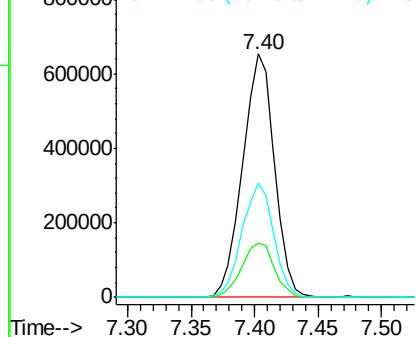

#10

Phenol

Concen: 2.46 ng

RT: 7.44 min Scan# 783

Delta R.T. 0.01 min

Lab File: BG024669.D

Acq: 4 Nov 2016 5:28


Tgt Ion: 94 Resp: 18321

Ion Ratio Lower Upper



94 100


65 32.7 20.6 60.6

66 41.6 35.5 75.5

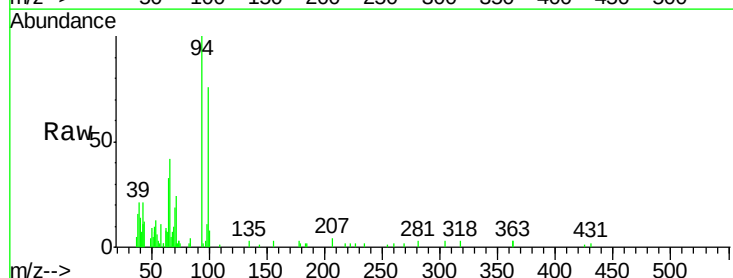

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

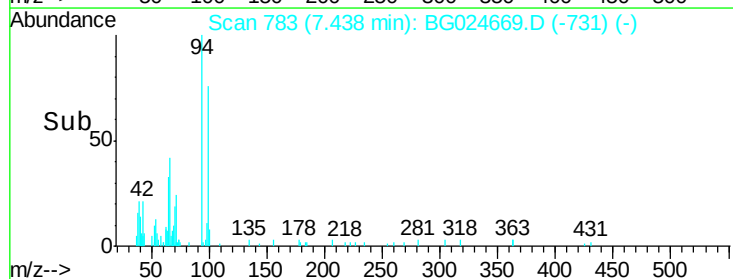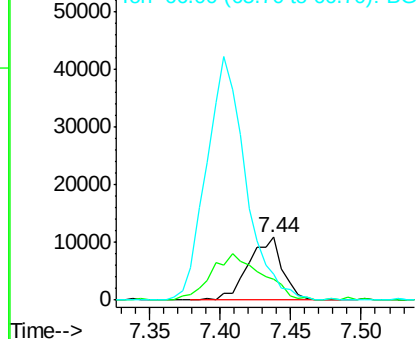

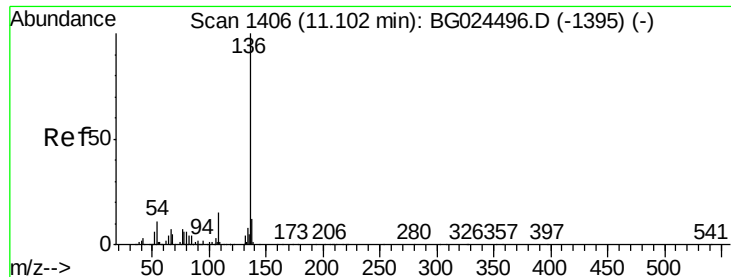

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.09 min Scan# 1405

Delta R.T. -0.01 min

Lab File: BG024669.D

Acq: 4 Nov 2016 5:28

Instrument :

BNA_G

ClientSampleId :

SB-92-22.5-23.0

Tgt Ion: 136 Resp: 345545


Ion Ratio Lower Upper

136 100

137 11.4 8.9 13.3

54 12.2 9.3 13.9

68 5.2 5.1 7.7



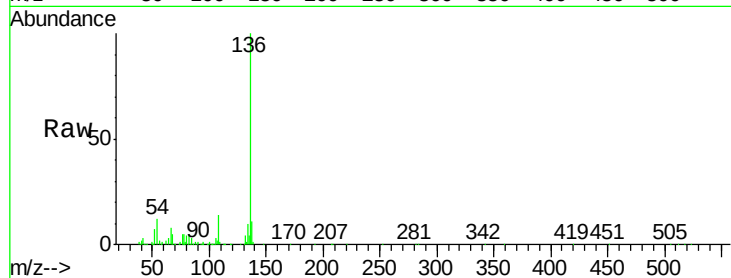


Abundance Ion 136.00 (135.70 to 136.70): B

Ion 137.00 (136.70 to 137.70): B

Ion 54.00 (53.70 to 54.70): B

Ion 68.00 (67.70 to 68.70): B

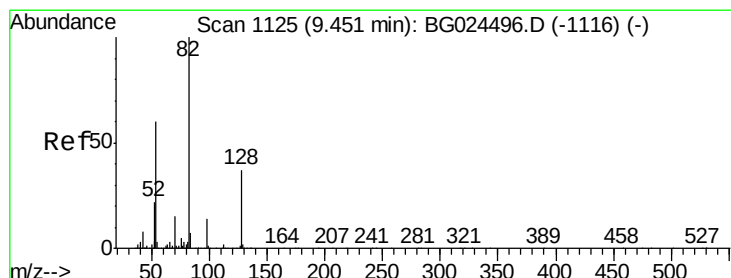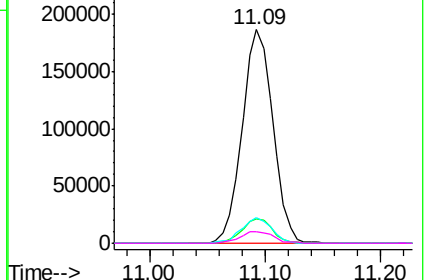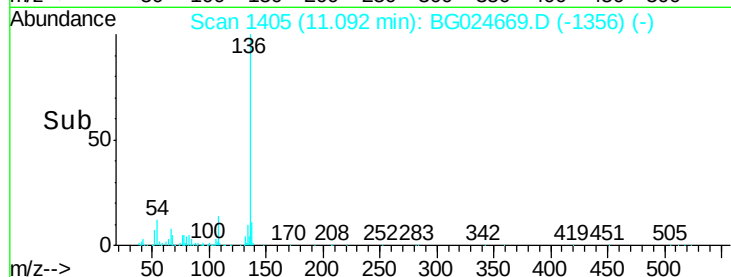

#23

Nitrobenzene-d5

Concen: 105.32 ng

RT: 9.44 min Scan# 1124

Delta R.T. -0.01 min

Lab File: BG024669.D

Acq: 4 Nov 2016 5:28


Tgt Ion: 82 Resp: 799320

Ion Ratio Lower Upper

82 100

128 35.2 26.4 39.6



54 57.2 49.4 74.2

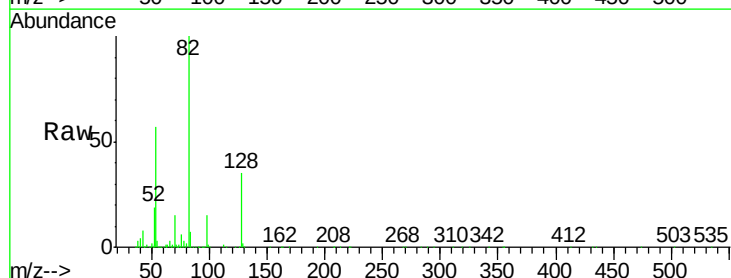


Abundance Ion 82.00 (81.70 to 82.70): B

Ion 128.00 (127.70 to 128.70): B

Ion 54.00 (53.70 to 54.70): B

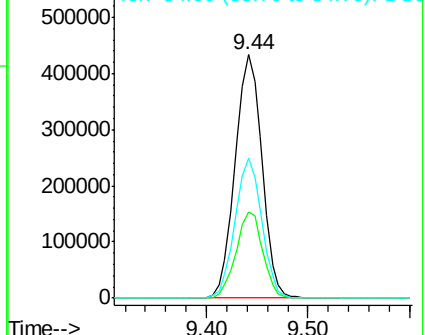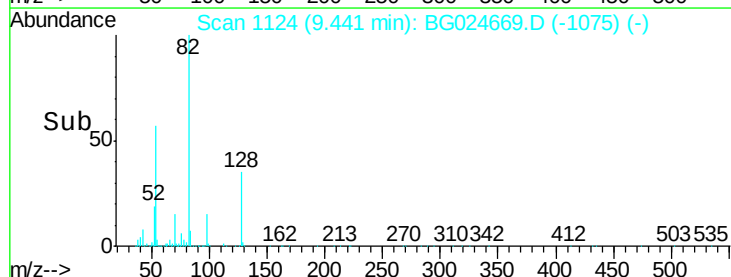

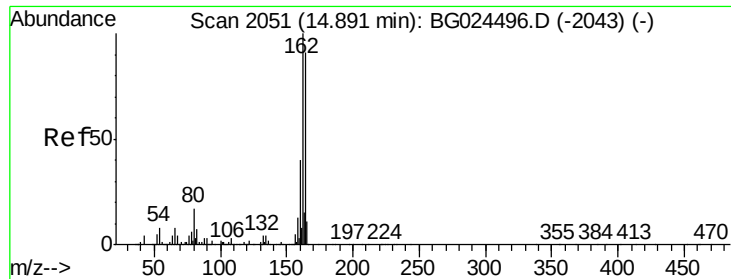

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.88 min Scan# 2050

Delta R.T. -0.01 min

Lab File: BG024669.D

Acq: 4 Nov 2016 5:28

Instrument :

BNA_G

ClientSampleId :

SB-92-22.5-23.0


Tgt Ion:164 Resp: 274656

Ion Ratio Lower Upper

164 100

162 105.0 85.1 127.7




160 40.4 34.7 52.1

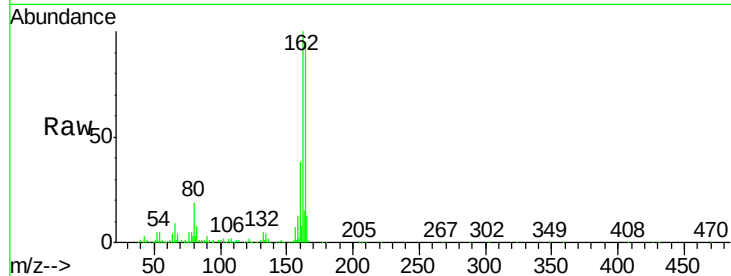

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

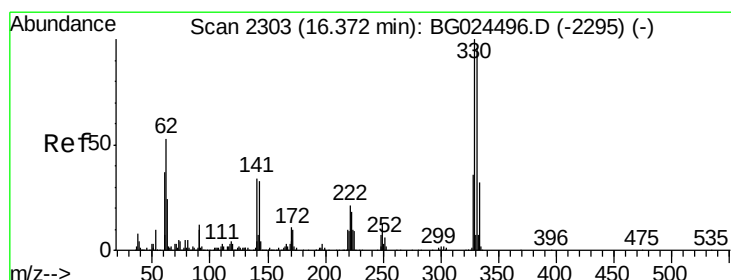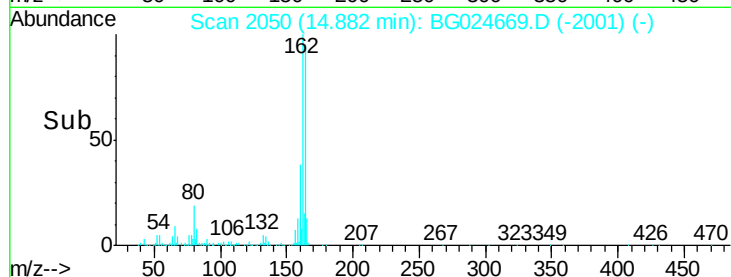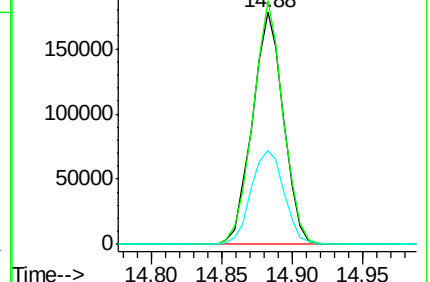

#41

2,4,6-Tribromophenol

Concen: 155.70 ng

RT: 16.37 min Scan# 2303

Delta R.T. -0.00 min

Lab File: BG024669.D

Acq: 4 Nov 2016 5:28


Tgt Ion:330 Resp: 638883

Ion Ratio Lower Upper

330 100

332 97.4 77.3 115.9

141 34.2 32.1 48.1

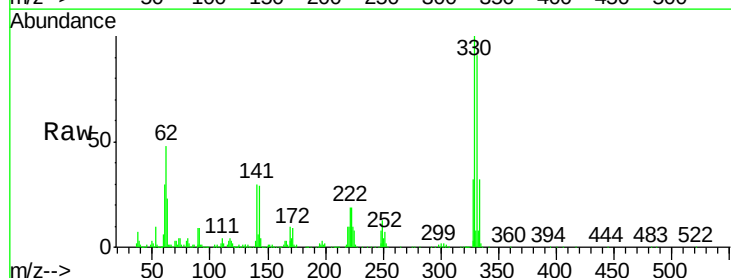

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

