





Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110316\
 Data File : BG024654.D
 Acq On : 3 Nov 2016 19:48
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 06:58:14 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration

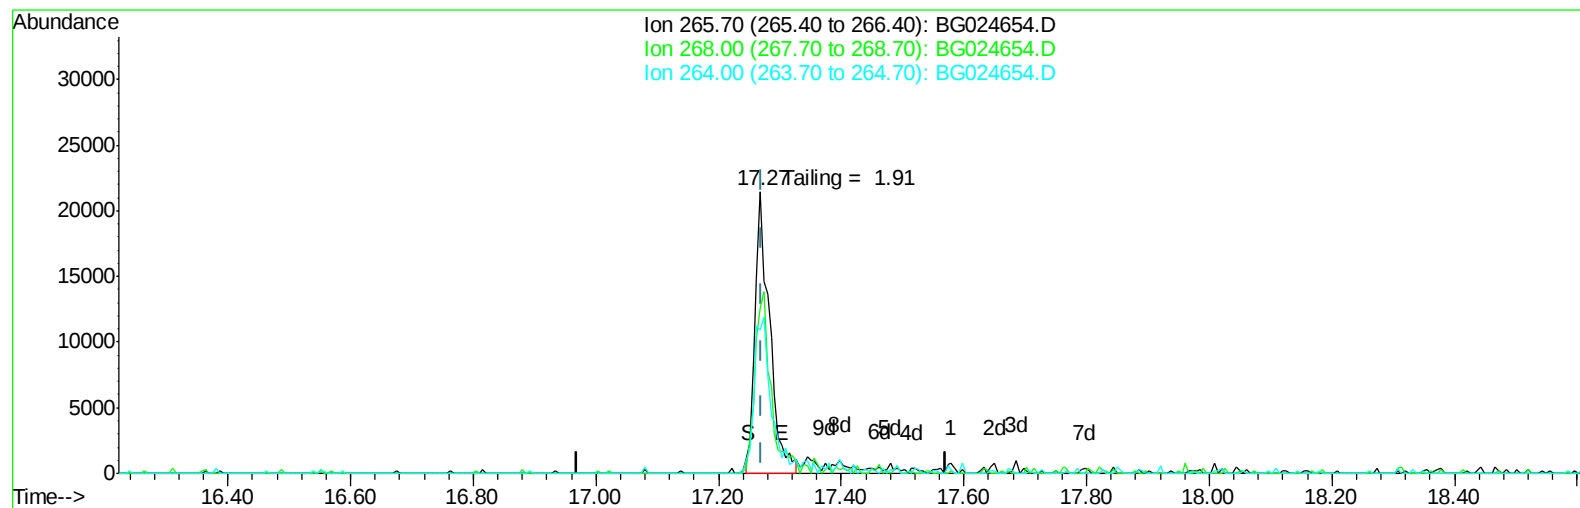

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110316\
 Data File : BG024654.D
 Acq On : 3 Nov 2016 19:48
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 06:58:14 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration

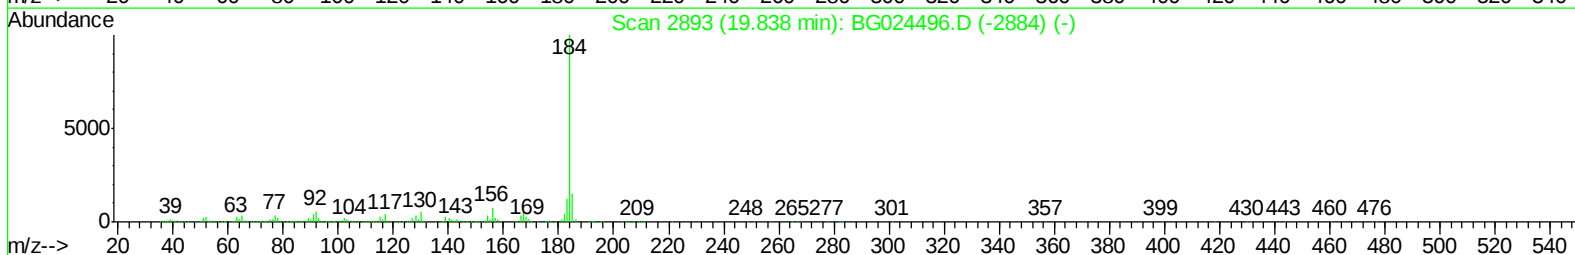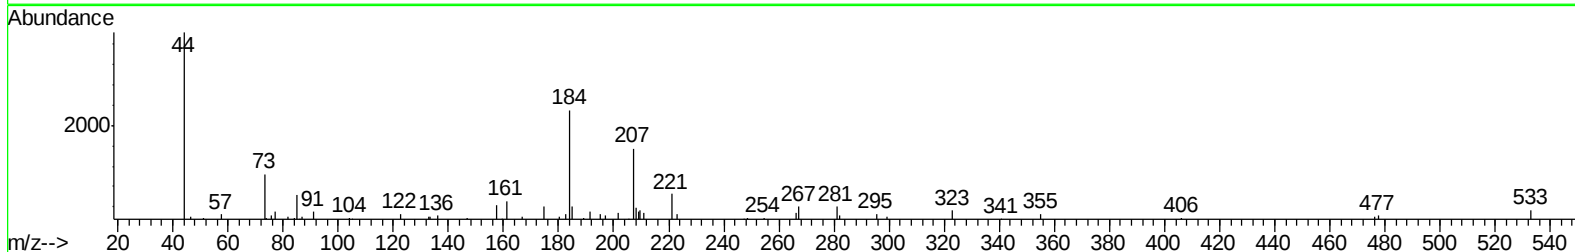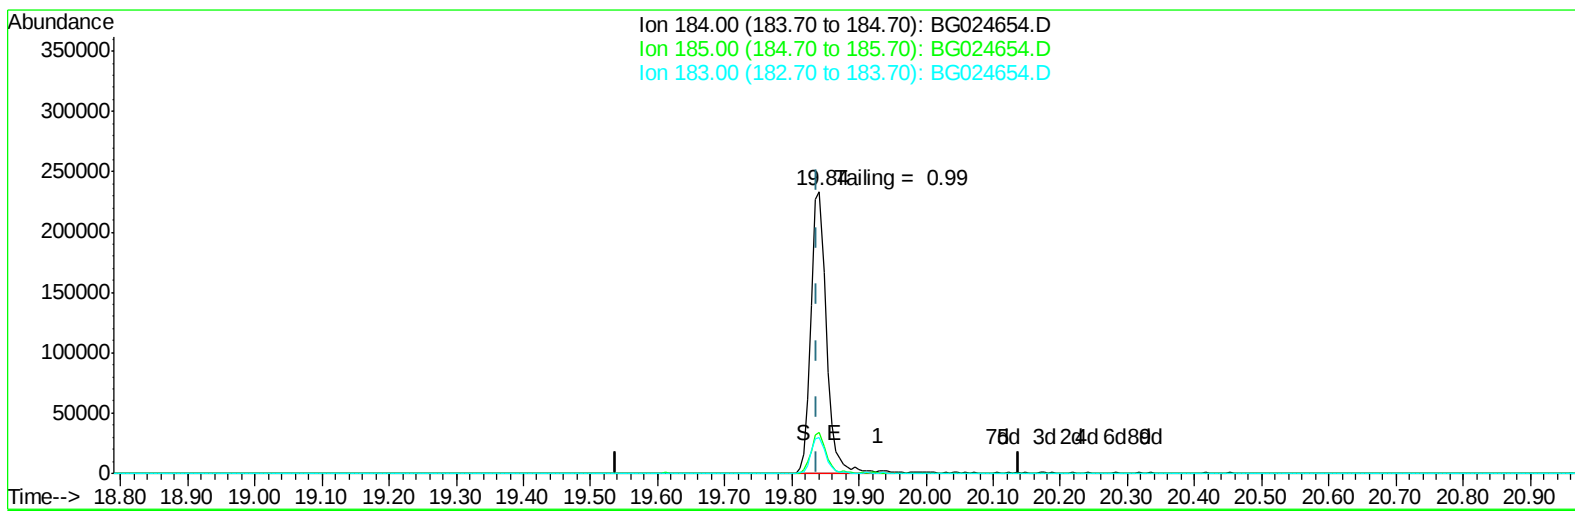

TIC: BG024654.D

(76) Benzidine

19.930min (+0.091) 715.20ng

response 3505

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	18.19
183.00	13.80	11.33
0.00	0.00	0.00