
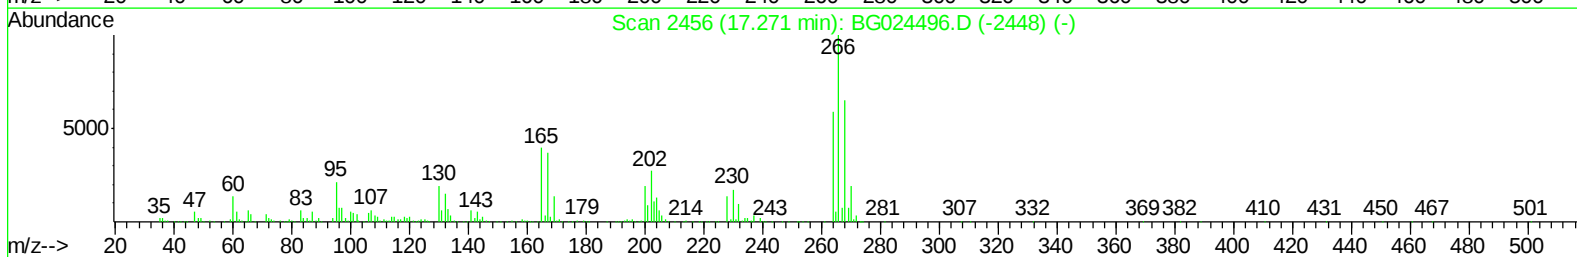
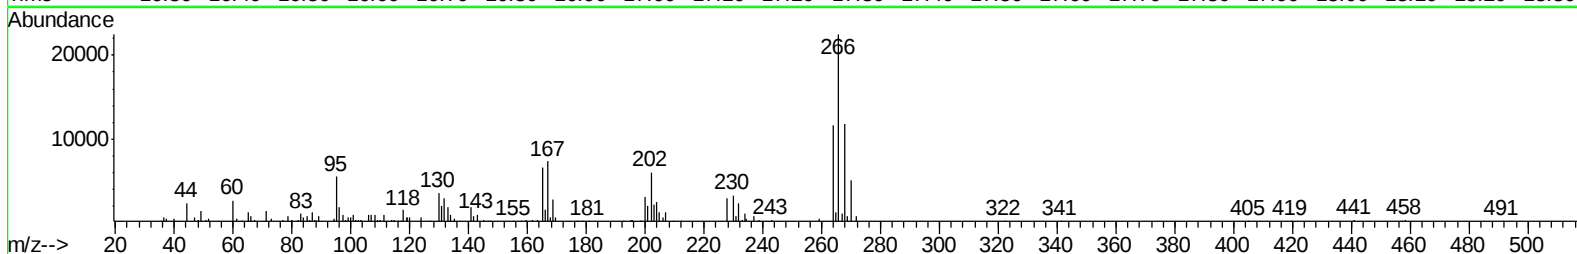


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110316\
Data File : BG024671.D
Acq On : 4 Nov 2016 7:35
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 07:19:01 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

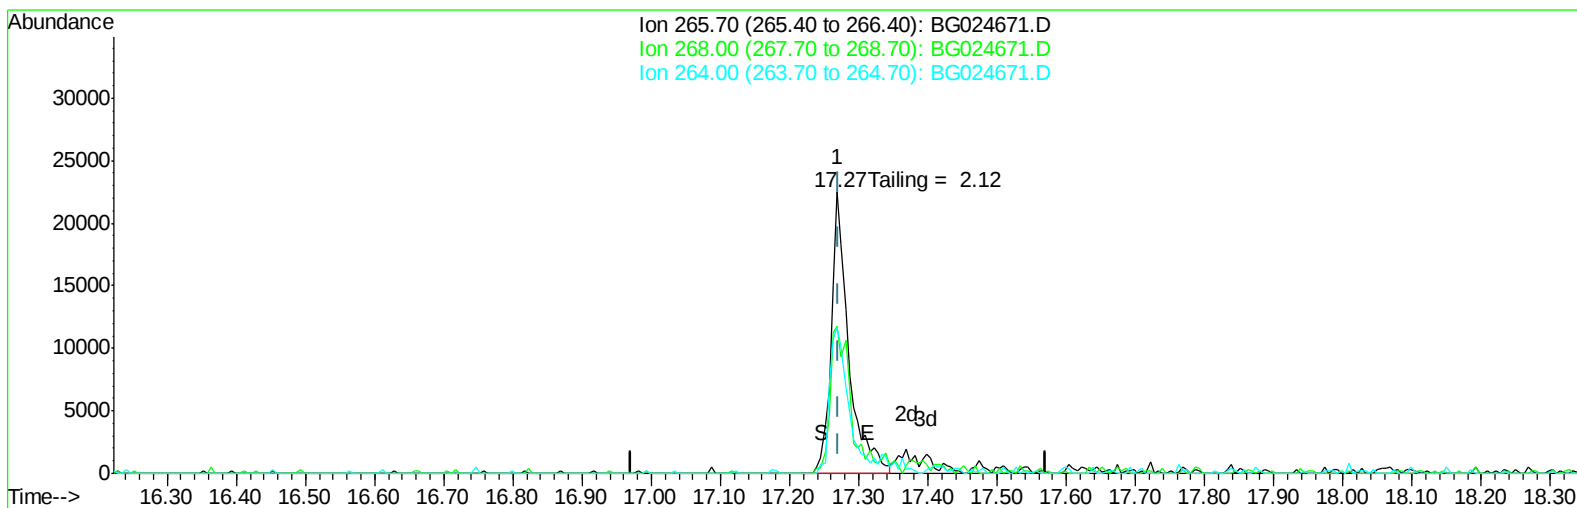

TIC: BG024671.D

(69) Pentachlorophenol (C)




17.269min (-0.002) 11267.84ng

response 39196

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	52.14
264.00	62.60	51.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110316\
Data File : BG024671.D
Acq On : 4 Nov 2016 7:35
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 07:19:01 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

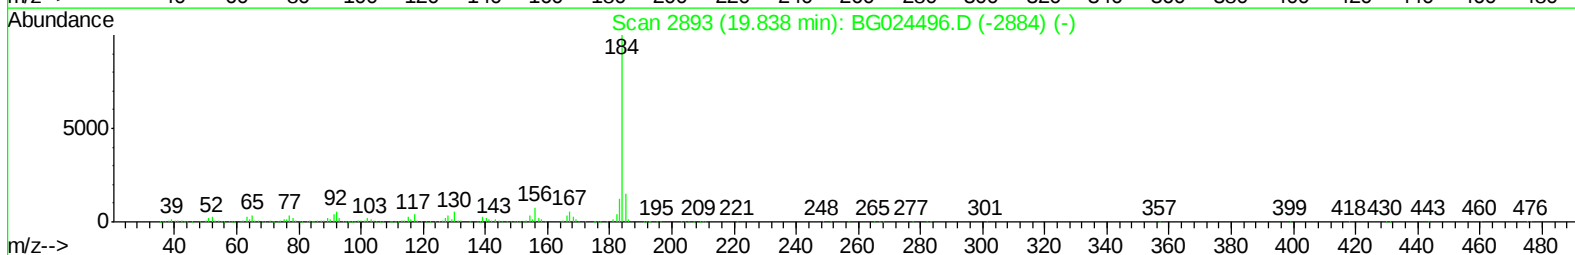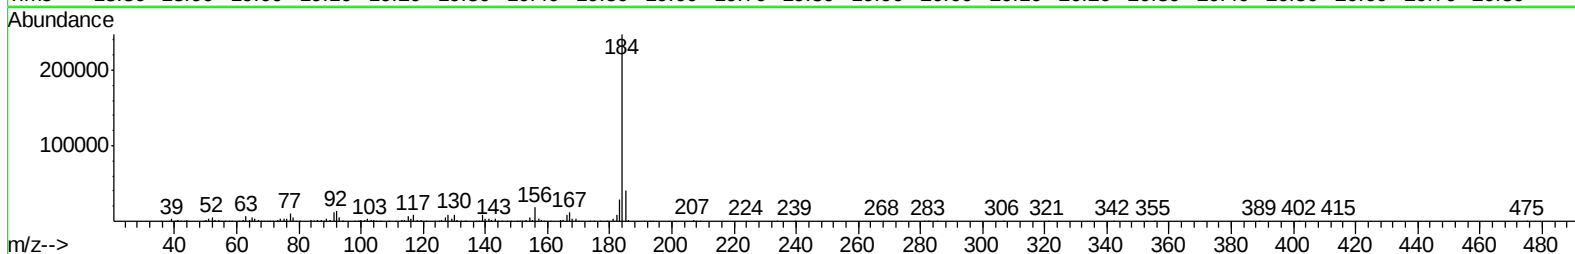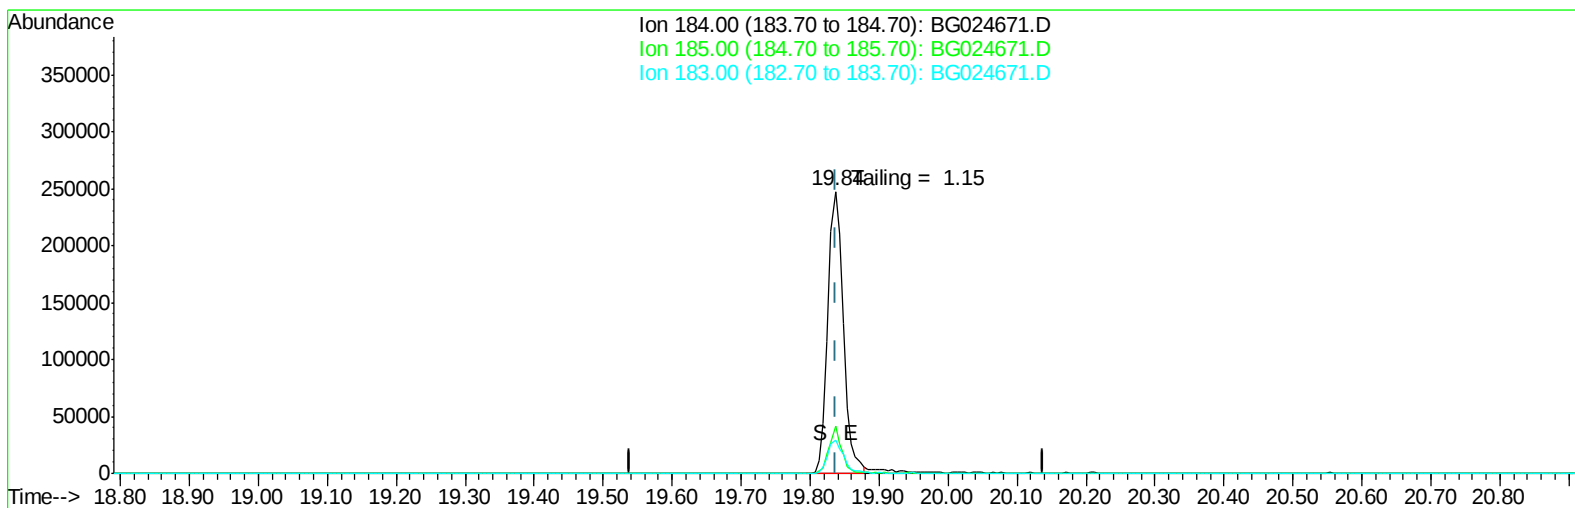

TIC: BG024671.D

(76) Benzidine

19.836min (-0.002) 129440.34ng

response 390370

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.77
183.00	13.80	11.95
0.00	0.00	0.00