

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110316\
 Data File : BG024670.D
 Acq On : 4 Nov 2016 6:06
 Operator : UM/SJ
 Sample : H5509-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-93-16.5-17.0

Quant Time: Nov 04 06:45:17 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	83342	20.00	ng	0.00
21) Naphthalene-d8	11.09	136	331879	20.00	ng	0.00
38) Acenaphthene-d10	14.88	164	255332	20.00	ng	0.00
63) Phenanthrene-d10	17.62	188	632154	20.00	ng	0.00
75) Chrysene-d12	21.92	240	837947	20.00	ng	-0.01
86) Perylene-d12	25.34	264	858609	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.80	112	790941	155.54	ng	0.00
7) Phenol-d6	7.40	99	1128296	161.76	ng	0.00
23) Nitrobenzene-d5	9.44	82	787722	108.07	ng	0.00
41) 2,4,6-Tribromophenol	16.36	330	637404	167.10	ng	0.00
44) 2-Fluorobiphenyl	13.51	172	1504102	97.91	ng	0.00
78) Terphenyl-d14	20.21	244	2707062	96.53	ng	0.00
Target Compounds						
10) Phenol	7.43	94	19658	2.73	ng	Qvalue # 81
49) Dimethylphthalate	14.32	163	524815	28.95	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110316\
Data File : BG024670.D
Acq On : 4 Nov 2016 6:06
Operator : UM/SJ
Sample : H5509-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-93-16.5-17.0

Quant Time: Nov 04 06:45:17 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

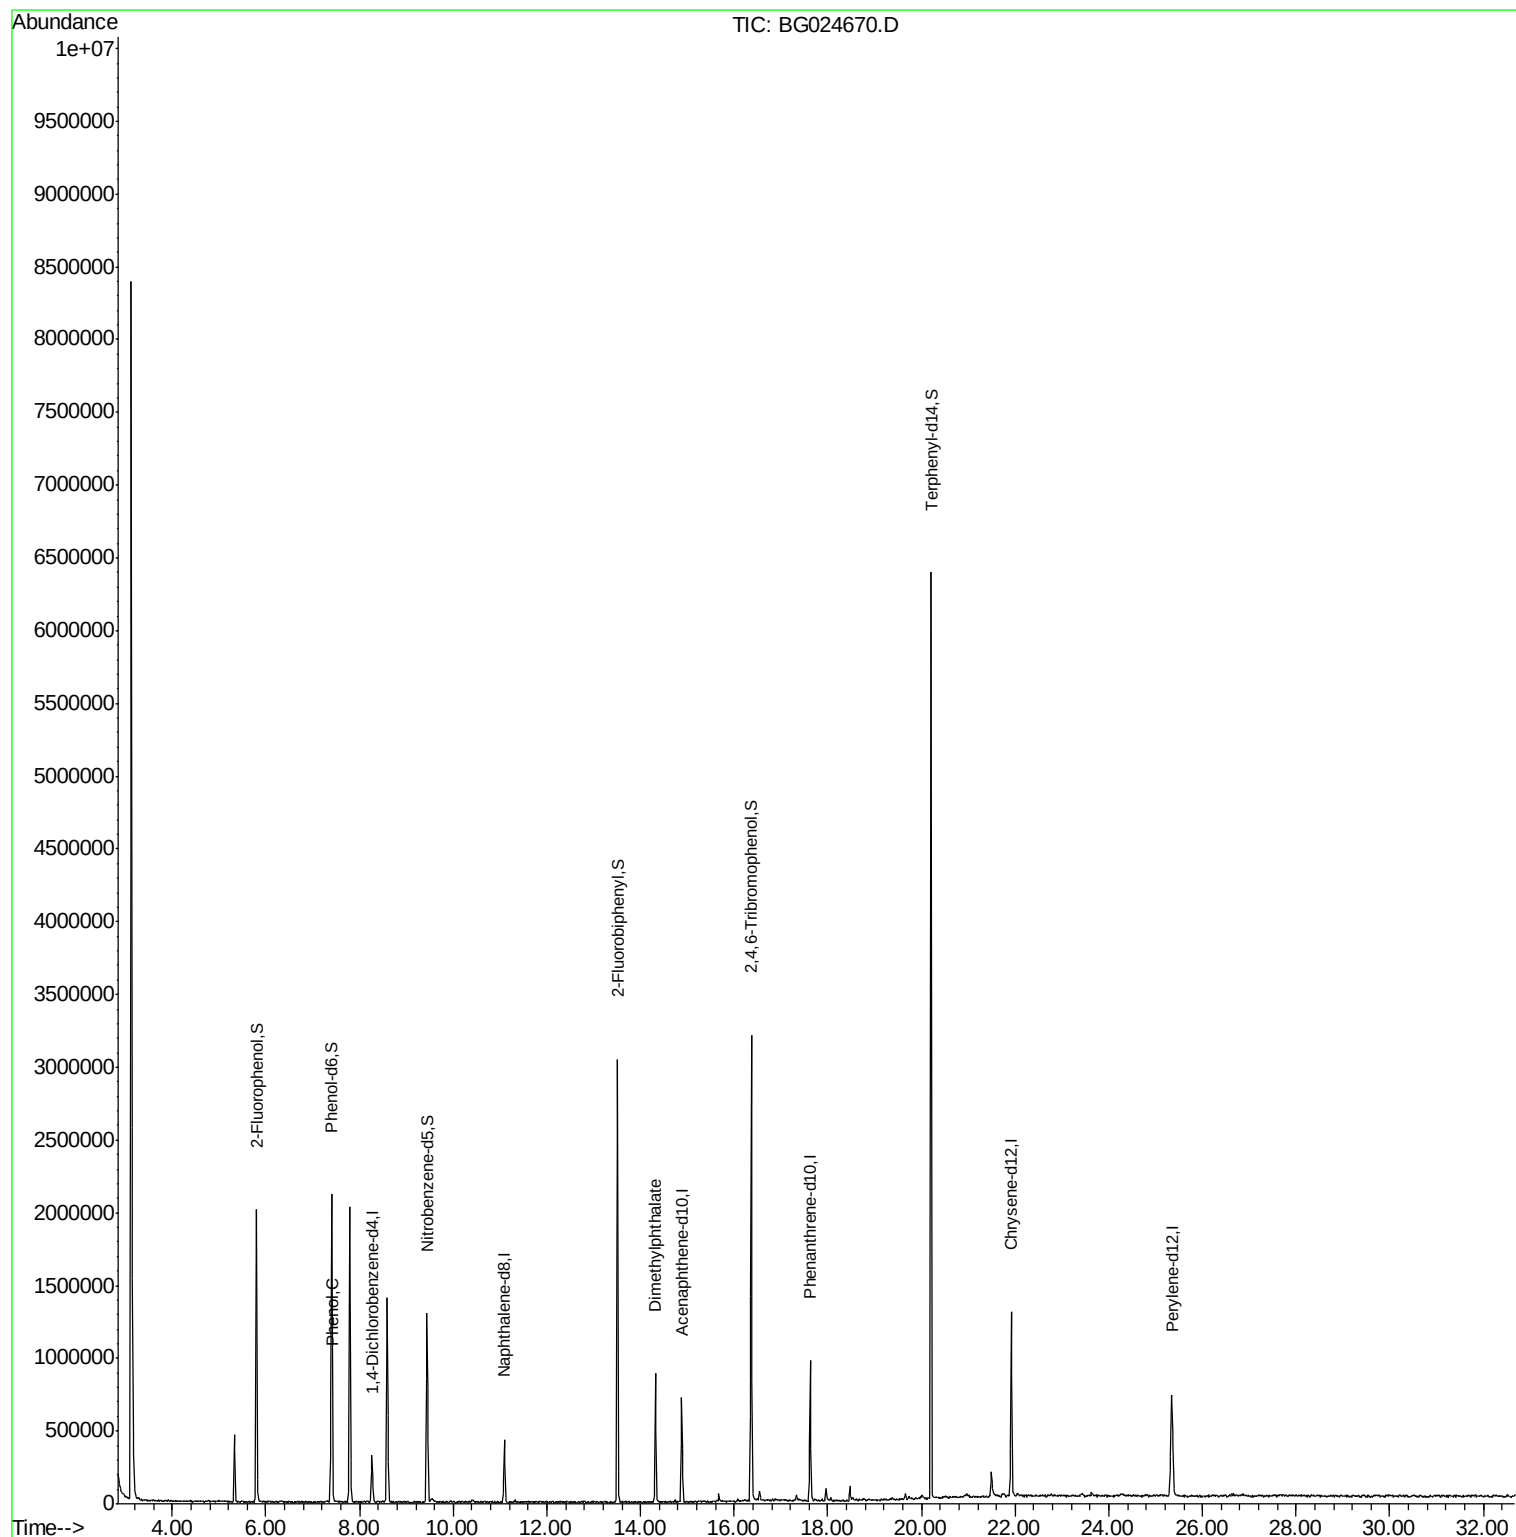

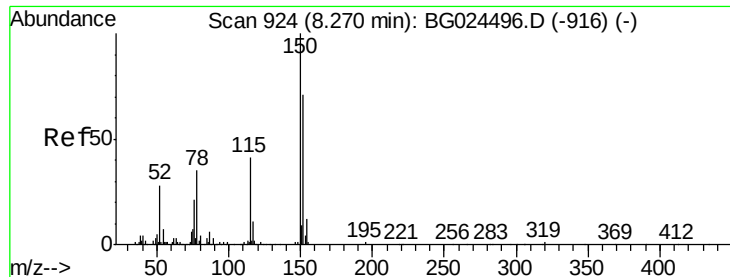

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.27 min Scan# 924

Delta R.T. -0.00 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06

Instrument :

BNA_G

ClientSampleId :

SB-93-16.5-17.0


Tgt Ion:152 Resp: 83342

Ion Ratio Lower Upper

152 100

150 172.2 114.0 171.0#




115 63.3 48.1 72.1

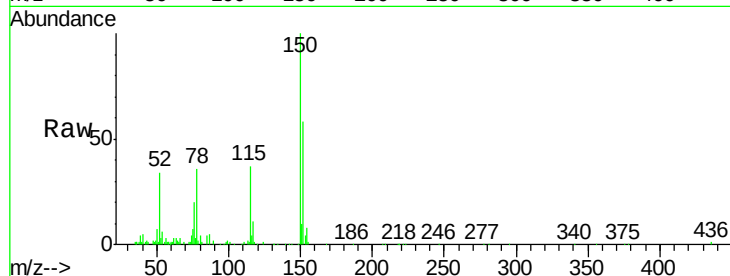

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

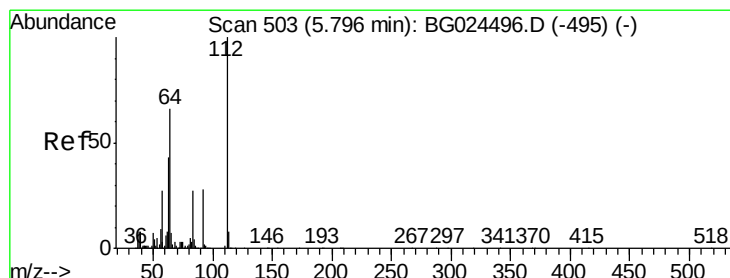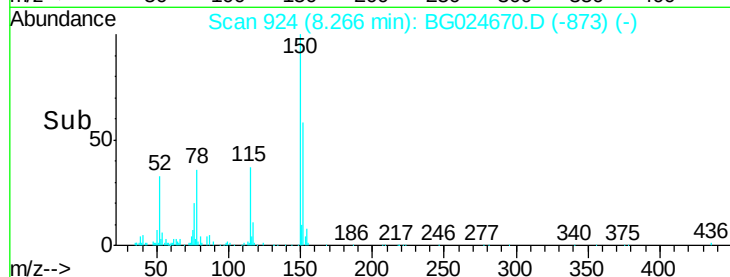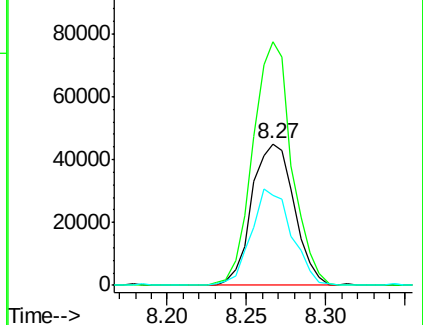

#5

2-Fluorophenol

Concen: 155.54 ng

RT: 5.80 min Scan# 504

Delta R.T. 0.00 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06


Tgt Ion:112 Resp: 790941

Ion Ratio Lower Upper

112 100

64 73.5 61.8 92.6



63 44.9 37.2 55.8

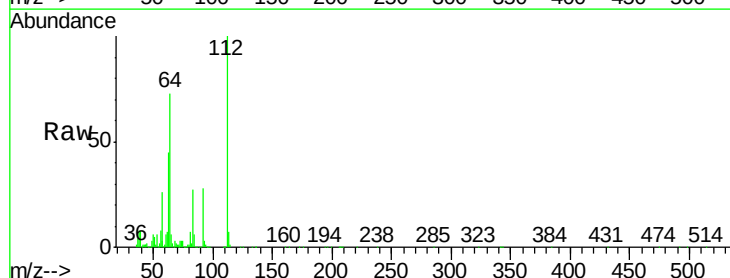


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

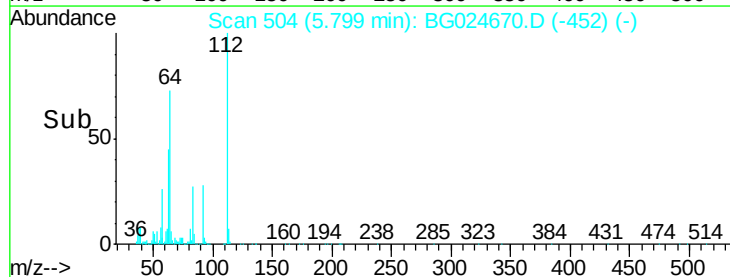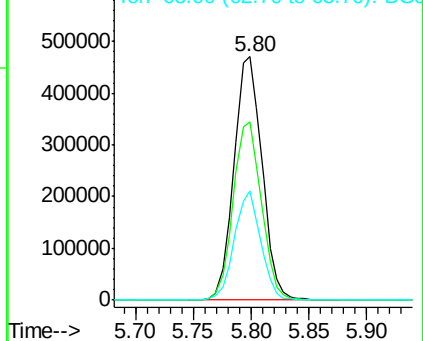

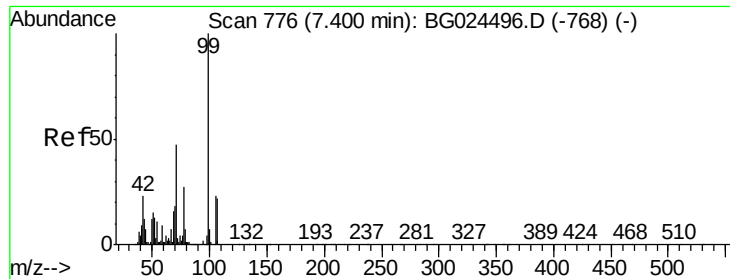

#7

Phenol-d6

Concen: 161.76 ng

RT: 7.40 min Scan# 777

Delta R.T. 0.00 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06

Instrument :

BNA_G

ClientSampleId :

SB-93-16.5-17.0


Tgt Ion: 99 Resp: 1128296

Ion Ratio Lower Upper




99 100

42 22.4 20.5 30.7

71 46.3 37.6 56.4

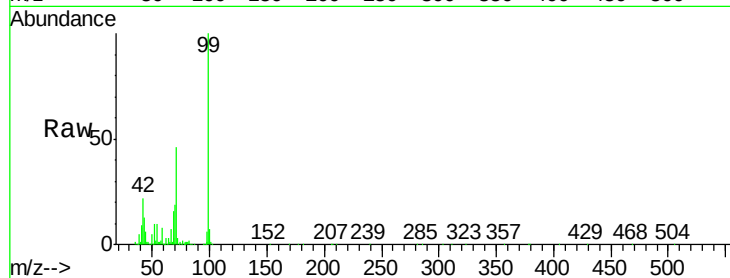

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

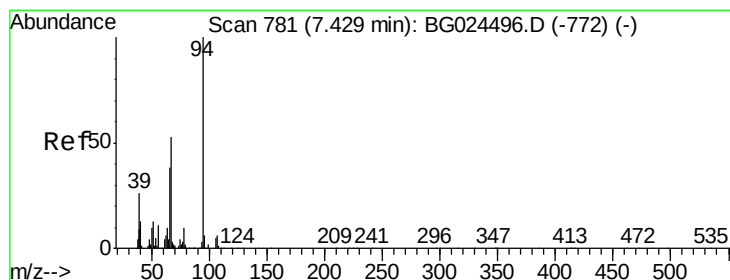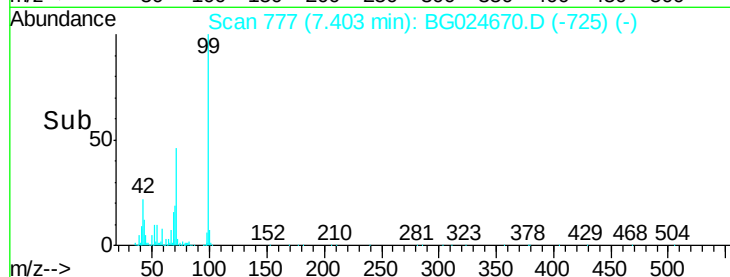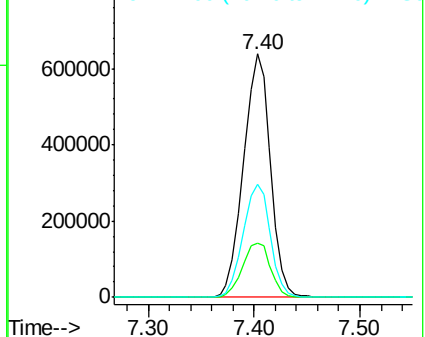

#10

Phenol

Concen: 2.73 ng

RT: 7.43 min Scan# 781

Delta R.T. -0.00 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06


Tgt Ion: 94 Resp: 19658

Ion Ratio Lower Upper



94 100


65 42.8 20.6 60.6

66 77.1 35.5 75.5#

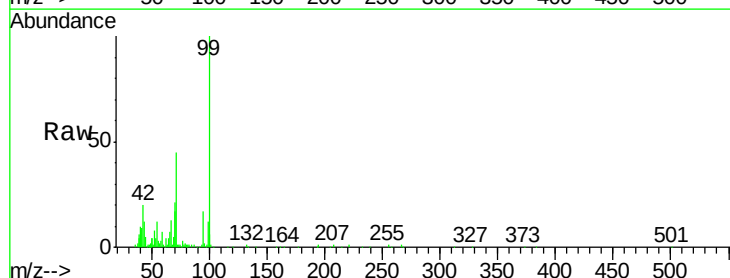

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

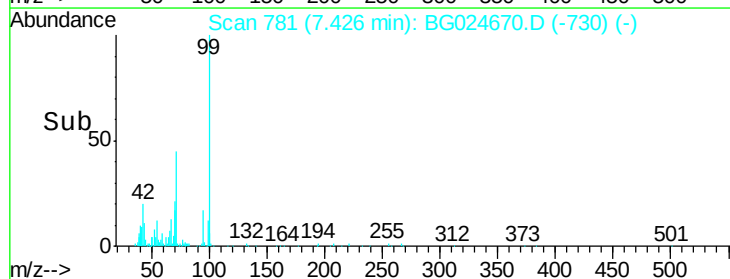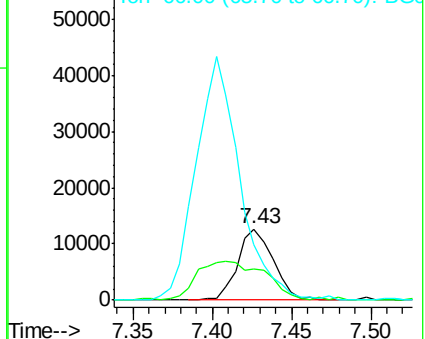







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.09 min Scan# 1405
Delta R.T. -0.01 min
Lab File: BG024670.D
Acq: 4 Nov 2016 6:06

Instrument :
BNA_G
ClientSampleId :
SB-93-16.5-17.0

Tgt Ion:	136	Resp:	331879
Ion	Ratio	Lower	Upper
136	100		
137	12.0	8.9	13.3
54	11.1	9.3	13.9
68	6.1	5.1	7.7

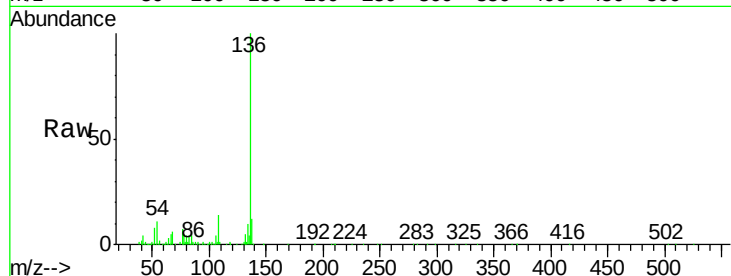


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

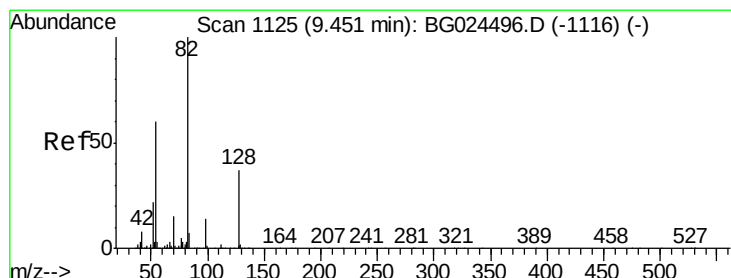
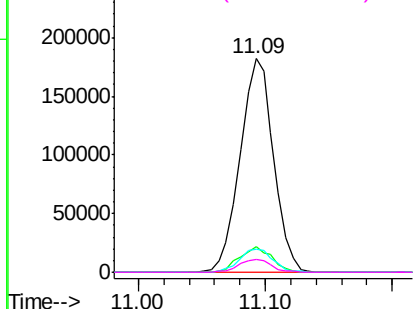



#23
Nitrobenzene-d5
Concen: 108.07 ng
RT: 9.44 min Scan# 1124
Delta R.T. -0.01 min
Lab File: BG024670.D
Acq: 4 Nov 2016 6:06

Tgt Ion:	82	Resp:	787722
Ion	Ratio	Lower	Upper
82	100		
128	37.1	26.4	39.6
54	60.0	49.4	74.2

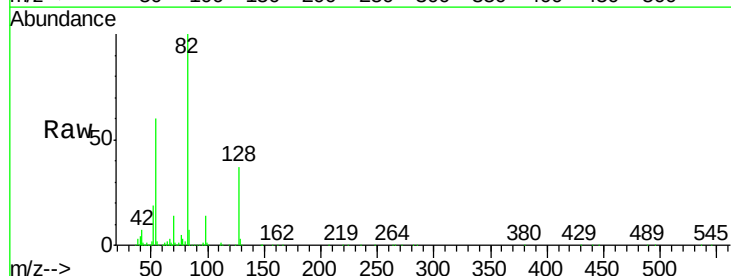

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

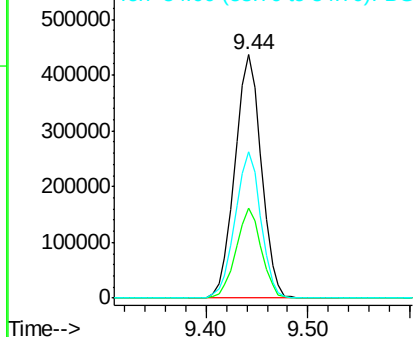



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.88 min Scan# 2050

Delta R.T. -0.01 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06

Instrument :

BNA_G

ClientSampleId :

SB-93-16.5-17.0


Tgt Ion:164 Resp: 255332

Ion Ratio Lower Upper

164 100

162 100.0 85.1 127.7




160 41.3 34.7 52.1

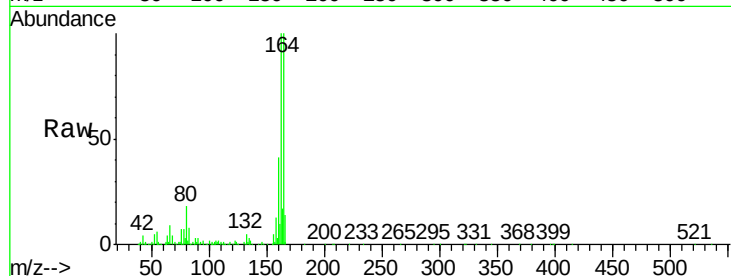

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

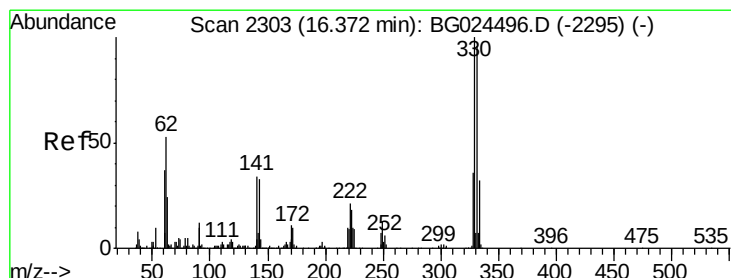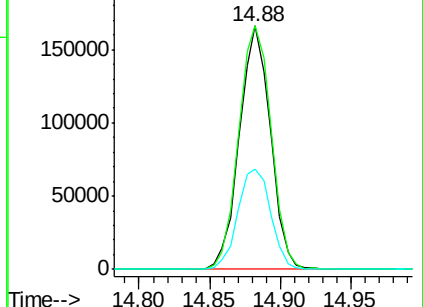

#41

2,4,6-Tribromophenol

Concen: 167.10 ng

RT: 16.36 min Scan# 2302

Delta R.T. -0.01 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06


Tgt Ion:330 Resp: 637404

Ion Ratio Lower Upper

330 100

332 95.3 77.3 115.9



141 32.9 32.1 48.1

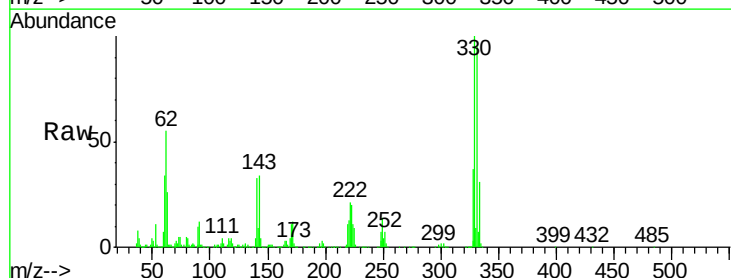


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

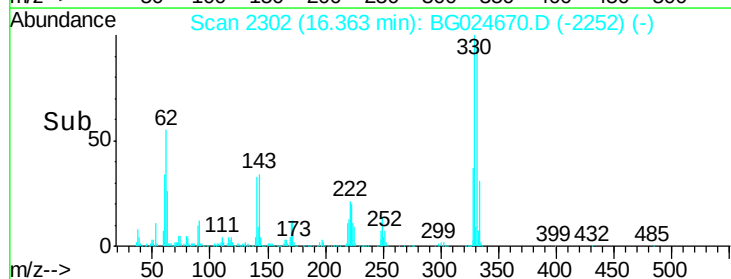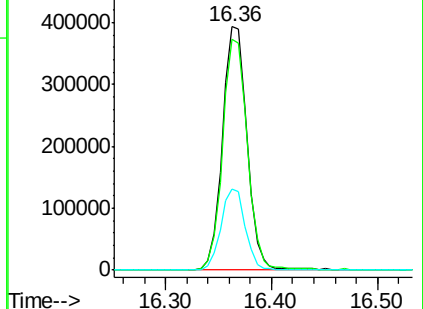

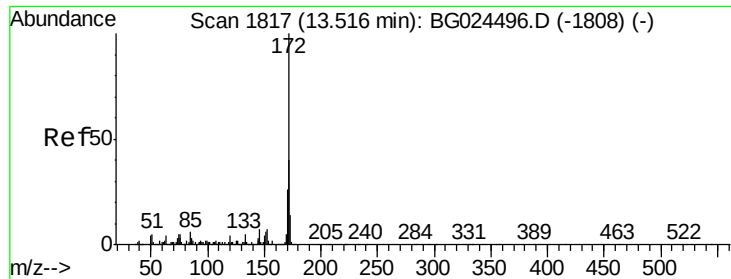

#44

2-Fluorobiphenyl

Concen: 97.91 ng

RT: 13.51 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06

Instrument :

BNA_G

ClientSampleId :

SB-93-16.5-17.0


Tgt Ion:172 Resp: 1504102

Ion Ratio Lower Upper

172 100

171 38.2 32.2 48.2




170 26.4 21.8 32.6

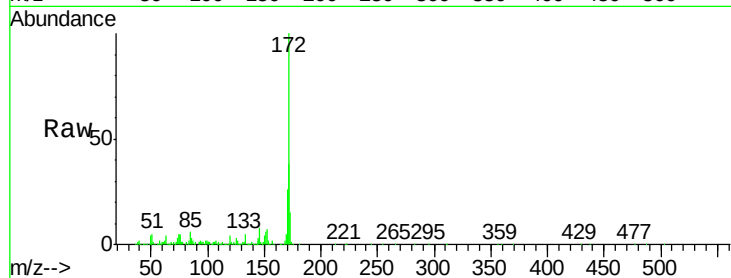

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

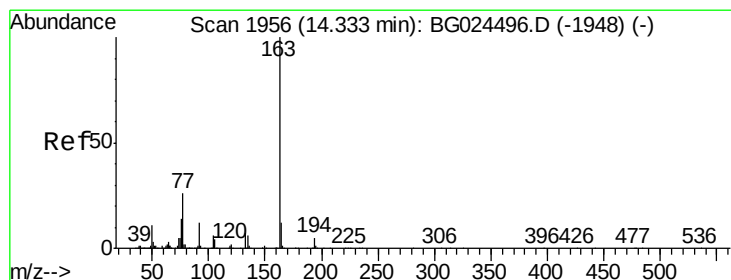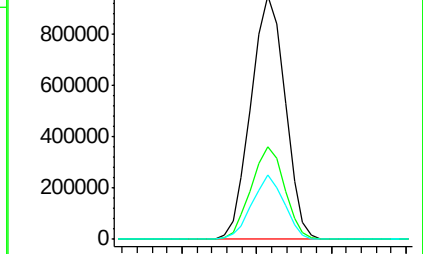

#49

Dimethylphthalate

Concen: 28.95 ng

RT: 14.32 min Scan# 1954

Delta R.T. -0.01 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06


Tgt Ion:163 Resp: 524815

Ion Ratio Lower Upper

163 100

194 5.4 3.8 5.6



164 10.6 9.3 13.9

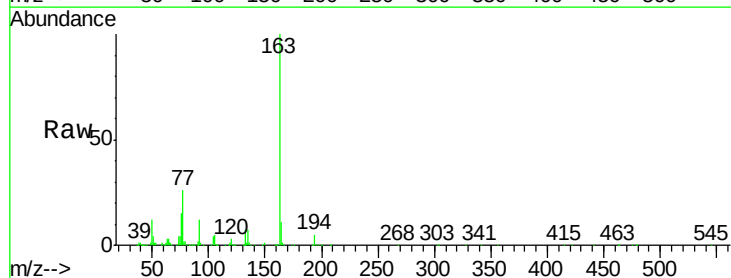


Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

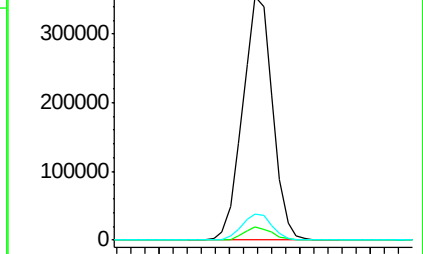



#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.62 min Scan# 2516

Delta R.T. -0.01 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06

Instrument :

BNA_G

ClientSampleId :

SB-93-16.5-17.0


Tgt Ion:188 Resp: 632154

Ion Ratio Lower Upper

188 100

94 7.2 5.8 8.8




80 7.0 7.5 11.3#

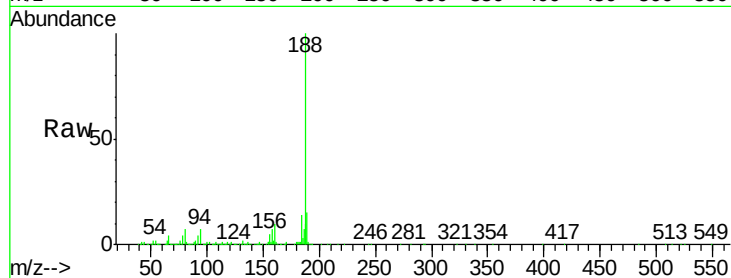

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

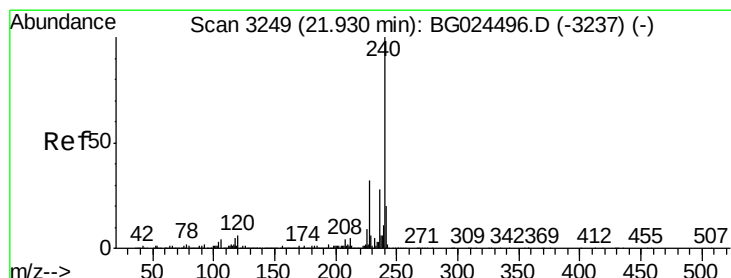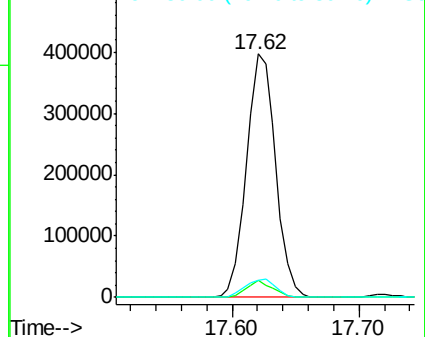

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.92 min Scan# 3247

Delta R.T. -0.01 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06


Tgt Ion:240 Resp: 837947

Ion Ratio Lower Upper

240 100

120 6.2 5.7 8.5



236 27.4 22.2 33.4

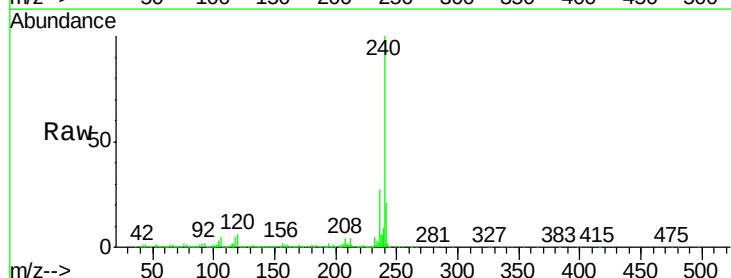


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

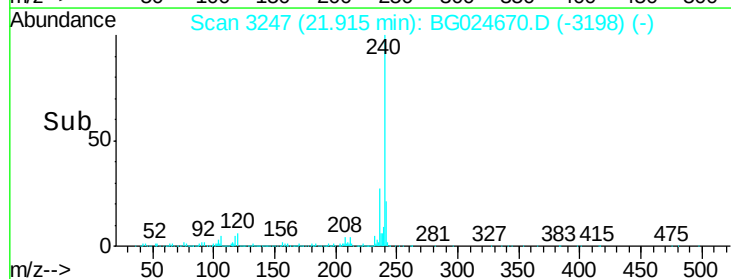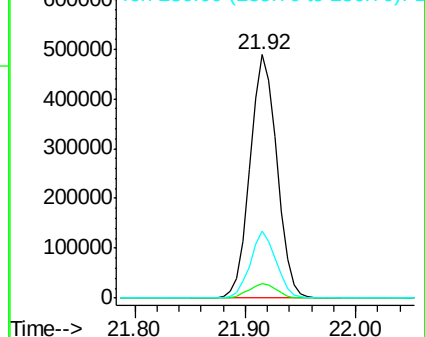

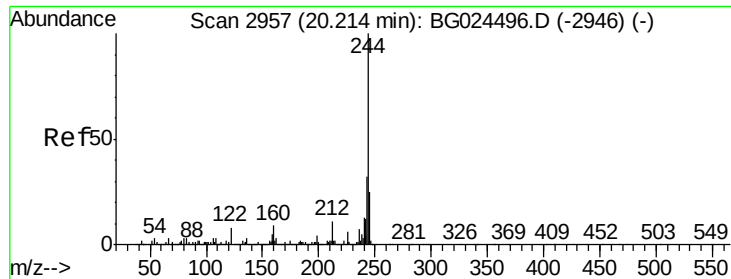

#78

Terphenyl-d14

Concen: 96.53 ng

RT: 20.21 min Scan# 2956

Delta R.T. -0.01 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06

Instrument :

BNA_G

ClientSampleId :

SB-93-16.5-17.0


Tgt Ion:244 Resp: 2707062

Ion Ratio Lower Upper

244 100

212 9.9 10.0 15.0#




122 9.1 8.6 12.8

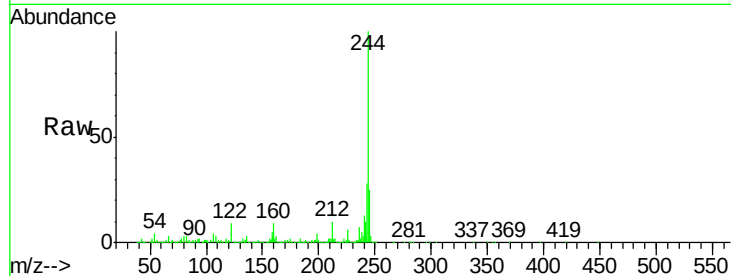

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

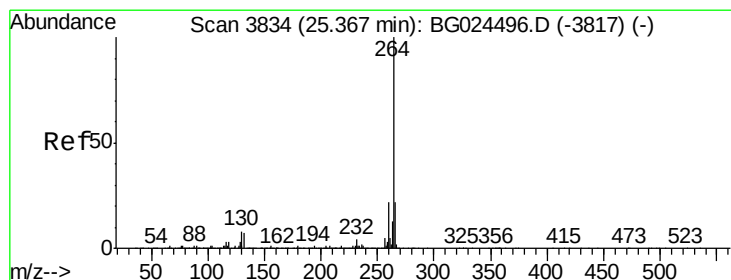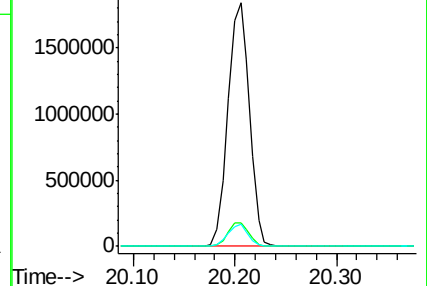

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.34 min Scan# 3830

Delta R.T. -0.03 min

Lab File: BG024670.D

Acq: 4 Nov 2016 6:06


Tgt Ion:264 Resp: 858609

Ion Ratio Lower Upper

264 100

260 23.8 21.8 32.8

265 22.4 18.2 27.4

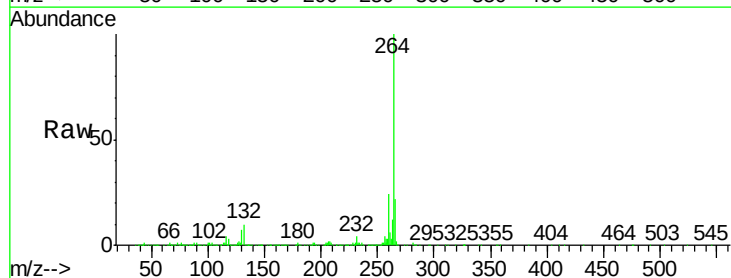

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

