

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110316\
 Data File : BG024647.D
 Acq On : 3 Nov 2016 11:16
 Operator : UM/SJ
 Sample : H5491-20
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GW-78-7.7-15.0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.332	415	424	434	rBV	564627	910428	10.46%	1.814%
2	5.796	491	503	513	rBV	876835	1551823	17.84%	3.091%
3	7.400	769	776	792	rVB	645929	1240263	14.25%	2.471%
4	7.793	836	843	851	rVB	1394539	2382537	27.38%	4.746%
5	8.269	917	924	932	rBV	458995	808510	9.29%	1.611%
6	8.592	967	979	986	rBV	1387346	2645173	30.40%	5.269%
7	9.374	1098	1112	1117	rBV5	133334	307567	3.53%	0.613%
8	9.444	1117	1124	1139	rVB	1295132	2498110	28.71%	4.976%
9	10.478	1293	1300	1308	rBV2	275751	472063	5.43%	0.940%
10	11.095	1384	1405	1411	rBV	575175	1415605	16.27%	2.820%
11	12.729	1678	1683	1689	rVB	337315	579015	6.65%	1.153%
12	12.946	1710	1720	1727	rVB	506046	935074	10.75%	1.863%
13	13.387	1790	1795	1806	rBV5	157380	337415	3.88%	0.672%
14	13.510	1808	1816	1825	rVB	3057983	4937658	56.75%	9.836%
15	13.916	1875	1885	1899	rVB4	121401	391203	4.50%	0.779%
16	14.057	1901	1909	1916	rBV3	266886	648210	7.45%	1.291%
17	14.209	1928	1935	1939	rBV	333985	629101	7.23%	1.253%
18	14.256	1939	1943	1951	rVV5	212821	527311	6.06%	1.050%
19	14.327	1951	1955	1960	rVB	252605	372256	4.28%	0.742%
20	14.444	1968	1975	1978	rBV2	260888	481617	5.54%	0.959%
21	14.609	1998	2003	2009	rVB3	161910	282882	3.25%	0.564%
22	14.885	2040	2050	2056	rBV	979137	1637214	18.82%	3.261%
23	15.085	2078	2084	2092	rBV7	113658	299935	3.45%	0.597%
24	15.267	2105	2115	2123	rBV8	191552	516644	5.94%	1.029%
25	15.343	2123	2128	2136	rBV5	198234	347000	3.99%	0.691%
26	15.484	2147	2152	2158	rBV3	192502	318094	3.66%	0.634%
27	15.661	2175	2182	2192	rBV7	123798	431316	4.96%	0.859%
28	15.925	2221	2227	2232	rBV4	126175	274334	3.15%	0.546%
29	16.084	2249	2254	2259	rVB2	237511	432177	4.97%	0.861%
30	16.366	2296	2302	2309	rBV	2292577	3665846	42.13%	7.303%
31	16.560	2329	2335	2350	rVB2	295805	692515	7.96%	1.380%
32	17.382	2471	2475	2481	rVB3	215666	354340	4.07%	0.706%
33	17.629	2510	2517	2522	rBV	1270026	2054952	23.62%	4.094%
34	18.475	2657	2661	2667	rBV5	147455	323383	3.72%	0.644%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110316\
Data File : BG024647.D
Acq On : 3 Nov 2016 11:16
Operator : UM/SJ
Sample : H5491-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-78-7.7-15.0

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	20.208	2949	2956	2968	rVB	6089015	8700737	100.00%	17.333%
36	21.924	3240	3248	3255	rBV	1579720	2826217	32.48%	5.630%
37	25.349	3820	3831	3851	rVB2	893597	2969856	34.13%	5.916%




Sum of corrected areas: 50198381

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110316\
Data File : BG024647.D
Acq On : 3 Nov 2016 11:16
Operator : UM/SJ
Sample : H5491-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-78-7.7-15.0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: rteint.p

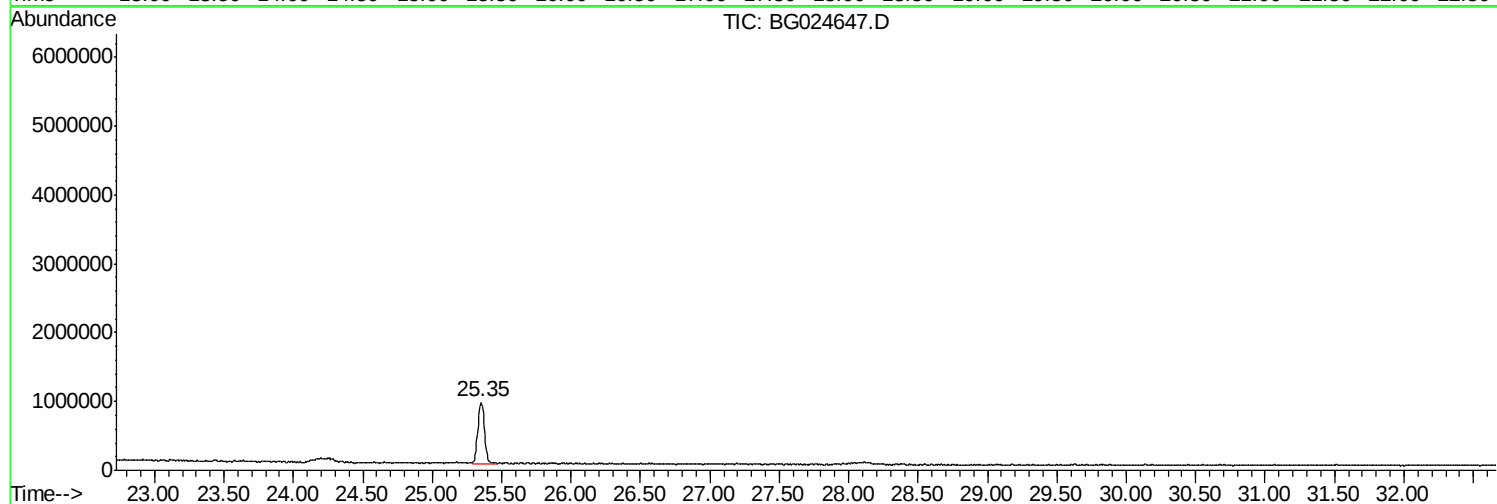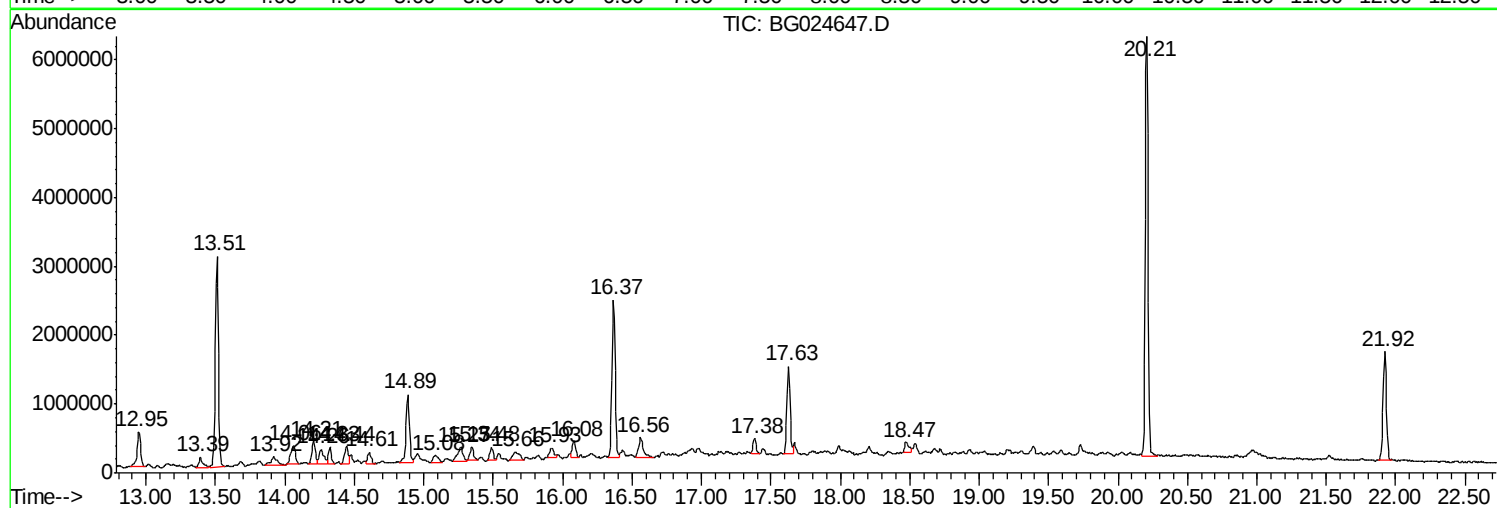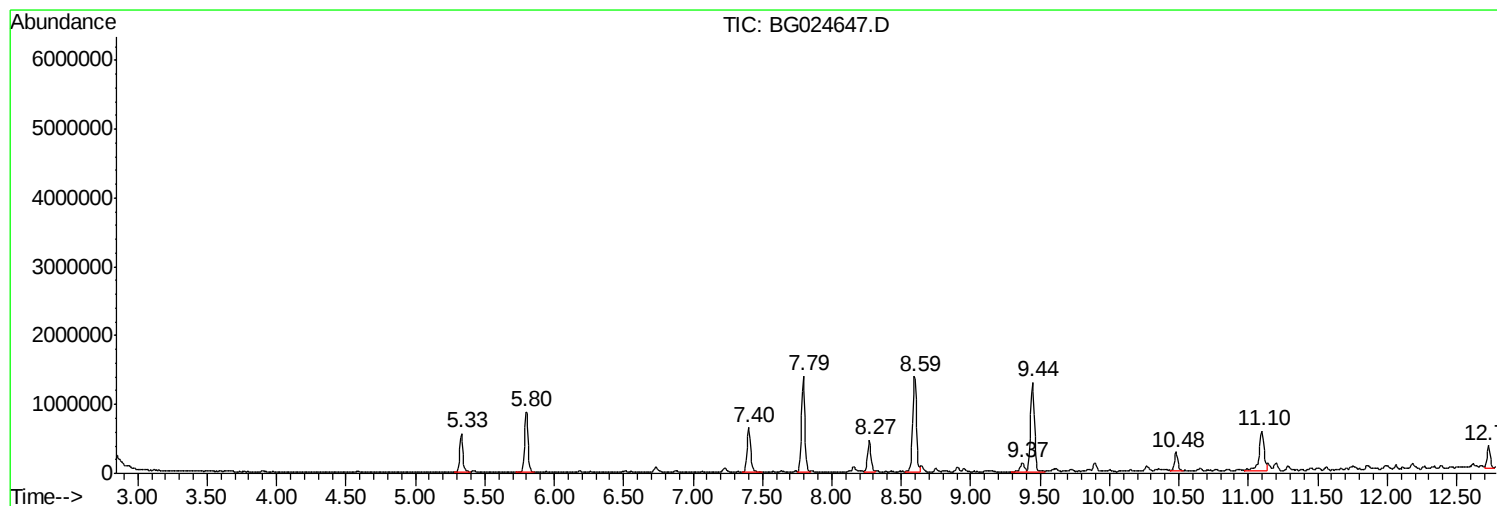

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110316\
Data File : BG024647.D
Acq On : 3 Nov 2016 11:16
Operator : UM/SJ
Sample : H5491-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-78-7.7-15.0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110316\
Data File : BG024647.D
Acq On : 3 Nov 2016 11:16
Operator : UM/SJ
Sample : H5491-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-78-7.7-15.0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc