


Data Path : Z:\HPCHEM1\BNA_G\Data\BG110316\
Data File : BG024645.D
Acq On : 3 Nov 2016 9:52
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 26 11:14:13 2016

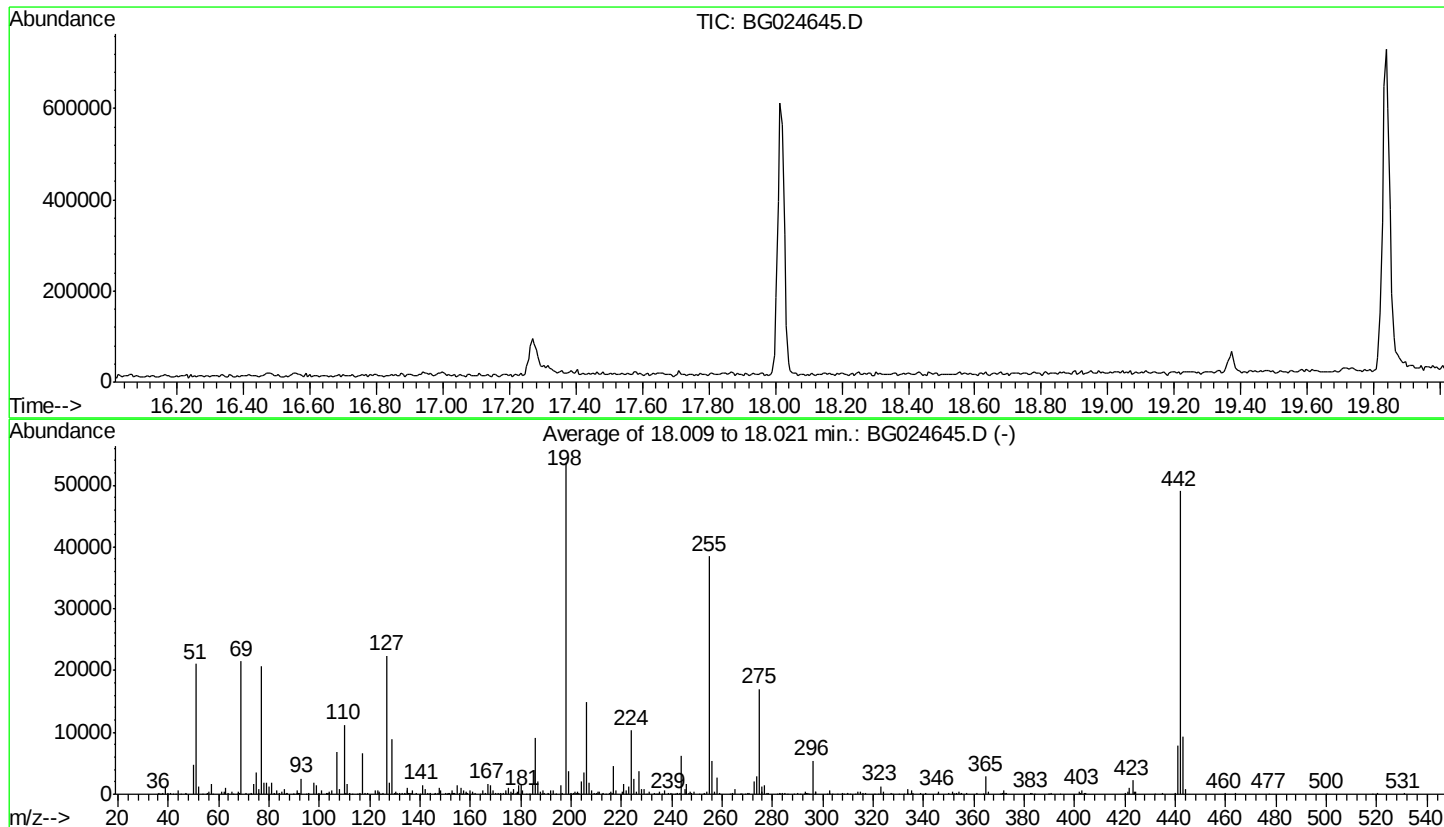

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	21067	PASS
68	69	0.00	2	1.8	389	PASS
69	198	0.00	100	40.1	21498	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.7	22373	PASS
197	198	0.00	2	0.2	128	PASS
198	198	100	100	100.0	53629	PASS
199	198	5	9	6.9	3688	PASS
275	198	10	60	31.8	17078	PASS
365	198	1	100	5.3	2836	PASS
441	442	0.01	24	15.9	7772	PASS
442	198	50	100	91.3	48976	PASS
443	442	15	24	18.9	9261	PASS