


Data Path : Z:\HPCHEM1\BNA_G\Data\BG110316\
 Data File : BG024654.D
 Acq On : 3 Nov 2016 19:48
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

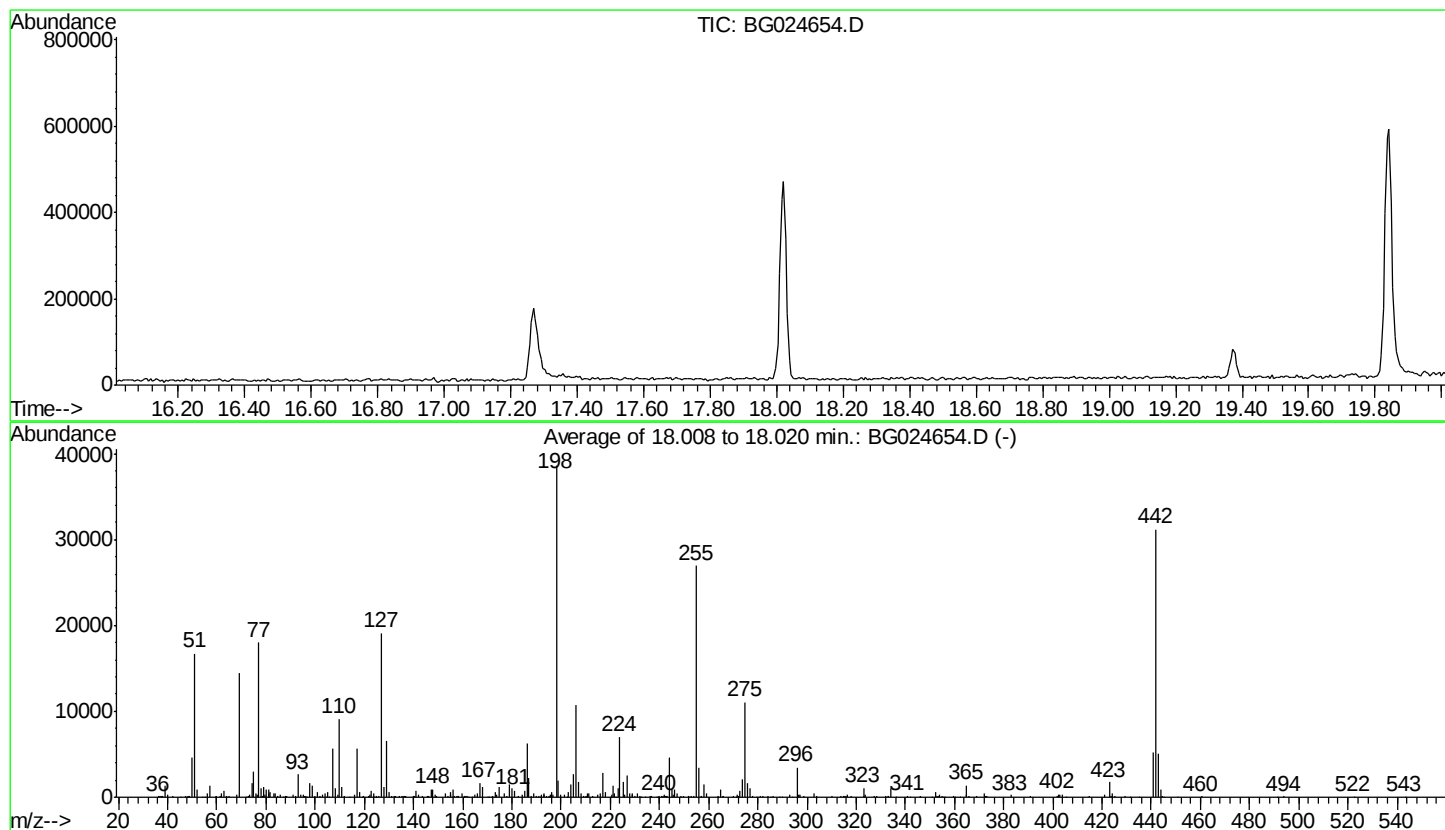

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	16725	PASS
68	69	0.00	2	1.7	248	PASS
69	198	0.00	100	37.6	14519	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	19080	PASS
197	198	0.00	2	0.8	318	PASS
198	198	100	100	100.0	38594	PASS
199	198	5	9	5.1	1978	PASS
275	198	10	60	28.6	11035	PASS
365	198	1	100	3.6	1400	PASS
441	442	0.01	24	16.7	5214	PASS
442	198	50	100	80.8	31179	PASS
443	442	15	24	16.4	5123	PASS