


Data Path : Z:\HPCHEM1\BNA_G\Data\BG110316\
 Data File : BG024671.D
 Acq On : 4 Nov 2016 7:35
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

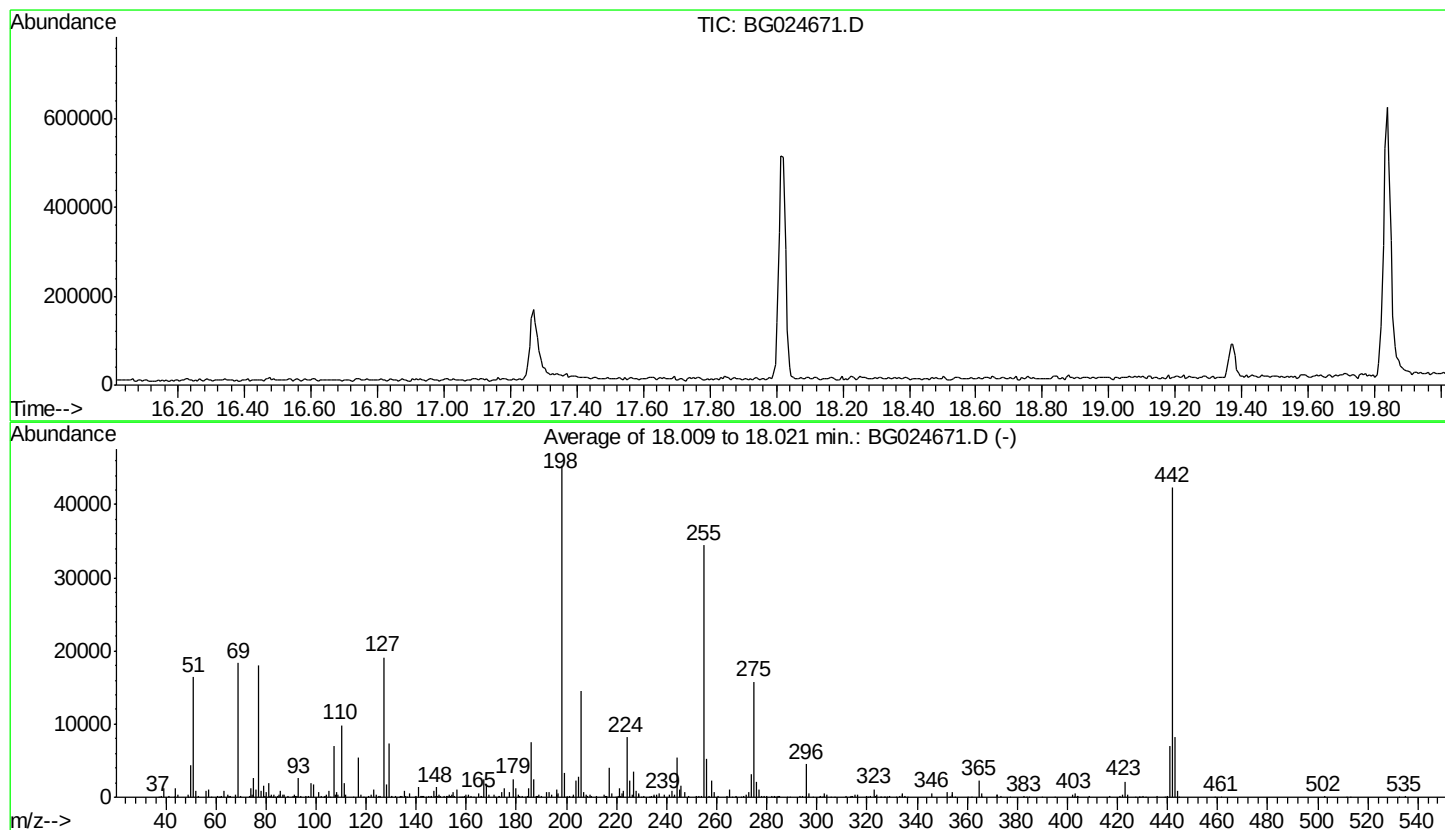

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	16398	PASS
68	69	0.00	2	1.8	324	PASS
69	198	0.00	100	40.4	18340	PASS
70	69	0.00	2	1.1	193	PASS
127	198	10	80	42.1	19088	PASS
197	198	0.00	2	1.0	454	PASS
198	198	100	100	100.0	45341	PASS
199	198	5	9	7.5	3381	PASS
275	198	10	60	34.8	15775	PASS
365	198	1	100	4.9	2213	PASS
441	442	0.01	24	16.4	6933	PASS
442	198	50	100	93.3	42320	PASS
443	442	15	24	19.4	8202	PASS