

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050818.D
 Acq On : 2 Nov 2021 15:36
 Operator : CG/JU
 Sample : PB140311BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK311

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.584	13	16	25	rVB2	8915	15156	1.50%	0.137%
2	4.013	84	89	104	rBV	109819	201611	19.91%	1.818%
3	4.359	143	148	153	rVB3	2319	3679	0.36%	0.033%
4	4.571	180	184	187	rBV2	1092	1488	0.15%	0.013%
5	4.982	249	254	256	rBV3	668	1142	0.11%	0.010%
6	6.075	439	440	447	rBV3	723	1105	0.11%	0.010%
7	7.374	652	661	671	rBV	140266	246232	24.32%	2.220%
8	7.544	681	690	700	rBV	107700	188307	18.60%	1.698%
9	7.756	719	726	734	rBV	127013	230451	22.76%	2.078%
10	8.231	799	807	817	rBV	143324	244132	24.11%	2.201%
11	8.931	919	926	935	rBV2	159685	292362	28.88%	2.636%
12	9.401	999	1006	1019	rVB	135528	251959	24.89%	2.272%
13	10.129	1123	1130	1137	rBV	112879	209107	20.65%	1.886%
14	10.670	1215	1222	1231	rBV	143757	272161	26.88%	2.454%
15	11.058	1278	1288	1297	rBV	218368	405237	40.03%	3.654%
16	11.187	1303	1310	1322	rBV	157164	309780	30.60%	2.793%
17	12.632	1551	1556	1560	rBV4	1890	3000	0.30%	0.027%
18	14.248	1824	1831	1839	rBV	350009	520485	51.41%	4.693%
19	14.553	1876	1883	1890	rBV	359648	580364	57.33%	5.233%
20	14.853	1927	1934	1942	rBV	384694	609206	60.18%	5.493%
21	15.041	1960	1966	1984	rBV	126525	246430	24.34%	2.222%
22	15.194	1990	1992	1996	rVB4	825	1036	0.10%	0.009%
23	15.846	2095	2103	2114	rVB	465202	740109	73.11%	6.674%
24	15.958	2116	2122	2134	rBV	143082	229557	22.67%	2.070%
25	16.081	2140	2143	2149	rVB3	2279	3284	0.32%	0.030%
26	17.391	2361	2366	2370	rBV2	1646	2690	0.27%	0.024%
27	17.603	2395	2402	2411	rVB	509198	801797	79.20%	7.230%
28	17.697	2411	2418	2428	rVV	533762	854878	84.44%	7.709%
29	19.383	2703	2705	2707	rVB3	1159	1104	0.11%	0.010%
30	19.548	2728	2733	2738	rBV4	6582	10065	0.99%	0.091%
31	19.612	2738	2744	2749	rBV2	7230	11626	1.15%	0.105%
32	19.865	2784	2787	2790	rVB4	2774	3448	0.34%	0.031%
33	19.976	2799	2806	2816	rBV	676016	1012381	100.00%	9.129%
34	20.253	2852	2853	2856	rVB2	1711	1279	0.13%	0.012%
35	20.282	2856	2858	2860	rBV3	1715	2022	0.20%	0.018%
36	20.317	2862	2864	2866	rBV2	1531	1298	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050818.D
 Acq On : 2 Nov 2021 15:36
 Operator : CG/JU
 Sample : PB140311BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK311

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	20.546	2901	2903	2904	rBV2	1305	1119	0.11%	0.010%
38	20.588	2909	2910	2913	rBV3	1780	2002	0.20%	0.018%
39	20.699	2927	2929	2931	rVB3	2064	1244	0.12%	0.011%
40	20.764	2938	2940	2942	rBV3	1293	1467	0.14%	0.013%
41	20.828	2950	2951	2953	rBV2	1941	1562	0.15%	0.014%
42	20.905	2960	2964	2965	rBV4	5807	6854	0.68%	0.062%
43	21.146	3003	3005	3007	rBV3	1998	1635	0.16%	0.015%
44	21.275	3025	3027	3028	rBV2	2123	1343	0.13%	0.012%
45	21.898	3126	3133	3142	rVB	458473	786517	77.69%	7.092%
46	24.277	3533	3538	3543	rVB4	12040	24521	2.42%	0.221%
47	25.065	3661	3672	3683	rBV2	287135	862679	85.21%	7.779%
48	25.300	3701	3712	3724	rVB2	246138	754381	74.52%	6.802%
49	25.852	3804	3806	3807	rBV2	2378	1478	0.15%	0.013%
50	26.246	3871	3873	3875	rBV3	2879	2991	0.30%	0.027%
51	26.481	3903	3913	3922	rVB4	16230	52862	5.22%	0.477%
52	26.716	3951	3953	3956	rBV4	2711	3089	0.31%	0.028%
53	26.962	3994	3995	4000	rVB5	3554	3839	0.38%	0.035%
54	26.998	4000	4001	4002	rBV	3245	1601	0.16%	0.014%
55	27.926	4148	4159	4169	rBV6	15511	61131	6.04%	0.551%
56	30.170	4539	4541	4543	rBV2	2447	2289	0.23%	0.021%
57	31.152	4706	4708	4709	rBV2	2678	2013	0.20%	0.018%
58	31.733	4805	4807	4808	rBV2	3655	3248	0.32%	0.029%




Sum of corrected areas: 11089833

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050818.D
Acq On : 2 Nov 2021 15:36
Operator : CG/JU
Sample : PB140311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK311

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

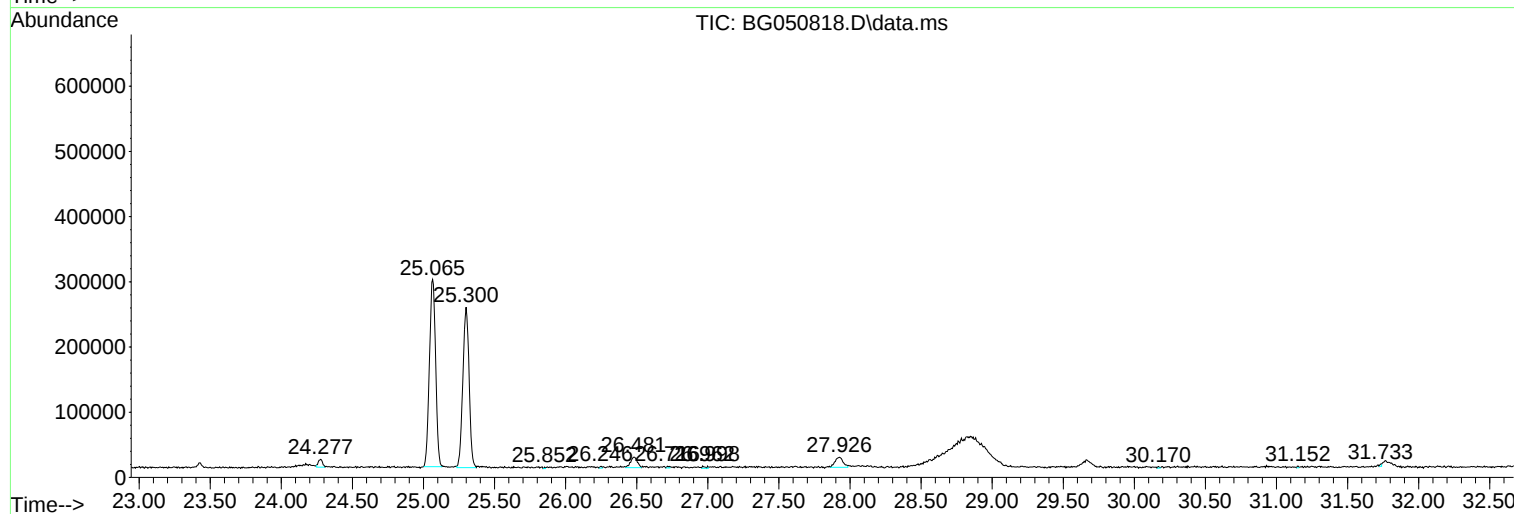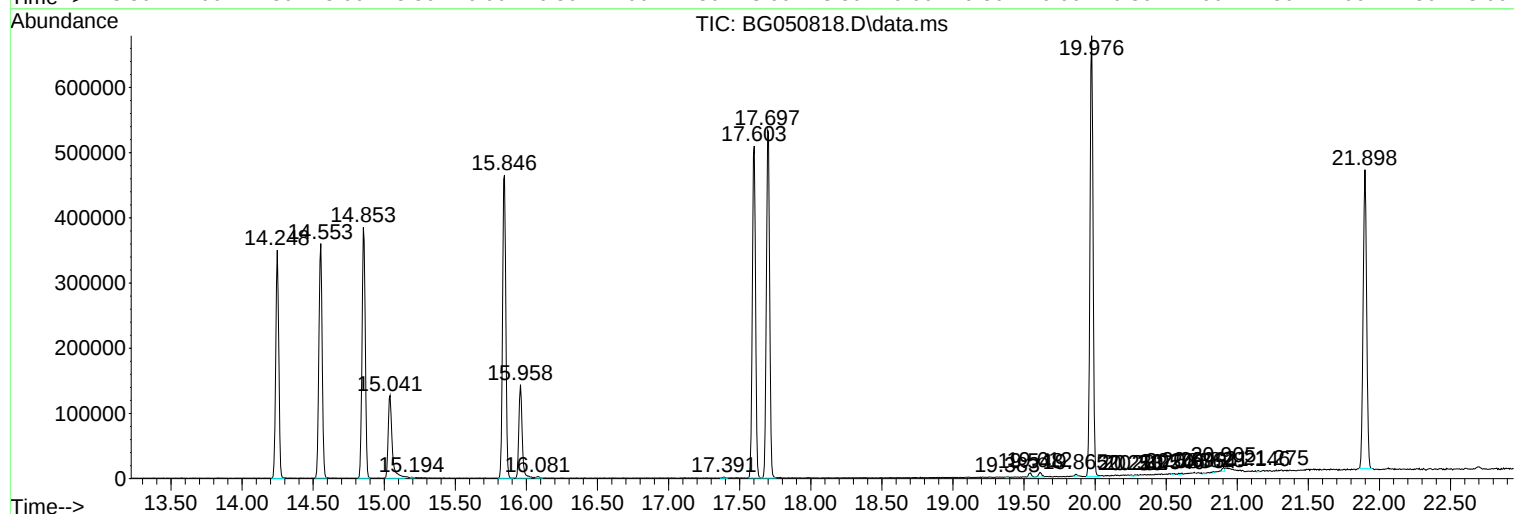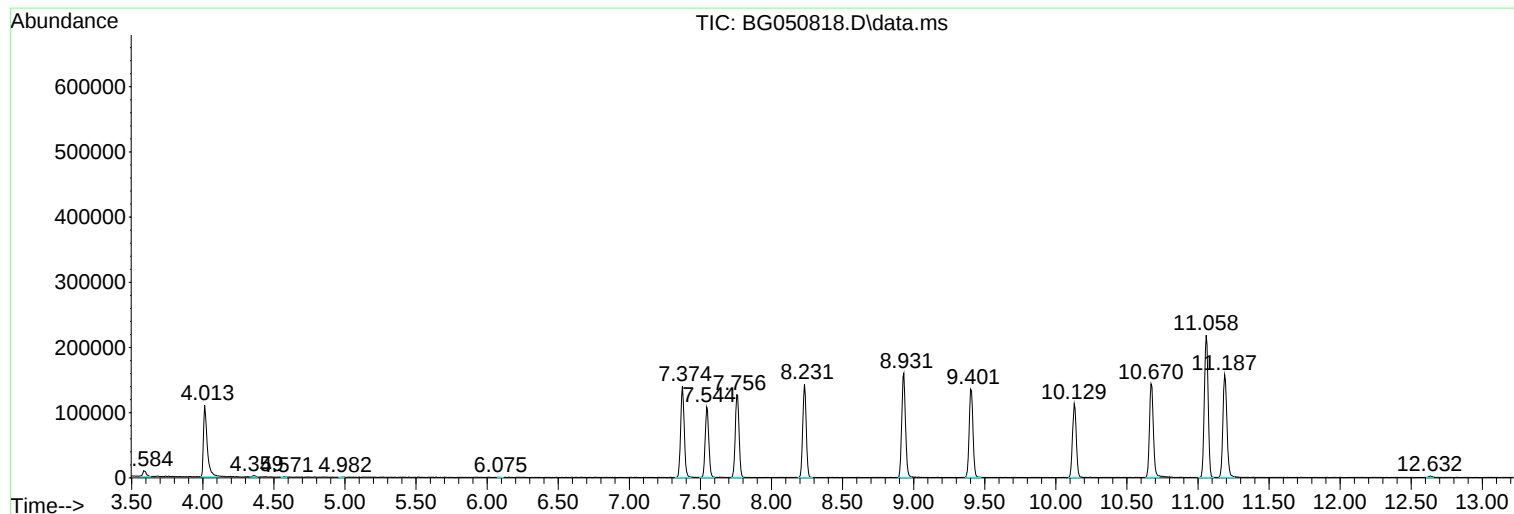

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050818.D
Acq On : 2 Nov 2021 15:36
Operator : CG/JU
Sample : PB140311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK311

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050818.D
Acq On : 2 Nov 2021 15:36
Operator : CG/JU
Sample : PB140311BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK311

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc