

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050832.D
 Acq On : 3 Nov 2021 1:55
 Operator : CG/JU
 Sample : M4364-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG324

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.590	12	17	22	rBV	7258	10978	0.85%	0.091%
2	3.872	61	65	68	rBV	3197	4375	0.34%	0.036%
3	4.019	86	90	101	rBV	25696	44582	3.44%	0.369%
4	4.254	123	130	136	rBV	4912	8009	0.62%	0.066%
5	4.360	144	148	153	rVB4	2598	3750	0.29%	0.031%
6	4.466	161	166	168	rBV4	1578	1768	0.14%	0.015%
7	4.671	196	201	204	rBV2	1842	2467	0.19%	0.020%
8	4.859	229	233	242	rBV2	7364	11438	0.88%	0.095%
9	5.294	302	307	310	rBV4	997	1716	0.13%	0.014%
10	5.876	402	406	411	rBV2	2346	3179	0.25%	0.026%
11	6.275	469	474	475	rBV2	1213	1601	0.12%	0.013%
12	6.299	475	478	481	rVB3	1428	2026	0.16%	0.017%
13	7.004	594	598	605	rVB2	1099	1751	0.14%	0.014%
14	7.374	655	661	671	rVB2	27695	54556	4.21%	0.451%
15	7.544	683	690	699	rVB	112027	189062	14.61%	1.564%
16	7.756	718	726	735	rBV	99646	180467	13.94%	1.493%
17	8.232	800	807	815	rBV	135433	237526	18.35%	1.965%
18	8.925	919	925	933	rBV	80526	149662	11.56%	1.238%
19	9.401	996	1006	1017	rBV	139805	260470	20.12%	2.155%
20	9.765	1062	1068	1073	rVB	3527	5302	0.41%	0.044%
21	10.130	1123	1130	1139	rBV	118983	213078	16.46%	1.763%
22	10.670	1215	1222	1235	rBV	145943	271219	20.95%	2.244%
23	10.805	1238	1245	1254	rVV5	7873	16940	1.31%	0.140%
24	11.058	1280	1288	1296	rVB	224416	412610	31.88%	3.414%
25	11.187	1303	1310	1323	rBV	130190	247123	19.09%	2.045%
26	12.257	1487	1492	1498	rVB	3726	5480	0.42%	0.045%
27	12.627	1549	1555	1561	rVB3	2494	4373	0.34%	0.036%
28	13.455	1690	1696	1698	rVB4	1190	1594	0.12%	0.013%
29	13.649	1726	1729	1732	rVB2	1355	1356	0.10%	0.011%
30	14.248	1823	1831	1838	rVB	412585	621251	48.00%	5.140%
31	14.548	1875	1882	1892	rBV	401769	654370	50.55%	5.414%
32	14.854	1926	1934	1945	rVB	408061	647387	50.02%	5.356%
33	15.042	1961	1966	1976	rBV3	24762	52105	4.03%	0.431%
34	15.106	1976	1977	1981	rVV3	2350	2518	0.19%	0.021%
35	15.623	2059	2065	2067	rBV3	1063	1442	0.11%	0.012%
36	15.841	2095	2102	2110	rVV	588345	912813	70.52%	7.552%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050832.D
 Acq On : 3 Nov 2021 1:55
 Operator : CG/JU
 Sample : M4364-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG324

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	15.958	2115	2122	2133	rBV	201609	321323	24.82%	2.658%
38	16.076	2138	2142	2147	rVB2	3044	4649	0.36%	0.038%
39	16.223	2163	2167	2173	rVB4	1448	1969	0.15%	0.016%
40	17.380	2360	2364	2369	rVB	1474	2244	0.17%	0.019%
41	17.597	2394	2401	2409	rBV	567286	856510	66.17%	7.086%
42	17.697	2411	2418	2427	rBV2	699280	1088936	84.13%	9.009%
43	18.238	2505	2510	2513	rVB4	2642	4057	0.31%	0.034%
44	18.532	2556	2560	2563	rBV3	1650	2570	0.20%	0.021%
45	18.743	2594	2596	2600	rBV2	1232	1320	0.10%	0.011%
46	18.878	2614	2619	2623	rVB2	1279	2162	0.17%	0.018%
47	19.278	2682	2687	2690	rBV3	1164	1968	0.15%	0.016%
48	19.366	2699	2702	2704	rBV3	1474	1907	0.15%	0.016%
49	19.384	2704	2705	2710	rVB3	2382	2279	0.18%	0.019%
50	19.542	2726	2732	2736	rVB2	9743	14921	1.15%	0.123%
51	19.607	2739	2743	2748	rVV	11095	15983	1.23%	0.132%
52	19.859	2780	2786	2789	rBV5	6748	8141	0.63%	0.067%
53	19.971	2794	2805	2813	rBV	890340	1294384	100.00%	10.709%
54	20.106	2826	2828	2831	rVB3	1912	1841	0.14%	0.015%
55	20.188	2840	2842	2843	rBV	1880	1450	0.11%	0.012%
56	20.382	2872	2875	2877	rBV4	1549	2065	0.16%	0.017%
57	20.470	2886	2890	2893	rBV5	2048	3165	0.24%	0.026%
58	20.494	2893	2894	2897	rVV3	1694	1374	0.11%	0.011%
59	20.535	2899	2901	2905	rVV5	1528	1577	0.12%	0.013%
60	20.647	2918	2920	2921	rBV3	2375	1621	0.13%	0.013%
61	20.682	2925	2926	2927	rVV	2000	1348	0.10%	0.011%
62	20.835	2951	2952	2954	rBV2	2223	1824	0.14%	0.015%
63	20.899	2960	2963	2965	rBV3	5013	5109	0.39%	0.042%
64	21.493	3060	3064	3070	rBV6	15097	36002	2.78%	0.298%
65	21.892	3125	3132	3142	rBV	496671	864958	66.82%	7.156%
66	22.691	3265	3268	3274	rVB6	6141	8919	0.69%	0.074%
67	22.909	3303	3305	3309	rBV4	2485	2330	0.18%	0.019%
68	23.079	3332	3334	3336	rBV3	2089	1445	0.11%	0.012%
69	23.420	3389	3392	3399	rVB6	10284	17892	1.38%	0.148%
70	24.049	3497	3499	3502	rBV4	3227	3352	0.26%	0.028%
71	24.272	3531	3537	3548	rVB3	16818	40203	3.11%	0.333%
72	25.059	3659	3671	3686	rVB2	382491	1127515	87.11%	9.329%
73	25.294	3698	3711	3723	rVB2	297739	913794	70.60%	7.560%
74	25.788	3794	3795	3797	rBV2	2538	2202	0.17%	0.018%
75	25.982	3826	3828	3830	rBV3	2364	2754	0.21%	0.023%
76	26.064	3841	3842	3846	rBV4	2470	2105	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050832.D
 Acq On : 3 Nov 2021 1:55
 Operator : CG/JU
 Sample : M4364-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG324

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

77	26.475	3903	3912	3924	rVB4	20382	65729	5.08%	0.544%
78	26.687	3946	3948	3950	rBV3	2203	1581	0.12%	0.013%
79	26.769	3960	3962	3963	rBV2	2159	1635	0.13%	0.014%
80	27.086	4014	4016	4019	rBV4	2328	2623	0.20%	0.022%
81	27.527	4089	4091	4095	rBV4	2218	2285	0.18%	0.019%
82	27.780	4132	4134	4135	rVB2	2969	1689	0.13%	0.014%
83	27.915	4149	4157	4168	rVB6	18155	60255	4.66%	0.499%
84	27.991	4168	4170	4172	rBV3	3040	1906	0.15%	0.016%
85	28.291	4220	4221	4223	rBV2	2313	1726	0.13%	0.014%
86	28.332	4226	4228	4231	rBV4	2231	1842	0.14%	0.015%
87	29.084	4355	4356	4362	rBV6	2479	4291	0.33%	0.036%
88	29.295	4390	4392	4395	rVB4	1706	1370	0.11%	0.011%
89	29.325	4395	4397	4398	rVB2	3386	1538	0.12%	0.013%
90	29.648	4446	4452	4453	rBV5	7460	13172	1.02%	0.109%
91	29.942	4500	4502	4504	rVB3	2346	1296	0.10%	0.011%
92	30.758	4639	4641	4643	rBV3	2347	1371	0.11%	0.011%
93	30.882	4660	4662	4663	rBV2	2172	1851	0.14%	0.015%
94	30.993	4679	4681	4683	rBV3	2496	2351	0.18%	0.019%
95	31.452	4757	4759	4760	rBV	2108	1559	0.12%	0.013%
96	31.681	4796	4798	4800	rBV3	2452	2822	0.22%	0.023%
97	31.734	4805	4807	4808	rBV2	4272	3372	0.26%	0.028%




Sum of corrected areas: 12086776

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050832.D
Acq On : 3 Nov 2021 1:55
Operator : CG/JU
Sample : M4364-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

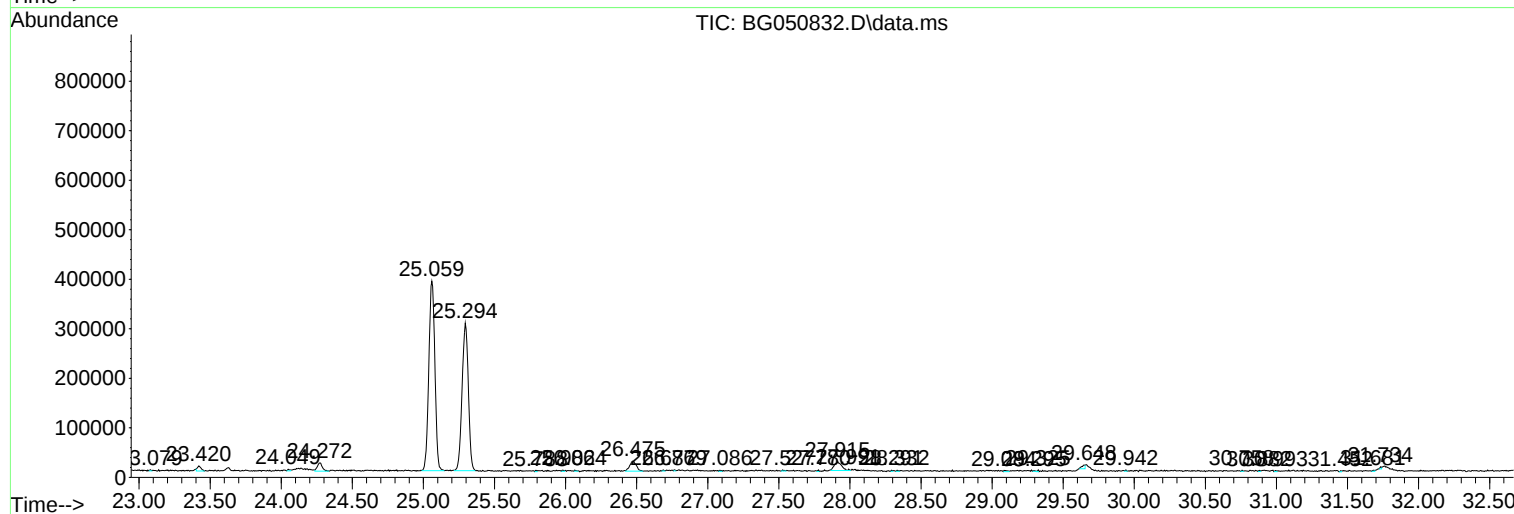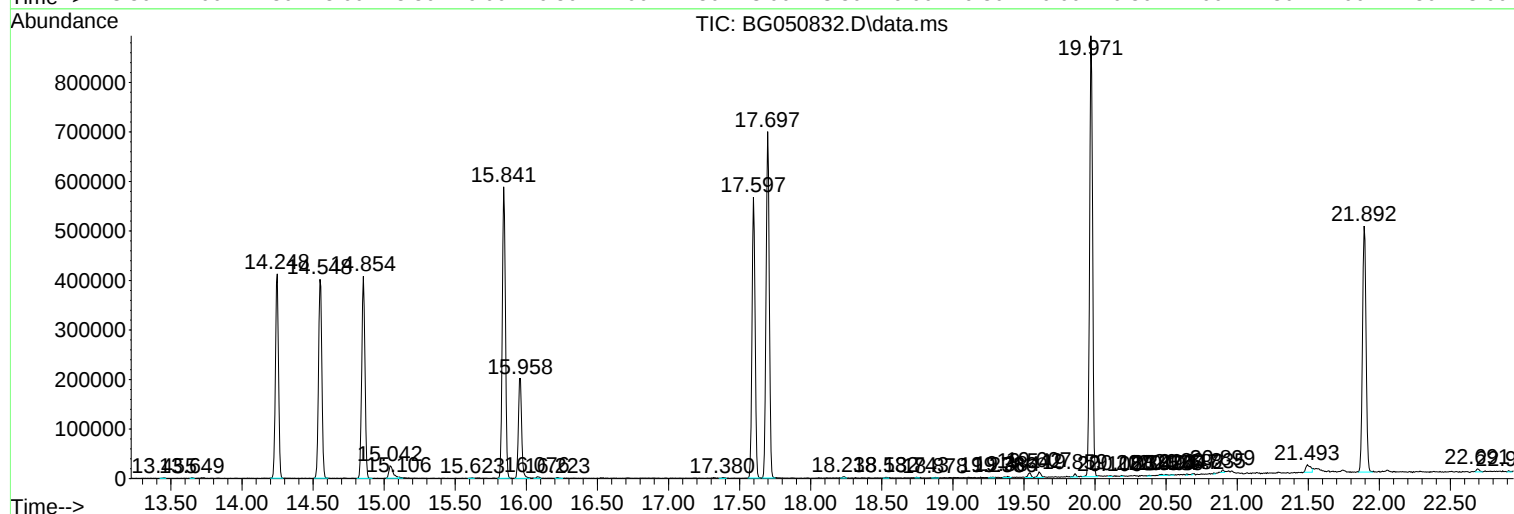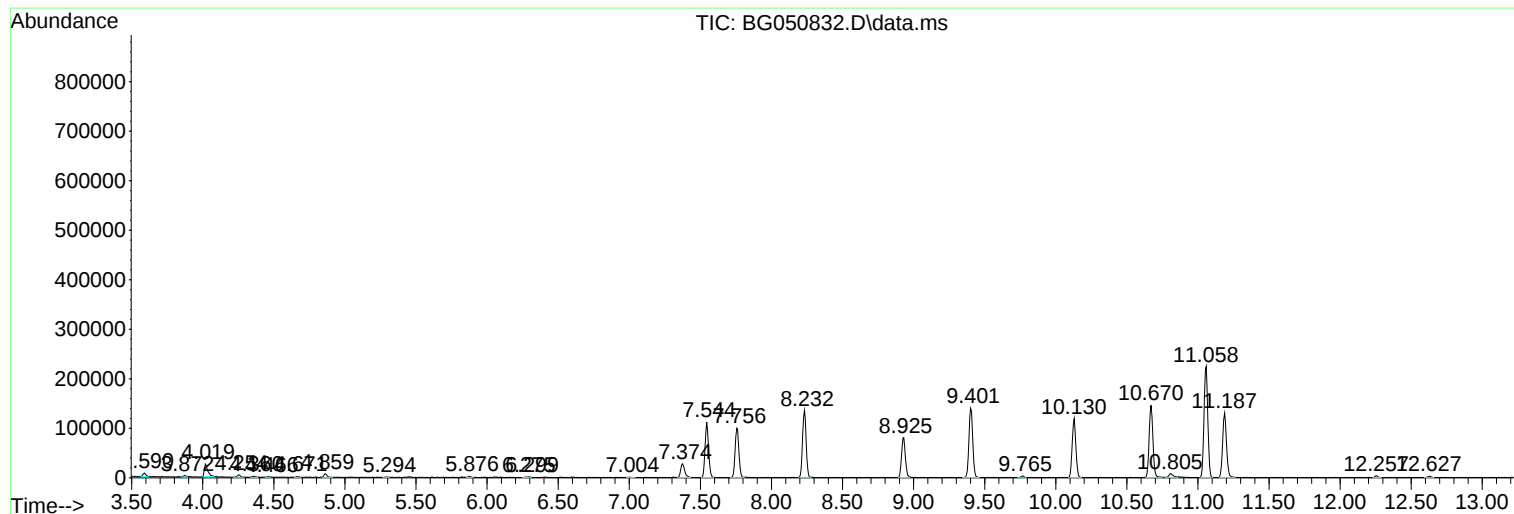

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050832.D
Acq On : 3 Nov 2021 1:55
Operator : CG/JU
Sample : M4364-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050832.D
Acq On : 3 Nov 2021 1:55
Operator : CG/JU
Sample : M4364-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc