

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050834.D
 Acq On : 3 Nov 2021 3:17
 Operator : CG/JU
 Sample : M4364-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG328

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.587	12	17	24	rVB	7716	12419	0.98%	0.103%
2	4.016	87	90	103	rBV	27381	50663	3.98%	0.419%
3	4.251	125	130	137	rVB2	5465	8392	0.66%	0.069%
4	4.357	143	148	153	rVB3	2319	3230	0.25%	0.027%
5	4.457	162	165	172	rBV5	1685	2762	0.22%	0.023%
6	6.595	526	529	535	rBV2	1222	2150	0.17%	0.018%
7	7.306	647	650	654	rBV	2021	2369	0.19%	0.020%
8	7.371	654	661	675	rVB2	29904	61384	4.82%	0.507%
9	7.541	684	690	699	rBV	125660	223141	17.53%	1.844%
10	7.759	719	727	734	rBV	111114	201613	15.84%	1.666%
11	8.229	800	807	814	rBV	136922	235187	18.48%	1.944%
12	8.928	919	926	935	rVB	86612	158251	12.43%	1.308%
13	9.404	999	1007	1017	rBV	159385	297557	23.38%	2.459%
14	9.768	1062	1069	1074	rBV	15186	22568	1.77%	0.187%
15	10.127	1123	1130	1138	rBV	125566	230590	18.12%	1.906%
16	10.667	1215	1222	1232	rBV	158464	296951	23.33%	2.454%
17	10.808	1241	1246	1252	rBV4	6617	13862	1.09%	0.115%
18	11.055	1280	1288	1297	rBV	214135	391861	30.79%	3.239%
19	11.184	1302	1310	1323	rBV	148212	289584	22.75%	2.394%
20	12.254	1487	1492	1499	rVB2	11388	16376	1.29%	0.135%
21	12.624	1549	1555	1560	rVB3	2940	4544	0.36%	0.038%
22	13.722	1739	1742	1747	rVB2	1272	1628	0.13%	0.013%
23	14.245	1819	1831	1838	rBV	423662	613611	48.21%	5.072%
24	14.551	1876	1883	1890	rBV	433590	699602	54.97%	5.782%
25	14.856	1928	1935	1943	rVB	380489	610488	47.97%	5.046%
26	15.044	1961	1967	1976	rBV3	19907	41779	3.28%	0.345%
27	15.843	2096	2103	2110	rBV	583084	910061	71.50%	7.522%
28	15.955	2116	2122	2135	rBV2	178159	284427	22.35%	2.351%
29	16.078	2140	2143	2150	rBV3	2977	4392	0.35%	0.036%
30	16.219	2163	2167	2170	rBV	2679	2913	0.23%	0.024%
31	17.383	2362	2365	2368	rVB3	1456	1734	0.14%	0.014%
32	17.600	2395	2402	2408	rVV	519846	814074	63.96%	6.729%
33	17.700	2411	2419	2427	rVV	678947	1061443	83.40%	8.773%
34	17.771	2429	2431	2434	rVB3	1923	1876	0.15%	0.016%
35	18.047	2473	2478	2480	rBV2	760	1288	0.10%	0.011%
36	18.117	2485	2490	2496	rVB3	1144	1862	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050834.D
 Acq On : 3 Nov 2021 3:17
 Operator : CG/JU
 Sample : M4364-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG328

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	18.235	2506	2510	2514	rVB3	3620	4795	0.38%	0.040%
38	18.534	2558	2561	2563	rVB2	1182	1367	0.11%	0.011%
39	19.151	2664	2666	2669	rVB2	1708	1570	0.12%	0.013%
40	19.392	2703	2707	2709	rBV2	1247	1519	0.12%	0.013%
41	19.422	2711	2712	2716	rBV3	1413	1455	0.11%	0.012%
42	19.539	2727	2732	2737	rVB4	8859	14840	1.17%	0.123%
43	19.610	2739	2744	2754	rVB	9749	15632	1.23%	0.129%
44	19.739	2760	2766	2767	rBV4	1318	2210	0.17%	0.018%
45	19.862	2781	2787	2790	rBV3	5999	8349	0.66%	0.069%
46	19.974	2798	2806	2813	rVV	892946	1272767	100.00%	10.520%
47	20.332	2865	2867	2870	rBV3	1186	1705	0.13%	0.014%
48	20.467	2887	2890	2893	rBV4	1772	1941	0.15%	0.016%
49	20.544	2901	2903	2904	rBV	1766	1338	0.11%	0.011%
50	20.679	2924	2926	2927	rBV2	1579	1466	0.12%	0.012%
51	20.796	2945	2946	2949	rBV3	1872	2181	0.17%	0.018%
52	20.873	2958	2959	2960	rBV	3069	1603	0.13%	0.013%
53	20.902	2961	2964	2967	rVV3	6456	7852	0.62%	0.065%
54	21.090	2993	2996	3000	rVB5	2378	3093	0.24%	0.026%
55	21.496	3060	3065	3070	rBV7	11731	25822	2.03%	0.213%
56	21.742	3105	3107	3113	rVB6	3428	5278	0.41%	0.044%
57	21.895	3126	3133	3142	rVB	477495	821172	64.52%	6.787%
58	22.054	3157	3160	3164	rBV5	4461	6707	0.53%	0.055%
59	22.218	3185	3188	3189	rBV3	2036	2499	0.20%	0.021%
60	22.694	3266	3269	3273	rVB5	6732	8988	0.71%	0.074%
61	22.741	3275	3277	3279	rBV3	1684	1347	0.11%	0.011%
62	22.782	3282	3284	3286	rVB3	2528	1979	0.16%	0.016%
63	22.806	3286	3288	3290	rBV3	2743	2322	0.18%	0.019%
64	23.423	3388	3393	3401	rVB5	12262	23795	1.87%	0.197%
65	23.623	3425	3427	3435	rVB7	5651	8336	0.65%	0.069%
66	24.269	3532	3537	3546	rVB3	17386	39323	3.09%	0.325%
67	24.568	3586	3588	3589	rVB2	2570	1298	0.10%	0.011%
68	24.992	3658	3660	3661	rBV2	3825	3100	0.24%	0.026%
69	25.062	3661	3672	3684	rVV2	368236	1110064	87.22%	9.175%
70	25.297	3700	3712	3726	rVB2	292737	879760	69.12%	7.272%
71	25.761	3789	3791	3793	rBV3	2007	1988	0.16%	0.016%
72	26.478	3905	3913	3924	rVB3	22631	66955	5.26%	0.553%
73	27.812	4137	4140	4142	rBV4	2062	2641	0.21%	0.022%
74	27.917	4149	4158	4169	rVB5	19918	68368	5.37%	0.565%
75	28.111	4189	4191	4196	rVB5	2071	2200	0.17%	0.018%
76	28.299	4221	4223	4224	rVB2	2372	1323	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050834.D
 Acq On : 3 Nov 2021 3:17
 Operator : CG/JU
 Sample : M4364-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG328

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

77	28.446	4246	4248	4251	rBV4	2765	3428	0.27%	0.028%
78	28.493	4254	4256	4258	rVV3	1965	1889	0.15%	0.016%
79	28.793	4305	4307	4311	rVB5	2200	2229	0.18%	0.018%
80	29.081	4354	4356	4357	rBV2	2370	2399	0.19%	0.020%
81	29.222	4378	4380	4381	rVB2	2166	1399	0.11%	0.012%
82	29.239	4381	4383	4385	rBV3	2326	2447	0.19%	0.020%
83	29.281	4388	4390	4391	rBV2	2154	1581	0.12%	0.013%
84	29.645	4444	4452	4454	rBV6	12834	28235	2.22%	0.233%
85	30.121	4531	4533	4535	rBV3	2355	2377	0.19%	0.020%
86	30.203	4546	4547	4551	rVB4	2282	1381	0.11%	0.011%
87	30.391	4577	4579	4582	rBV4	2012	2365	0.19%	0.020%
88	30.614	4615	4617	4619	rVB3	1982	1613	0.13%	0.013%
89	31.378	4746	4747	4748	rBV	2791	1795	0.14%	0.015%
90	31.754	4798	4811	4813	rBV10	12336	38007	2.99%	0.314%




Sum of corrected areas: 12098725

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050834.D
Acq On : 3 Nov 2021 3:17
Operator : CG/JU
Sample : M4364-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG328

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

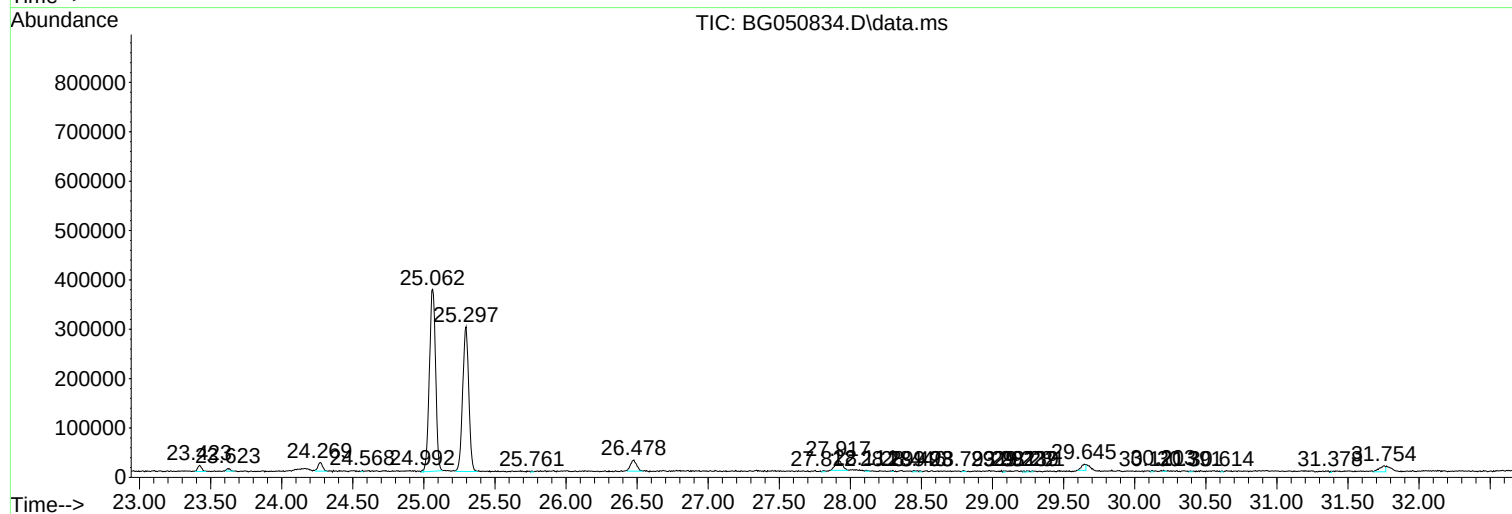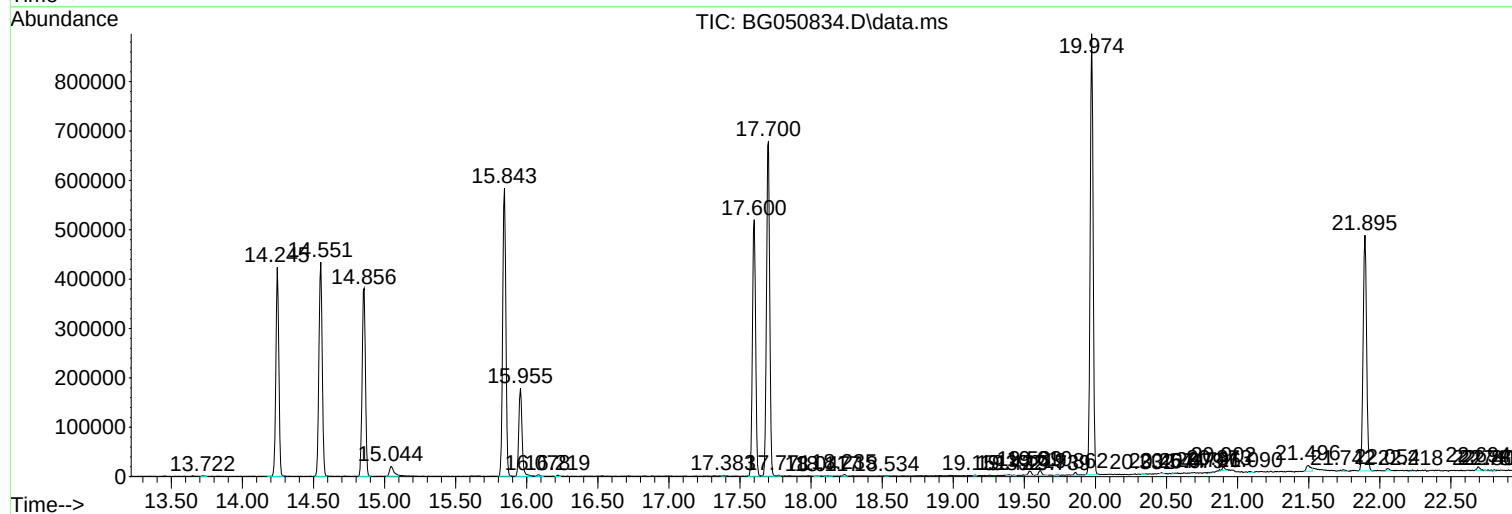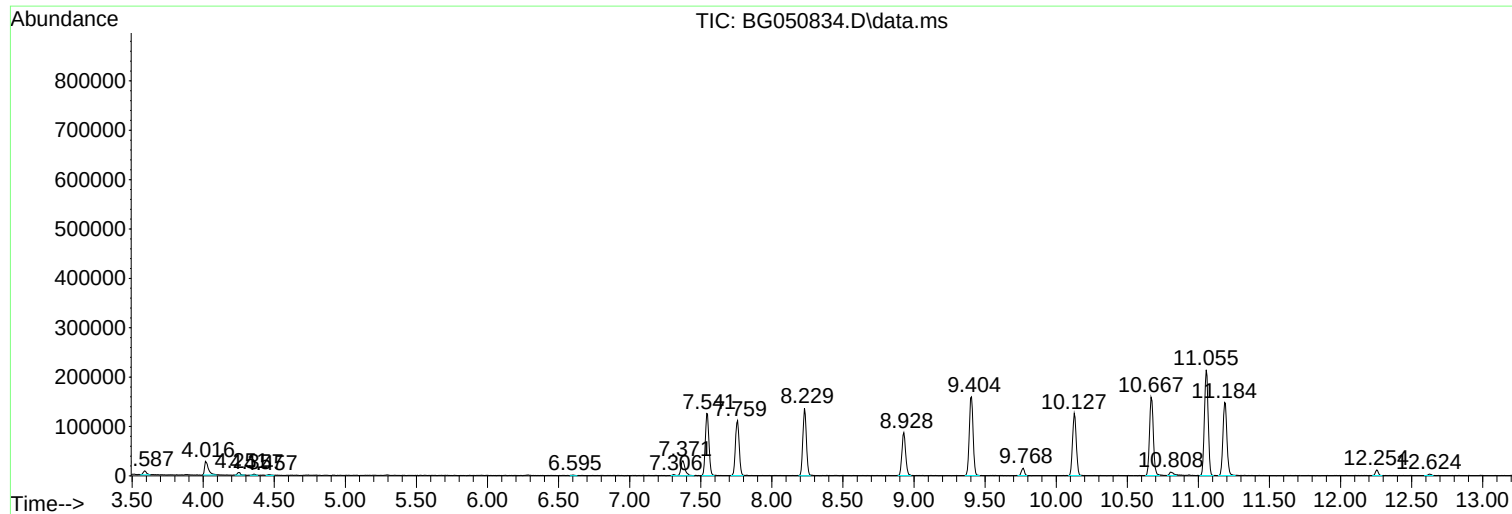

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050834.D
Acq On : 3 Nov 2021 3:17
Operator : CG/JU
Sample : M4364-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG328

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050834.D
Acq On : 3 Nov 2021 3:17
Operator : CG/JU
Sample : M4364-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG328

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc