

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050836.D
 Acq On : 3 Nov 2021 5:19
 Operator : CG/JU
 Sample : PB140350BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK350

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.585	12	16	23	rVB	9343	14004	1.26%	0.111%
2	4.014	84	89	101	rBV	114391	210143	18.95%	1.665%
3	4.354	143	147	151	rBV	5064	7514	0.68%	0.060%
4	7.369	654	660	673	rBV	144627	257904	23.25%	2.043%
5	7.545	683	690	697	rBV	112317	196709	17.74%	1.558%
6	7.756	717	726	735	rVB	136349	239167	21.56%	1.895%
7	8.232	800	807	815	rBV	150194	261589	23.59%	2.072%
8	8.925	918	925	937	rBV	172233	310941	28.04%	2.463%
9	9.401	998	1006	1015	rBV	146613	261992	23.62%	2.076%
10	10.130	1122	1130	1139	rVB	118675	221769	20.00%	1.757%
11	10.671	1213	1222	1231	rBV	152909	295143	26.61%	2.338%
12	11.052	1280	1287	1299	rVB	240043	449935	40.57%	3.565%
13	11.188	1302	1310	1320	rBV	172944	331011	29.85%	2.622%
14	12.627	1551	1555	1563	rVB3	2409	4446	0.40%	0.035%
15	14.243	1824	1830	1838	rBV	366998	568833	51.29%	4.507%
16	14.548	1875	1882	1892	rBV	393522	638489	57.57%	5.058%
17	14.854	1926	1934	1943	rBV	454104	714553	64.43%	5.661%
18	15.036	1959	1965	1982	rBV	144033	273073	24.62%	2.163%
19	15.165	1985	1987	1994	rVB4	1596	2903	0.26%	0.023%
20	15.841	2095	2102	2112	rBV	534481	814479	73.44%	6.453%
21	15.953	2115	2121	2138	rBV	155719	262007	23.62%	2.076%
22	16.082	2138	2143	2147	rVB3	2829	3825	0.34%	0.030%
23	17.386	2361	2365	2371	rVB	1677	2741	0.25%	0.022%
24	17.598	2394	2401	2411	rBV	598128	951302	85.78%	7.537%
25	17.698	2411	2418	2426	rBV2	613079	942503	84.98%	7.467%
26	18.021	2470	2473	2478	rBV3	593	1167	0.11%	0.009%
27	19.542	2727	2732	2737	rBV3	8078	11103	1.00%	0.088%
28	19.607	2739	2743	2749	rBV	7902	11730	1.06%	0.093%
29	19.860	2778	2786	2789	rVB4	5186	6606	0.60%	0.052%
30	19.971	2799	2805	2812	rBV	760773	1109054	100.00%	8.787%
31	20.124	2830	2831	2834	rBV2	1081	1174	0.11%	0.009%
32	20.154	2834	2836	2839	rVB3	1125	1136	0.10%	0.009%
33	20.300	2857	2861	2864	rVB4	1043	1489	0.13%	0.012%
34	20.342	2864	2868	2872	rBV4	1500	2413	0.22%	0.019%
35	20.371	2872	2873	2877	rBV3	958	1457	0.13%	0.012%
36	20.553	2901	2904	2905	rBV2	1639	1323	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050836.D
 Acq On : 3 Nov 2021 5:19
 Operator : CG/JU
 Sample : PB140350BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK350

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	20.688	2925	2927	2930	rVB4	1514	1395	0.13%	0.011%
38	20.817	2944	2949	2950	rBV5	2396	2887	0.26%	0.023%
39	20.900	2950	2963	2965	rBV7	12931	33567	3.03%	0.266%
40	21.235	3019	3020	3024	rBV4	1638	1849	0.17%	0.015%
41	21.405	3047	3049	3051	rVB3	2121	1407	0.13%	0.011%
42	21.423	3051	3052	3054	rBV2	1867	1718	0.15%	0.014%
43	21.476	3059	3061	3063	rBV2	2266	2680	0.24%	0.021%
44	21.564	3074	3076	3078	rBV2	1478	1321	0.12%	0.010%
45	21.640	3087	3089	3093	rVB5	2156	2003	0.18%	0.016%
46	21.746	3105	3107	3110	rBV4	1790	1826	0.16%	0.014%
47	21.893	3123	3132	3141	rBV	564663	985182	88.83%	7.805%
48	22.686	3265	3267	3268	rBV2	3520	2451	0.22%	0.019%
49	23.420	3388	3392	3397	rVB6	7452	13191	1.19%	0.105%
50	24.266	3532	3536	3546	rVB3	14012	31444	2.84%	0.249%
51	24.654	3600	3602	3604	rBV3	2741	2231	0.20%	0.018%
52	25.060	3659	3671	3683	rBV2	332280	979221	88.29%	7.758%
53	25.295	3699	3711	3726	rVB2	322186	1001128	90.27%	7.931%
54	26.370	3892	3894	3897	rBV4	1538	1296	0.12%	0.010%
55	26.476	3904	3912	3920	rBV4	17712	47471	4.28%	0.376%
56	27.098	4016	4018	4019	rBV2	1902	1372	0.12%	0.011%
57	27.692	4117	4119	4121	rBV3	1990	2145	0.19%	0.017%
58	27.780	4132	4134	4139	rVB6	2037	2542	0.23%	0.020%
59	27.909	4146	4156	4157	rBV6	18791	40655	3.67%	0.322%
60	28.362	4231	4233	4235	rBV3	1967	1719	0.15%	0.014%
61	29.178	4370	4372	4375	rBV4	2092	2463	0.22%	0.020%
62	29.372	4404	4405	4408	rBV3	2478	1857	0.17%	0.015%
63	29.584	4439	4441	4442	rBV2	2016	1280	0.12%	0.010%
64	29.648	4442	4452	4466	rVV9	12828	59955	5.41%	0.475%
65	29.760	4469	4471	4474	rVB4	2344	2339	0.21%	0.019%
66	30.500	4595	4597	4598	rBV2	1670	1274	0.11%	0.010%
67	31.011	4682	4684	4685	rBV2	2042	1191	0.11%	0.009%
68	31.558	4775	4777	4778	rBV	2262	1143	0.10%	0.009%
69	32.639	4959	4961	4962	rBV2	3062	2368	0.21%	0.019%




Sum of corrected areas: 12622198

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050836.D
Acq On : 3 Nov 2021 5:19
Operator : CG/JU
Sample : PB140350BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK350

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

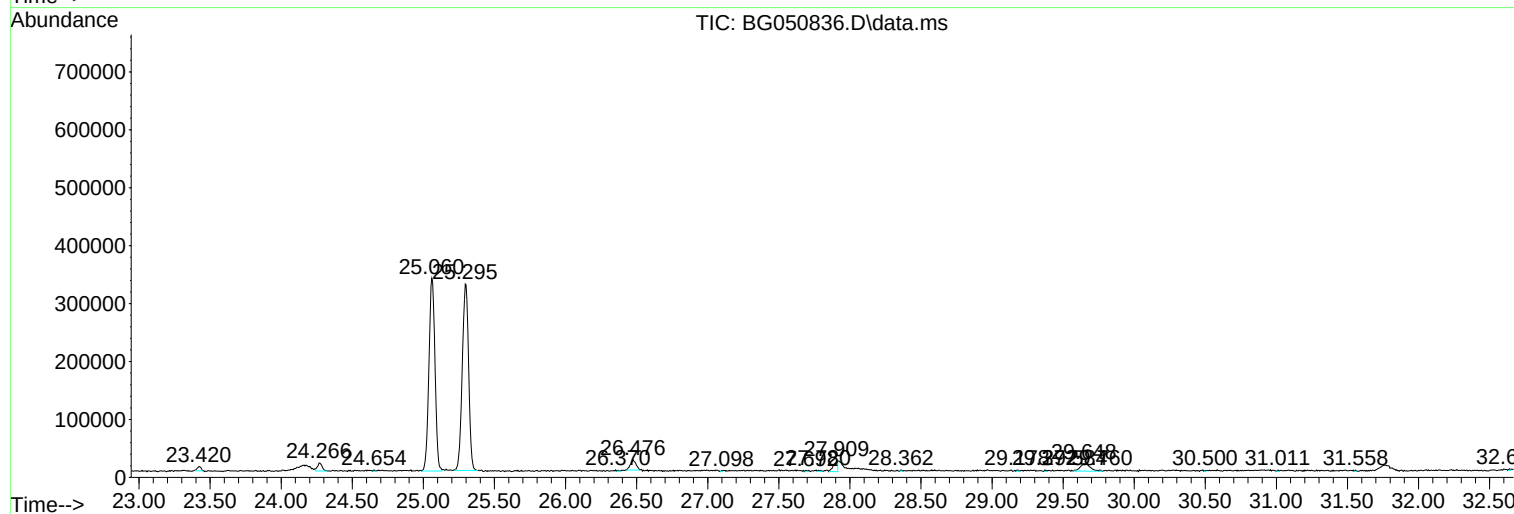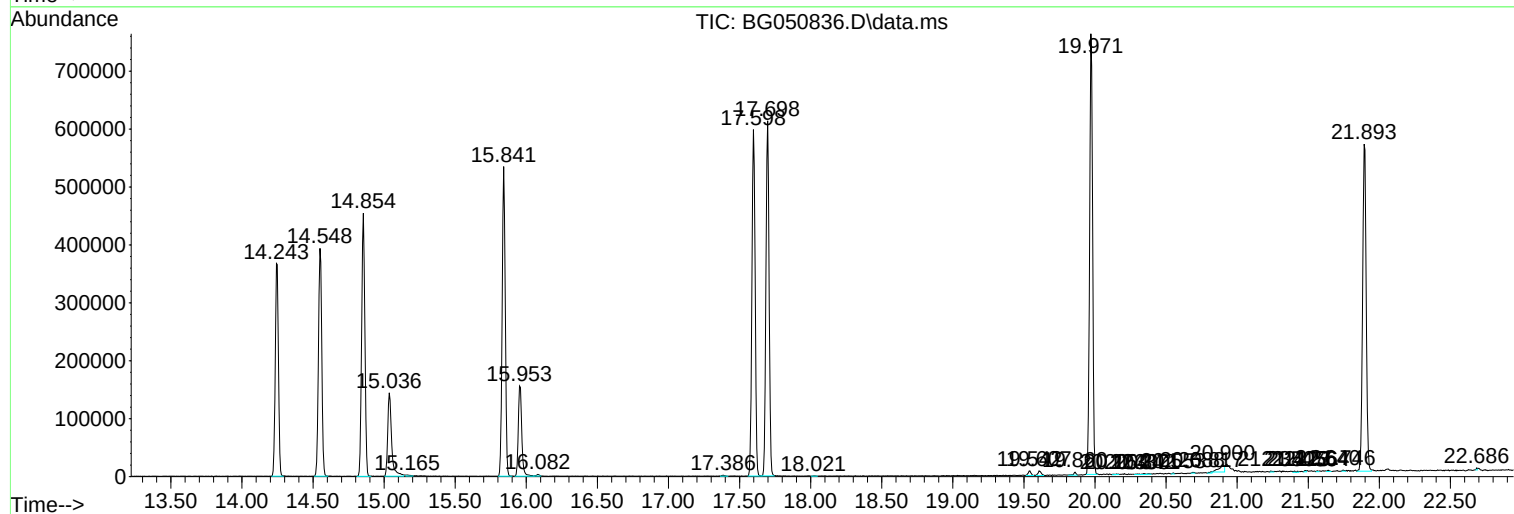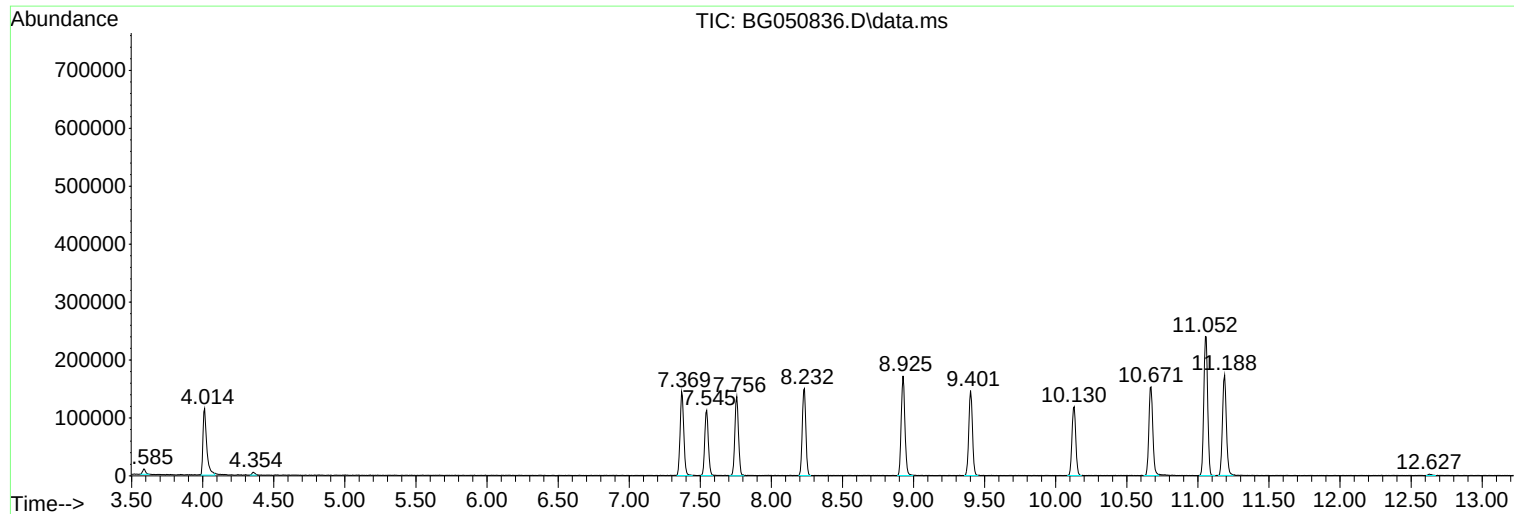

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050836.D
Acq On : 3 Nov 2021 5:19
Operator : CG/JU
Sample : PB140350BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK350

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050836.D
Acq On : 3 Nov 2021 5:19
Operator : CG/JU
Sample : PB140350BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK350

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc