

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050852.D
 Acq On : 3 Nov 2021 16:14
 Operator : CG/JU
 Sample : PB140353BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.588	13	17	24	rVB2	9349	13757	1.41%	0.142%
2	4.011	85	89	105	rBV	109878	202009	20.63%	2.084%
3	4.358	144	148	153	rVB4	1265	2094	0.21%	0.022%
4	7.025	599	602	605	rVB4	1016	1109	0.11%	0.011%
5	7.372	654	661	672	rVV	135086	241659	24.68%	2.493%
6	7.448	672	674	679	rVV2	779	1479	0.15%	0.015%
7	7.542	682	690	699	rBV	110557	187965	19.20%	1.939%
8	7.754	718	726	736	rBV	125295	225114	22.99%	2.323%
9	8.230	800	807	814	rBV	103003	175849	17.96%	1.814%
10	8.929	918	926	935	rBV	157000	286762	29.29%	2.959%
11	9.405	998	1007	1015	rBV	127049	239927	24.51%	2.475%
12	10.127	1123	1130	1138	rBV	111437	195833	20.00%	2.021%
13	10.668	1215	1222	1237	rBV2	144029	272123	27.79%	2.808%
14	11.056	1280	1288	1295	rBV	151642	270813	27.66%	2.794%
15	11.185	1303	1310	1324	rBV	156889	303572	31.01%	3.132%
16	11.996	1445	1448	1452	rBV2	739	1123	0.11%	0.012%
17	12.501	1531	1534	1538	rVB3	803	1360	0.14%	0.014%
18	12.636	1553	1557	1562	rVB4	2184	3505	0.36%	0.036%
19	14.246	1824	1831	1841	rBV	336784	498451	50.91%	5.143%
20	14.552	1875	1883	1891	rBV	346717	562930	57.50%	5.808%
21	14.851	1928	1934	1943	rVB	257432	405150	41.38%	4.180%
22	15.039	1960	1966	1987	rBV2	119577	239685	24.48%	2.473%
23	15.838	2095	2102	2110	rBV	450979	713726	72.90%	7.364%
24	15.956	2116	2122	2133	rBV	134737	211225	21.57%	2.179%
25	16.032	2133	2135	2137	rVV2	1565	1383	0.14%	0.014%
26	16.079	2140	2143	2147	rVV2	2497	3348	0.34%	0.035%
27	16.273	2173	2176	2180	rVB3	588	1057	0.11%	0.011%
28	16.925	2284	2287	2291	rBV3	770	1019	0.10%	0.011%
29	17.507	2381	2386	2388	rBV2	651	1040	0.11%	0.011%
30	17.595	2395	2401	2408	rVV	347538	525835	53.71%	5.425%
31	17.695	2411	2418	2432	rVV	506456	818725	83.62%	8.447%
32	18.994	2636	2639	2641	rBV3	819	980	0.10%	0.010%
33	19.176	2665	2670	2671	rBV2	773	1082	0.11%	0.011%
34	19.293	2688	2690	2693	rVB3	1104	1240	0.13%	0.013%
35	19.540	2727	2732	2737	rBV3	7293	10452	1.07%	0.108%
36	19.610	2740	2744	2749	rVB2	7218	9832	1.00%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050852.D
 Acq On : 3 Nov 2021 16:14
 Operator : CG/JU
 Sample : PB140353BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	19.975	2799	2806	2814	rBV	645987	979090	100.00%	10.102%
38	20.063	2818	2821	2822	rBV3	833	1056	0.11%	0.011%
39	20.151	2834	2836	2839	rVB3	1071	1185	0.12%	0.012%
40	20.263	2851	2855	2856	rVB3	1167	1187	0.12%	0.012%
41	20.451	2883	2887	2889	rBV4	1375	2069	0.21%	0.021%
42	20.692	2926	2928	2932	rBV4	1054	1421	0.15%	0.015%
43	21.003	2979	2981	2984	rBV4	1125	1136	0.12%	0.012%
44	21.126	3000	3002	3005	rBV4	1314	1400	0.14%	0.014%
45	21.649	3089	3091	3095	rBV5	1894	2381	0.24%	0.025%
46	21.896	3126	3133	3142	rBV2	304931	530226	54.15%	5.471%
47	22.771	3281	3282	3284	rBV2	2236	1359	0.14%	0.014%
48	22.977	3315	3317	3320	rVB3	1616	1719	0.18%	0.018%
49	23.054	3328	3330	3331	rBV2	1767	1439	0.15%	0.015%
50	23.424	3388	3393	3398	rVB6	6428	12881	1.32%	0.133%
51	23.477	3398	3402	3403	rVB4	2832	3138	0.32%	0.032%
52	23.794	3455	3456	3459	rBV3	2118	2314	0.24%	0.024%
53	23.923	3477	3478	3481	rBV3	1886	2058	0.21%	0.021%
54	24.276	3534	3538	3546	rVB9	7569	15301	1.56%	0.158%
55	24.452	3566	3568	3569	rBV2	1507	1113	0.11%	0.011%
56	24.804	3626	3628	3630	rBV3	1620	1289	0.13%	0.013%
57	25.057	3660	3671	3686	rVB2	305111	863185	88.16%	8.906%
58	25.292	3700	3711	3725	rVB3	177354	551695	56.35%	5.692%
59	26.085	3844	3846	3848	rBV3	1902	1416	0.14%	0.015%
60	26.467	3905	3911	3924	rVB5	11644	34030	3.48%	0.351%
61	26.661	3942	3944	3946	rVB3	1738	1394	0.14%	0.014%
62	26.690	3946	3949	3953	rBV5	2168	3178	0.32%	0.033%
63	27.160	4026	4029	4032	rVB4	2559	3021	0.31%	0.031%
64	27.760	4130	4131	4134	rVB3	2076	1104	0.11%	0.011%
65	28.253	4213	4215	4217	rVB3	1975	1238	0.13%	0.013%
66	28.764	4300	4302	4304	rBV3	1696	989	0.10%	0.010%
67	28.800	4306	4308	4309	rBV2	1631	1166	0.12%	0.012%
68	29.511	4427	4429	4430	rBV	1575	1050	0.11%	0.011%
69	29.622	4446	4448	4449	rBV2	2939	2215	0.23%	0.023%
70	29.646	4449	4452	4462	rVB10	5743	14656	1.50%	0.151%
71	30.333	4567	4569	4571	rBV3	2093	1620	0.17%	0.017%
72	30.421	4582	4584	4586	rBV2	1800	1658	0.17%	0.017%
73	31.185	4712	4714	4715	rBV2	2048	1143	0.12%	0.012%
74	31.267	4726	4728	4730	rBV3	2555	2048	0.21%	0.021%
75	31.297	4730	4733	4735	rVV4	2102	1966	0.20%	0.020%
76	31.320	4735	4737	4739	rBV3	1729	1368	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050852.D
Acq On : 3 Nov 2021 16:14
Operator : CG/JU
Sample : PB140353BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK353

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Title : SVOA CALIBRATION

77	31.573	4779	4780	4784	rBV3	2631	2208	0.23%	0.023%
78	32.372	4914	4916	4919	rVB4	2335	1607	0.16%	0.017%
79	32.472	4931	4933	4935	rVB2	1820	1312	0.13%	0.014%




Sum of corrected areas: 9692242

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050852.D
Acq On : 3 Nov 2021 16:14
Operator : CG/JU
Sample : PB140353BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

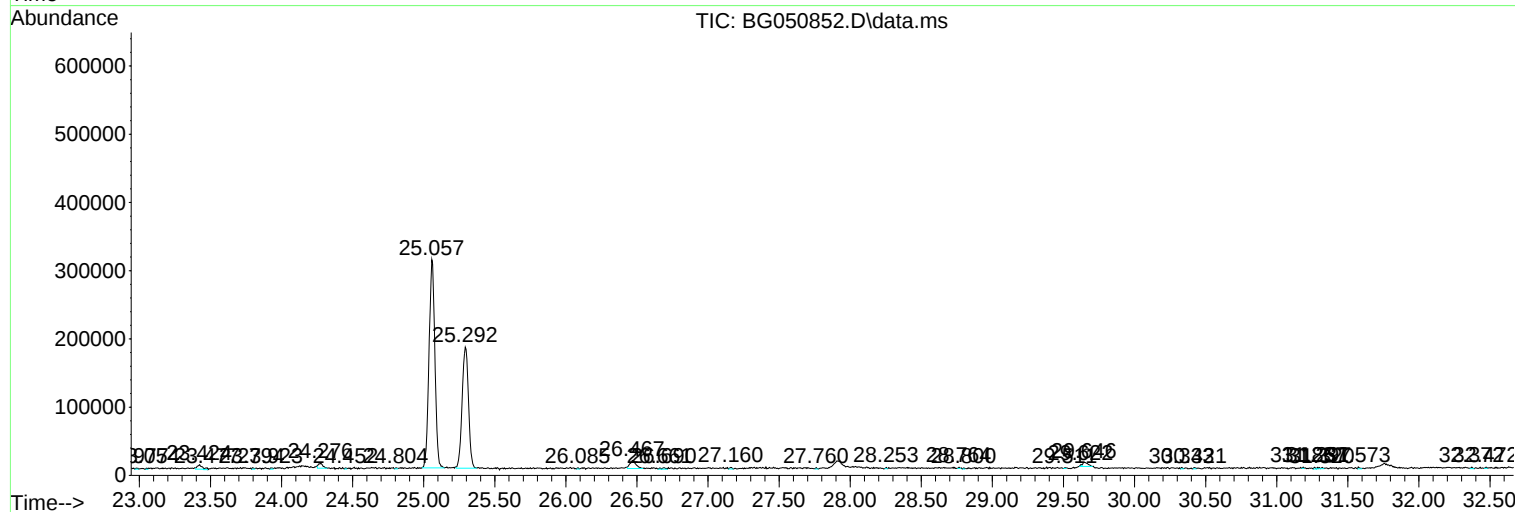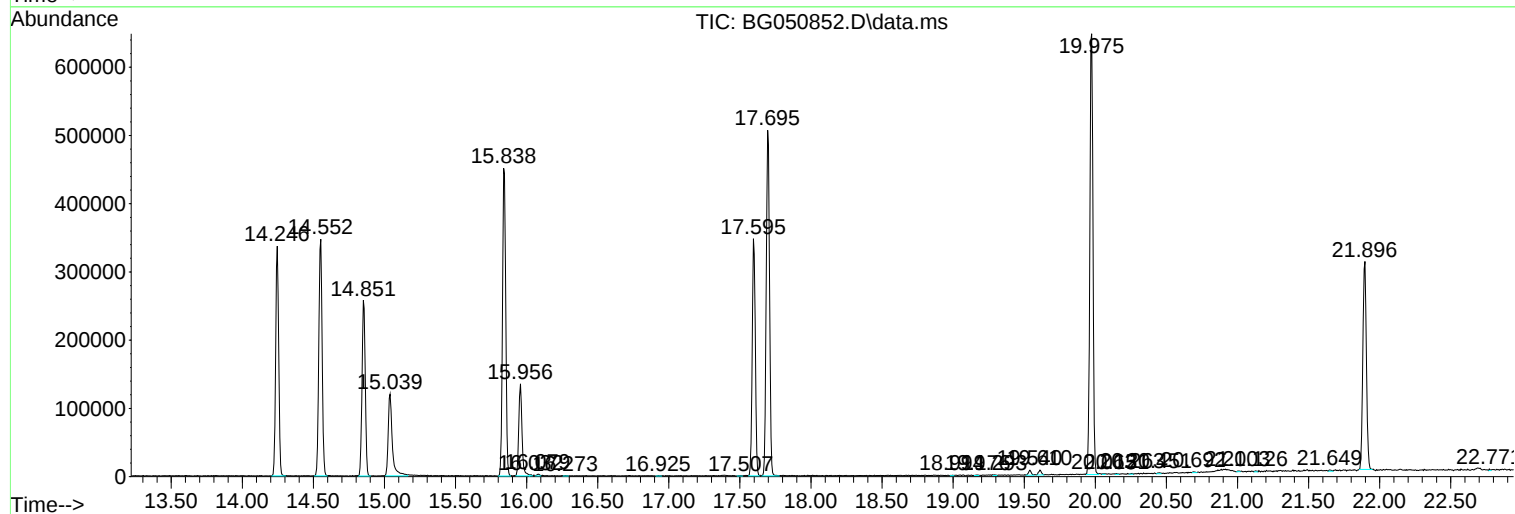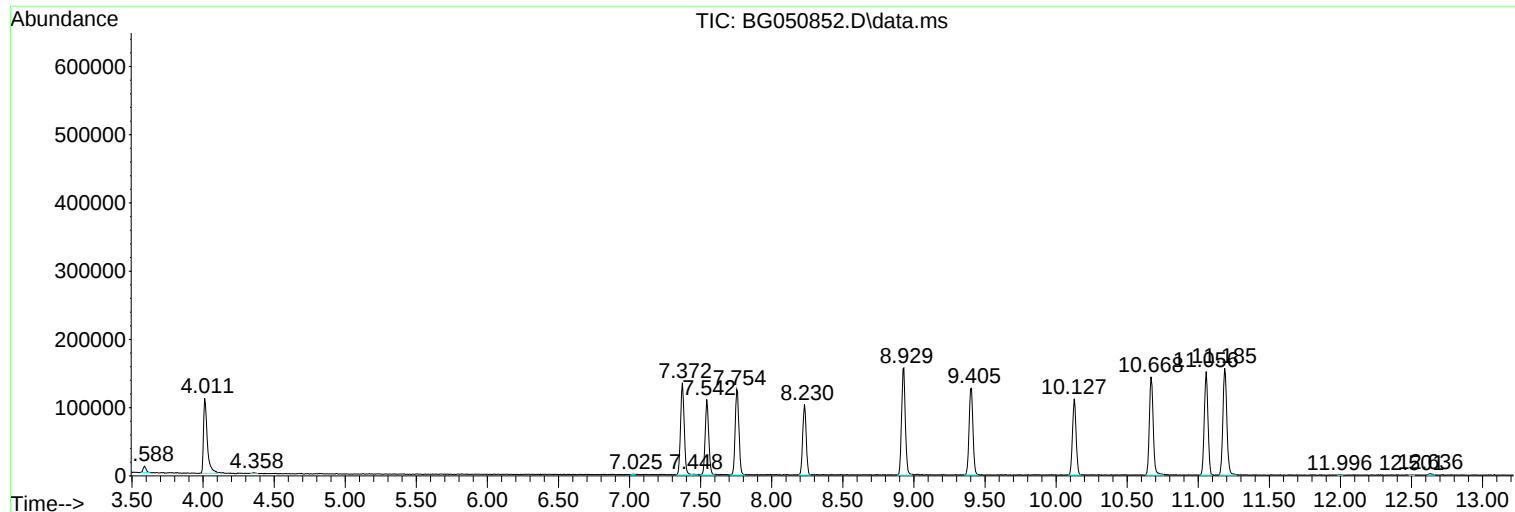

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050852.D
Acq On : 3 Nov 2021 16:14
Operator : CG/JU
Sample : PB140353BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050852.D
Acq On : 3 Nov 2021 16:14
Operator : CG/JU
Sample : PB140353BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------