

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050865.D
 Acq On : 4 Nov 2021 3:09
 Operator : CG/JU
 Sample : PB140458BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK458

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.587	13	17	23	rVB	10027	14829	1.40%	0.141%
2	4.010	85	89	108	rBV	126020	230000	21.76%	2.192%
3	4.363	144	149	155	rVB4	2113	3810	0.36%	0.036%
4	6.642	536	537	543	rVB3	699	1120	0.11%	0.011%
5	6.713	543	549	550	rBV2	699	1198	0.11%	0.011%
6	7.371	654	661	671	rBV	154733	273075	25.84%	2.603%
7	7.541	683	690	701	rVB	123101	209188	19.79%	1.994%
8	7.753	719	726	736	rVB	143416	253850	24.02%	2.420%
9	8.229	801	807	814	rBV	106434	179561	16.99%	1.712%
10	8.922	918	925	934	rBV	181294	325252	30.77%	3.100%
11	9.398	998	1006	1022	rVB	147347	273997	25.92%	2.612%
12	10.126	1123	1130	1140	rVB	124472	226971	21.47%	2.163%
13	10.667	1214	1222	1236	rBV	169357	312114	29.53%	2.975%
14	11.055	1280	1288	1296	rVB	155836	285453	27.01%	2.721%
15	11.184	1303	1310	1325	rBV	177898	345506	32.69%	3.293%
16	12.624	1551	1555	1561	rBV3	2477	4359	0.41%	0.042%
17	14.245	1824	1831	1839	rVB	369582	539827	51.07%	5.145%
18	14.551	1875	1883	1890	rBV	387414	634798	60.06%	6.051%
19	14.850	1926	1934	1942	rBV	269950	422548	39.98%	4.028%
20	15.038	1959	1966	1988	rBV	130539	259647	24.57%	2.475%
21	15.843	2094	2103	2110	rBV	487165	789696	74.71%	7.527%
22	15.955	2116	2122	2132	rBV	148477	235727	22.30%	2.247%
23	16.084	2140	2144	2148	rVB3	1116	1984	0.19%	0.019%
24	17.594	2394	2401	2408	rBV	360779	538264	50.93%	5.131%
25	17.694	2411	2418	2429	rVB	594985	900862	85.23%	8.587%
26	19.539	2727	2732	2737	rBV2	7519	11006	1.04%	0.105%
27	19.609	2739	2744	2750	rVB	6423	10355	0.98%	0.099%
28	19.974	2799	2806	2815	rBV	740735	1056958	100.00%	10.075%
29	20.373	2872	2874	2876	rBV3	1358	1068	0.10%	0.010%
30	20.573	2906	2908	2912	rVB4	1163	1381	0.13%	0.013%
31	20.826	2947	2951	2952	rBV3	1633	2239	0.21%	0.021%
32	20.849	2953	2955	2957	rBV3	1551	1226	0.12%	0.012%
33	20.879	2958	2960	2961	rBV2	1789	1093	0.10%	0.010%
34	21.002	2980	2981	2984	rBV2	1371	1102	0.10%	0.011%
35	21.437	3053	3055	3057	rBV3	1666	1108	0.10%	0.011%
36	21.560	3074	3076	3079	rBV2	1276	1117	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
 Data File : BG050865.D
 Acq On : 4 Nov 2021 3:09
 Operator : CG/JU
 Sample : PB140458BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK458

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	21.889	3126	3132	3142	rBV2	314655	544347	51.50%	5.189%
38	22.030	3154	3156	3157	rBV3	1937	1346	0.13%	0.013%
39	22.060	3157	3161	3164	rVB4	2258	3100	0.29%	0.030%
40	22.506	3235	3237	3239	rVB2	3192	1789	0.17%	0.017%
41	22.782	3281	3284	3286	rBV3	2368	2957	0.28%	0.028%
42	23.229	3358	3360	3361	rBV2	1610	1563	0.15%	0.015%
43	23.481	3401	3403	3404	rBV2	1304	1345	0.13%	0.013%
44	23.511	3406	3408	3411	rBV3	2258	1817	0.17%	0.017%
45	23.734	3444	3446	3447	rBV	2513	1423	0.13%	0.014%
46	23.793	3454	3456	3459	rBV4	2238	1869	0.18%	0.018%
47	24.269	3534	3537	3539	rVB4	3650	4017	0.38%	0.038%
48	24.327	3545	3547	3549	rBV3	1927	1329	0.13%	0.013%
49	24.750	3617	3619	3620	rVB2	1860	1067	0.10%	0.010%
50	24.850	3634	3636	3638	rBV3	1438	1165	0.11%	0.011%
51	25.056	3660	3671	3682	rBV3	323443	948024	89.69%	9.036%
52	25.285	3700	3710	3723	rVB3	184068	555249	52.53%	5.292%
53	25.826	3800	3802	3805	rBV4	1499	1716	0.16%	0.016%
54	26.225	3869	3870	3872	rBV2	2379	1091	0.10%	0.010%
55	26.466	3905	3911	3917	rBV6	6795	15938	1.51%	0.152%
56	27.870	4148	4150	4151	rBV2	2214	1677	0.16%	0.016%
57	27.911	4152	4157	4165	rVB10	7528	17047	1.61%	0.162%
58	28.070	4182	4184	4186	rBV3	2387	2180	0.21%	0.021%
59	28.270	4216	4218	4219	rBV2	1887	1073	0.10%	0.010%
60	28.429	4243	4245	4247	rBV3	1573	1190	0.11%	0.011%
61	28.975	4336	4338	4340	rBV3	1625	1441	0.14%	0.014%
62	29.110	4359	4361	4363	rBV3	1648	1092	0.10%	0.010%
63	29.157	4367	4369	4371	rBV2	2466	2481	0.23%	0.024%
64	29.427	4413	4415	4416	rBV	1997	1071	0.10%	0.010%
65	29.604	4441	4445	4446	rBV4	2166	2521	0.24%	0.024%
66	29.639	4447	4451	4452	rBV3	3929	5201	0.49%	0.050%
67	30.115	4530	4532	4533	rBV2	1692	1645	0.16%	0.016%
68	30.409	4580	4582	4585	rVB4	1867	1738	0.16%	0.017%
69	30.685	4627	4629	4630	rBV2	1849	1151	0.11%	0.011%
70	30.837	4653	4655	4657	rBV2	1639	1225	0.12%	0.012%
71	31.237	4719	4723	4726	rVB5	2093	2613	0.25%	0.025%
72	31.443	4755	4758	4760	rBV4	2115	2518	0.24%	0.024%




Sum of corrected areas: 10491305

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050865.D
Acq On : 4 Nov 2021 3:09
Operator : CG/JU
Sample : PB140458BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK458

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

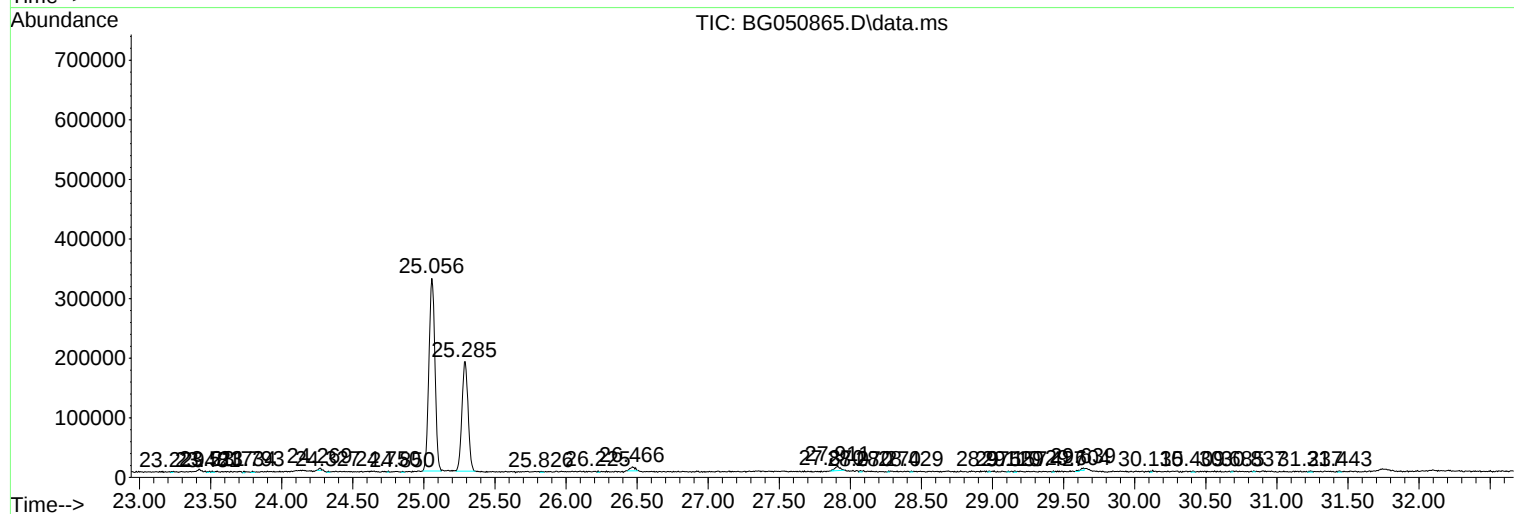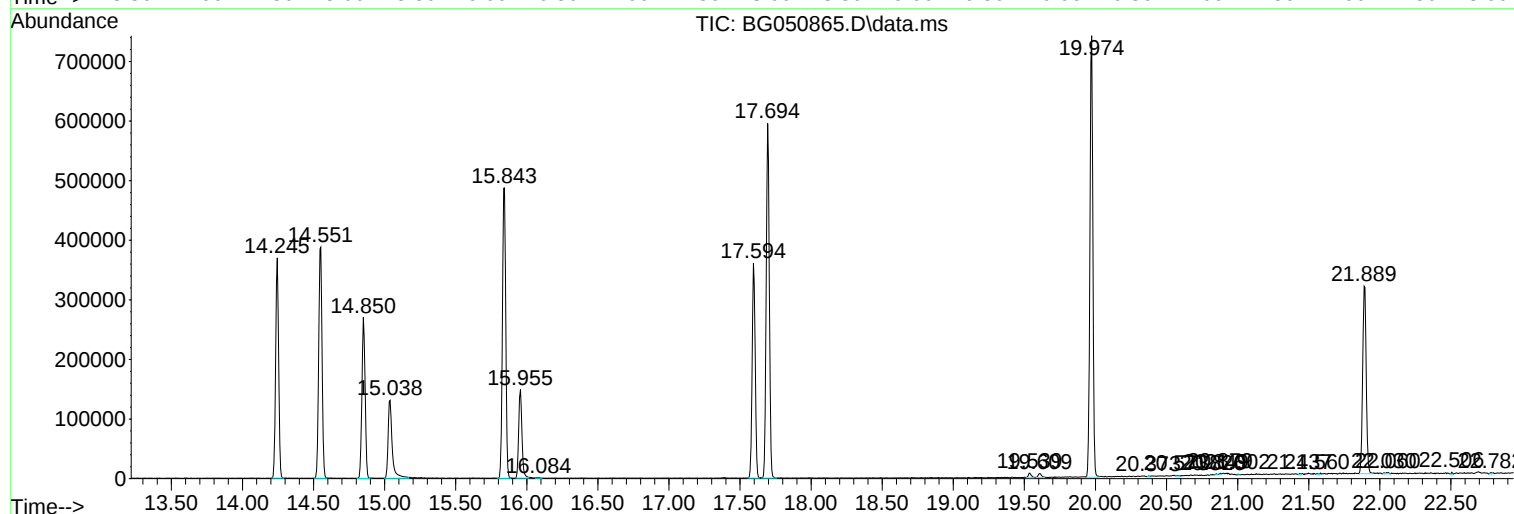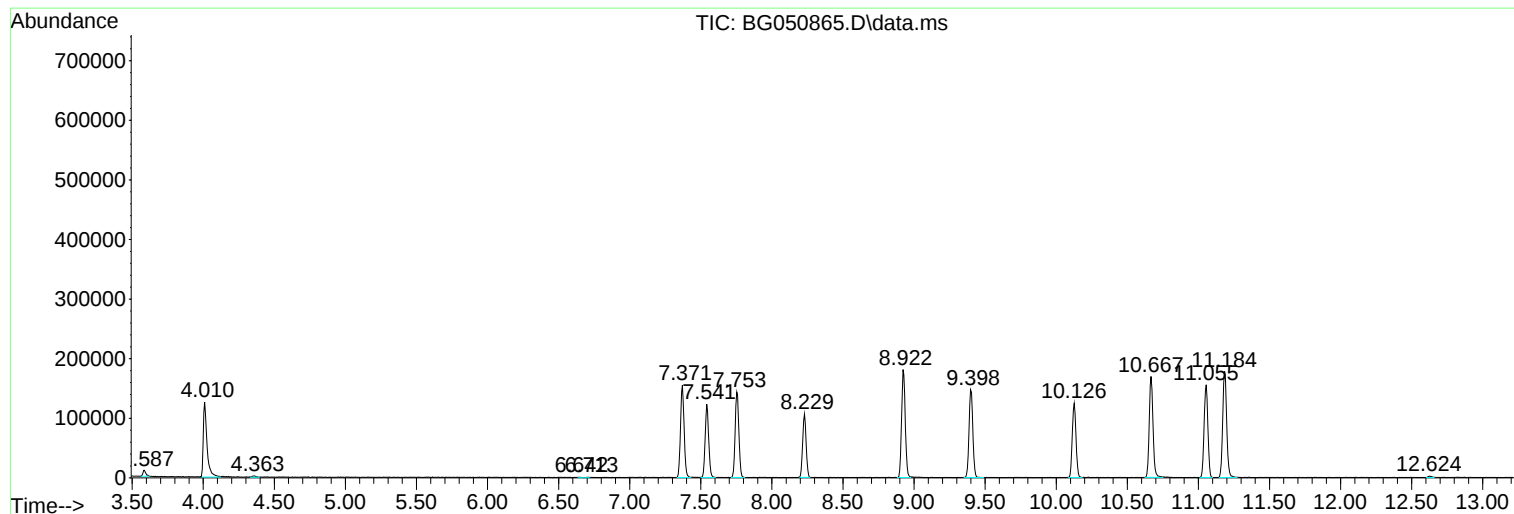

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050865.D
Acq On : 4 Nov 2021 3:09
Operator : CG/JU
Sample : PB140458BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK458

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110321\
Data File : BG050865.D
Acq On : 4 Nov 2021 3:09
Operator : CG/JU
Sample : PB140458BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK458

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc