
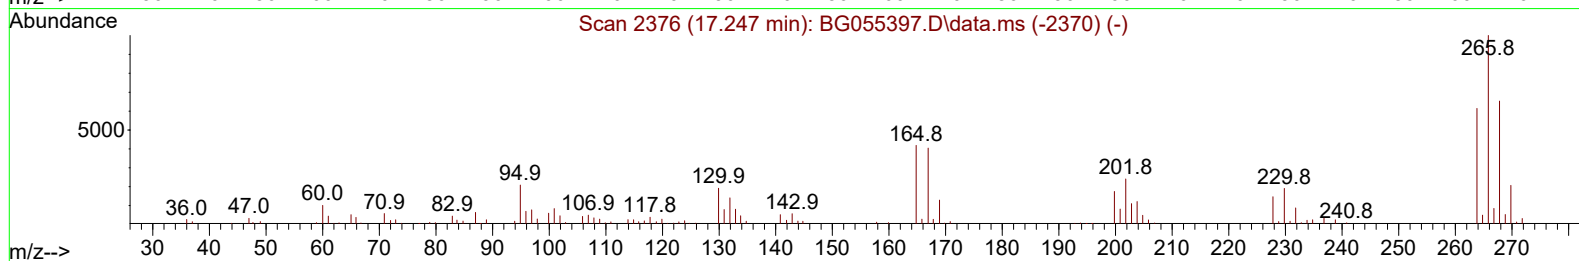
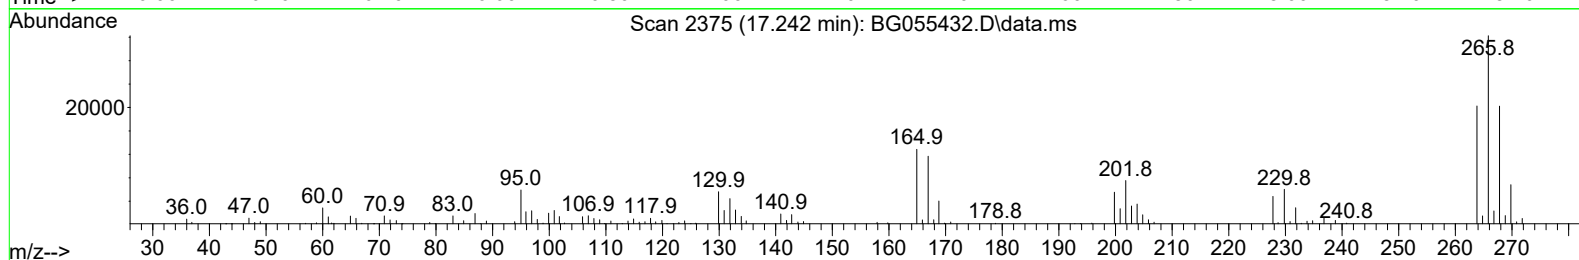


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110322\
Data File : BG055432.D
Acq On : 3 Nov 2022 10:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 08:20:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 05:28:43 2022
Response via : Initial Calibration

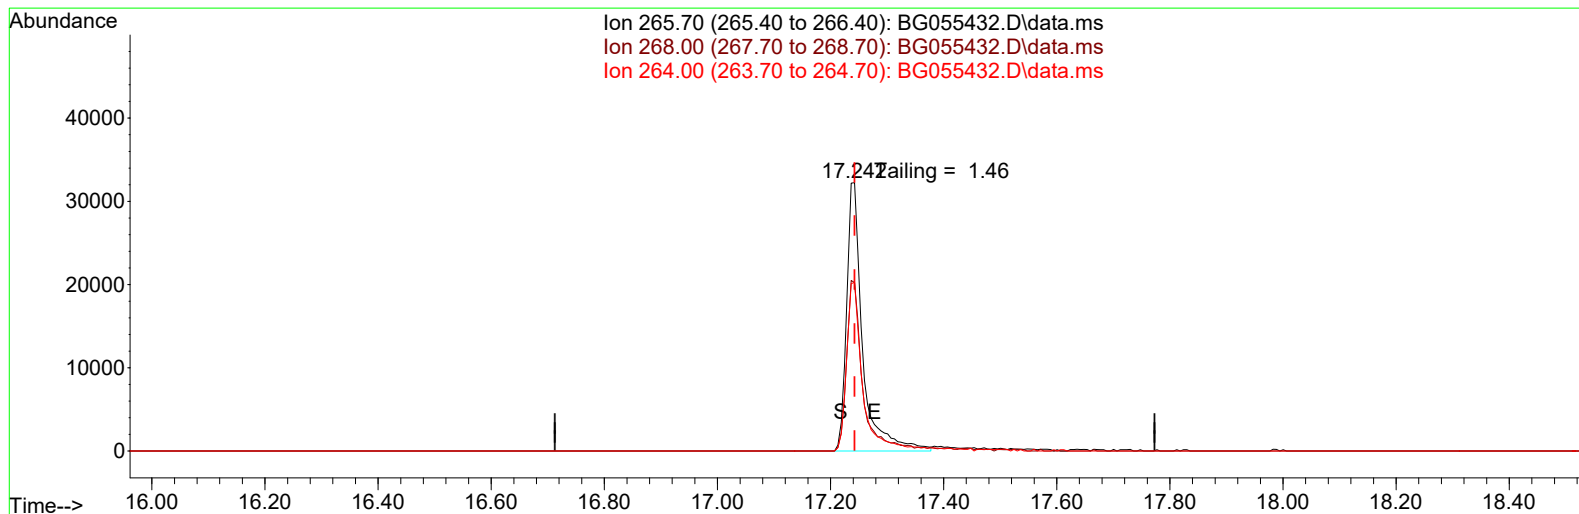

TIC: BG055432.D\data.ms

(70) Pentachlorophenol (C)




17.242min (-0.000) 43523.91 ng

response 63867

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.71
264.00	61.50	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110322\
 Data File : BG055432.D
 Acq On : 3 Nov 2022 10:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 08:20:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 05:28:43 2022
 Response via : Initial Calibration

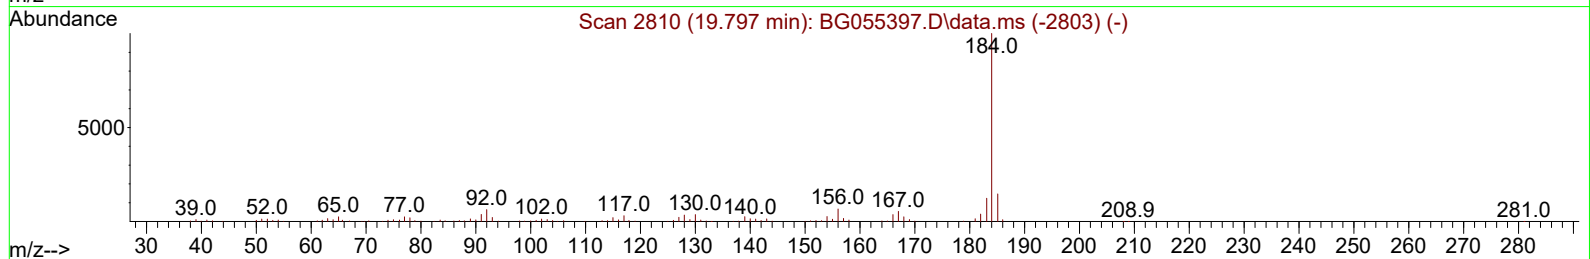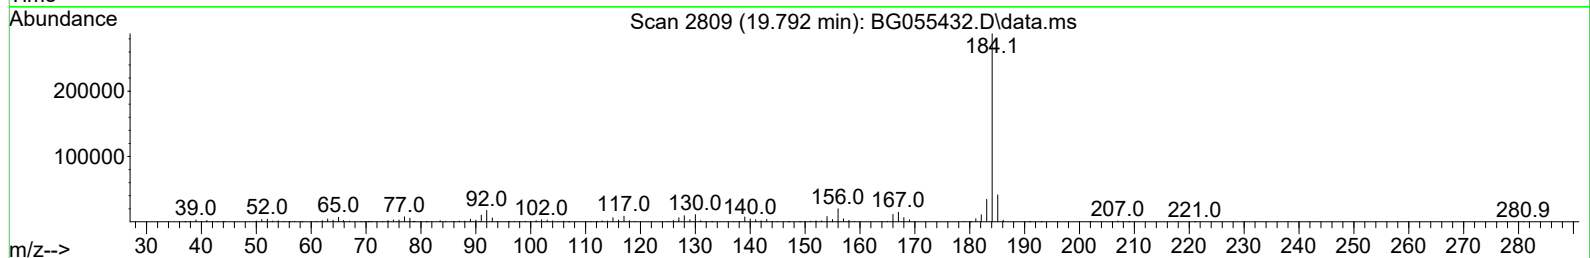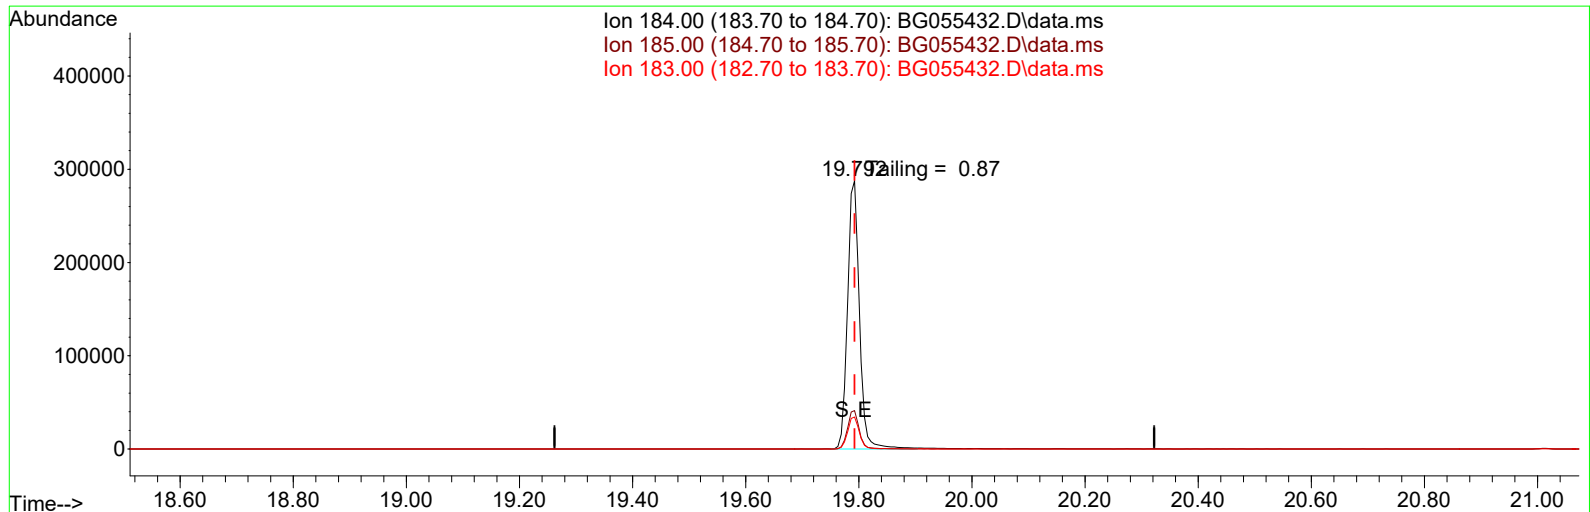

TIC: BG055432.D\data.ms

(77) Benzidine

19.792min (-0.000) 71579.79 ng

response 424719

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.35
183.00	12.30	11.93
0.00	0.00	0.00