


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110322\
 Data File : BG055432.D
 Acq On : 3 Nov 2022 10:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 04 05:28:43 2022

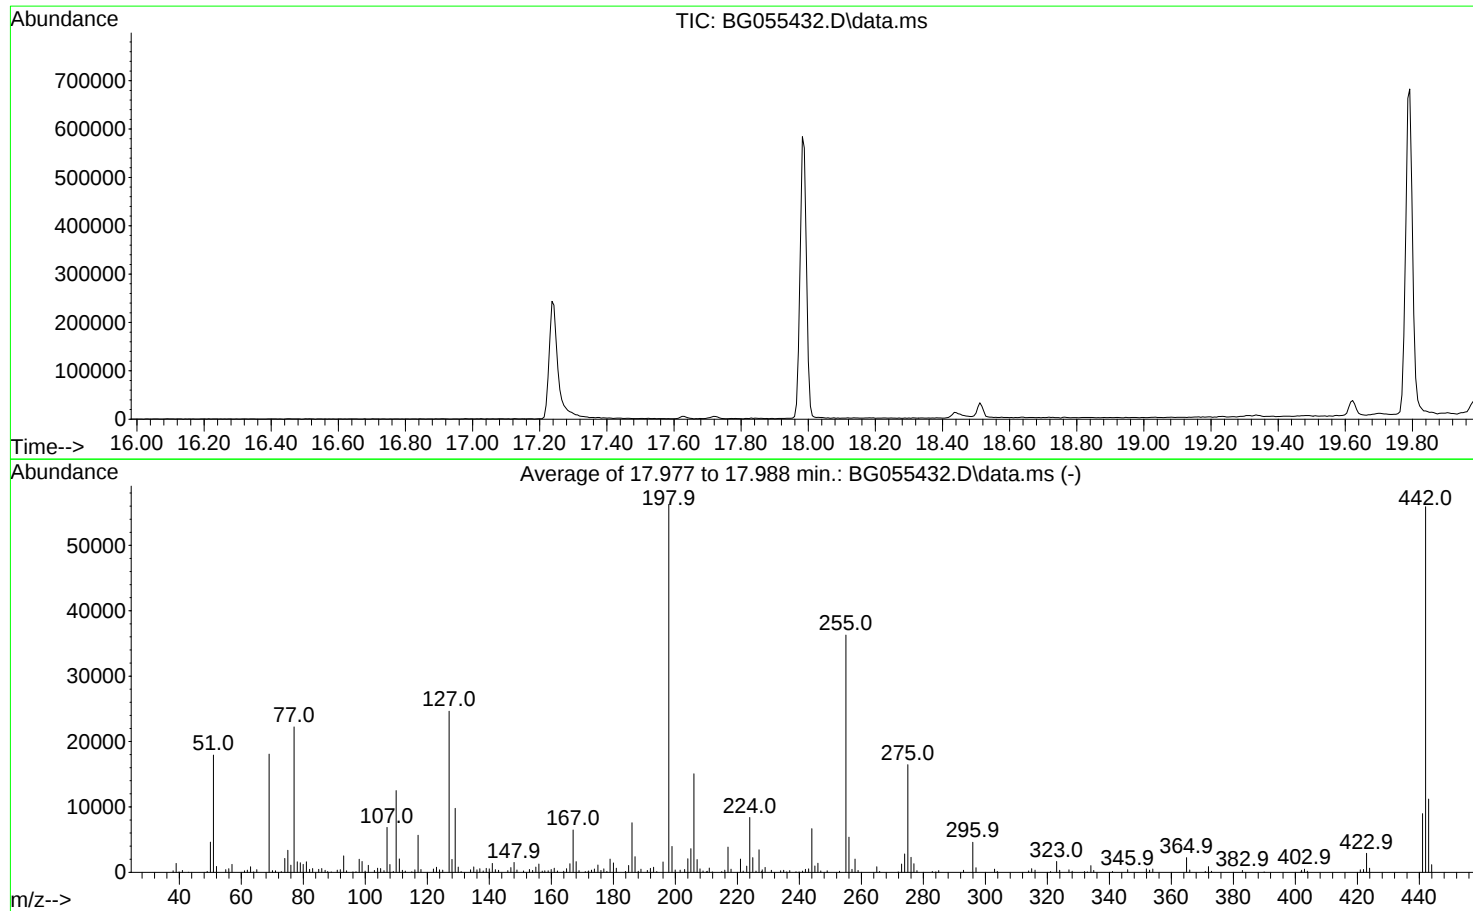




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	17938	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	18082	PASS
70	69	0.00	2	1.4	260	PASS
127	198	10	80	43.8	24643	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56261	PASS
199	198	5	9	7.0	3952	PASS
275	198	10	60	29.2	16455	PASS
365	198	1	100	4.0	2236	PASS
441	198	0.01	100	15.9	8959	PASS
442	442	50	100	100.0	55912	PASS
443	442	15	24	20.0	11188	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110322\
Data File : BG055432.D
Acq On : 3 Nov 2022 10:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 04 08:20:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 05:28:43 2022
Response via : Initial Calibration

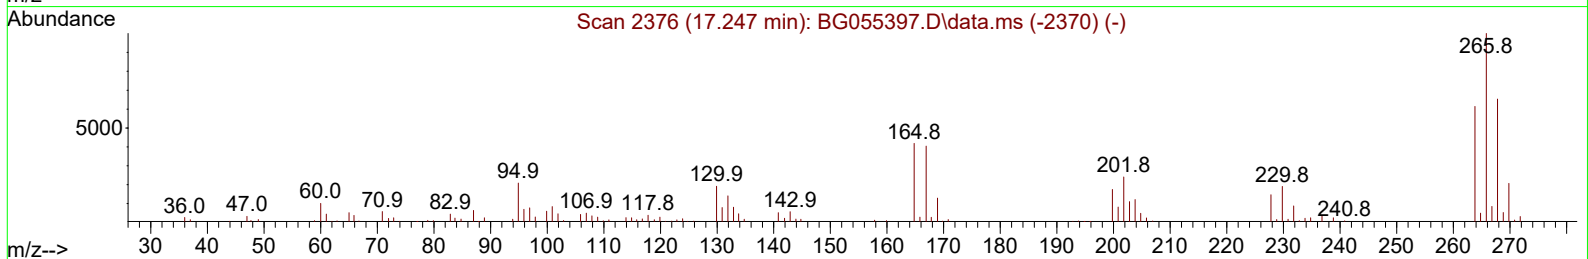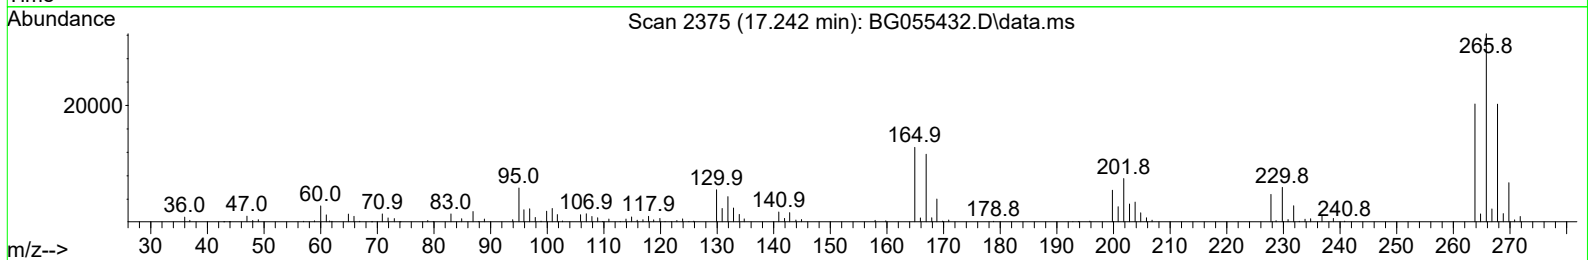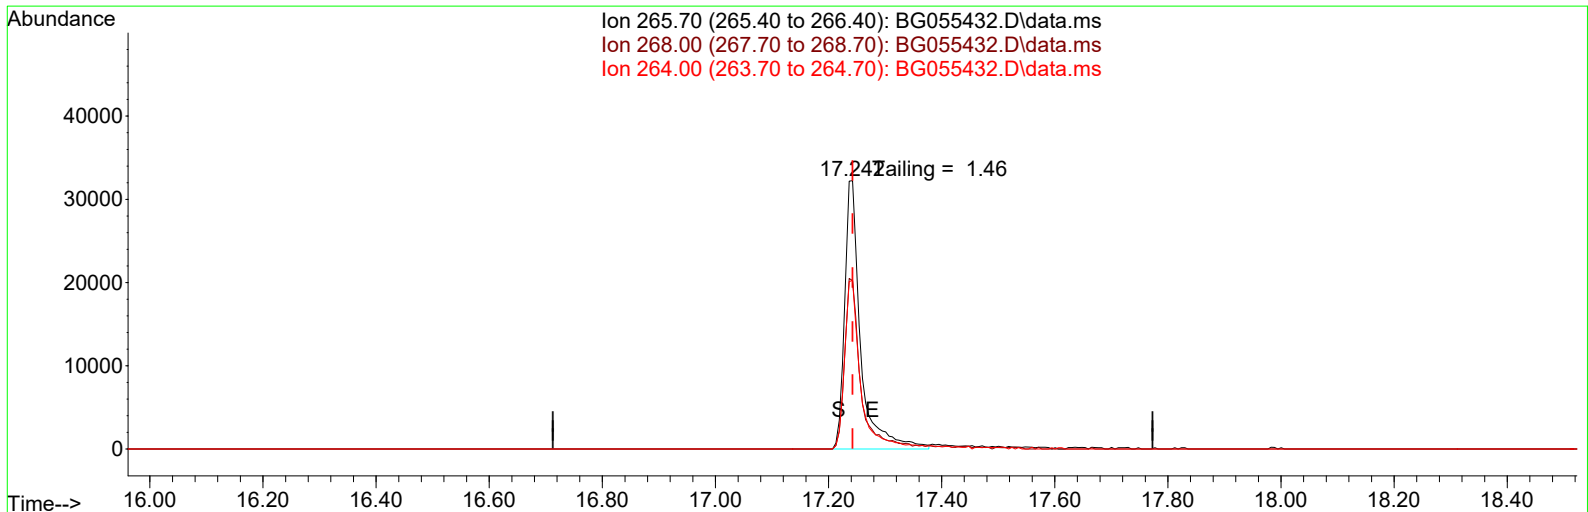

TIC: BG055432.D\data.ms

(70) Pentachlorophenol (C)

17.242min (-0.000) 43523.91 ng




response 63867

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.71
264.00	61.50	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110322\
Data File : BG055432.D
Acq On : 3 Nov 2022 10:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 04 08:20:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 05:28:43 2022
Response via : Initial Calibration

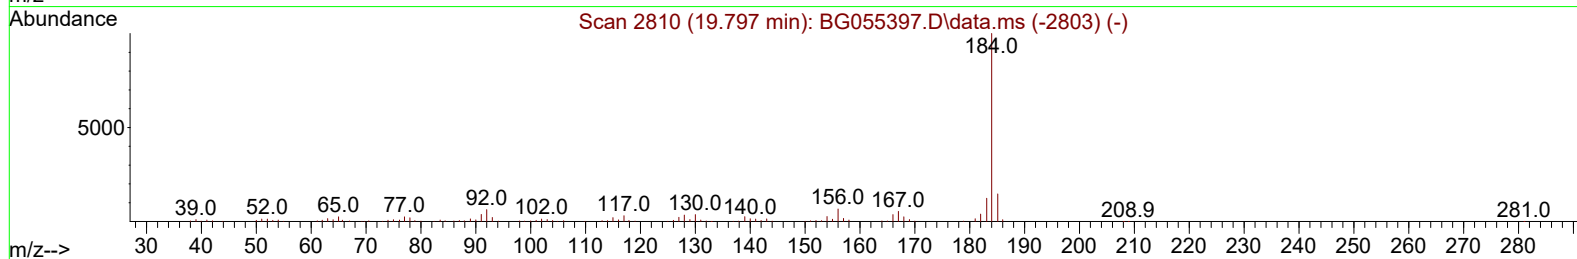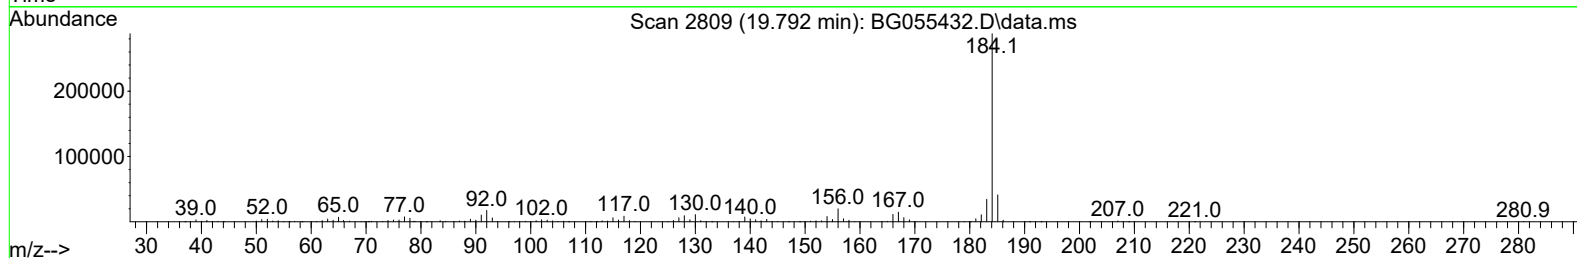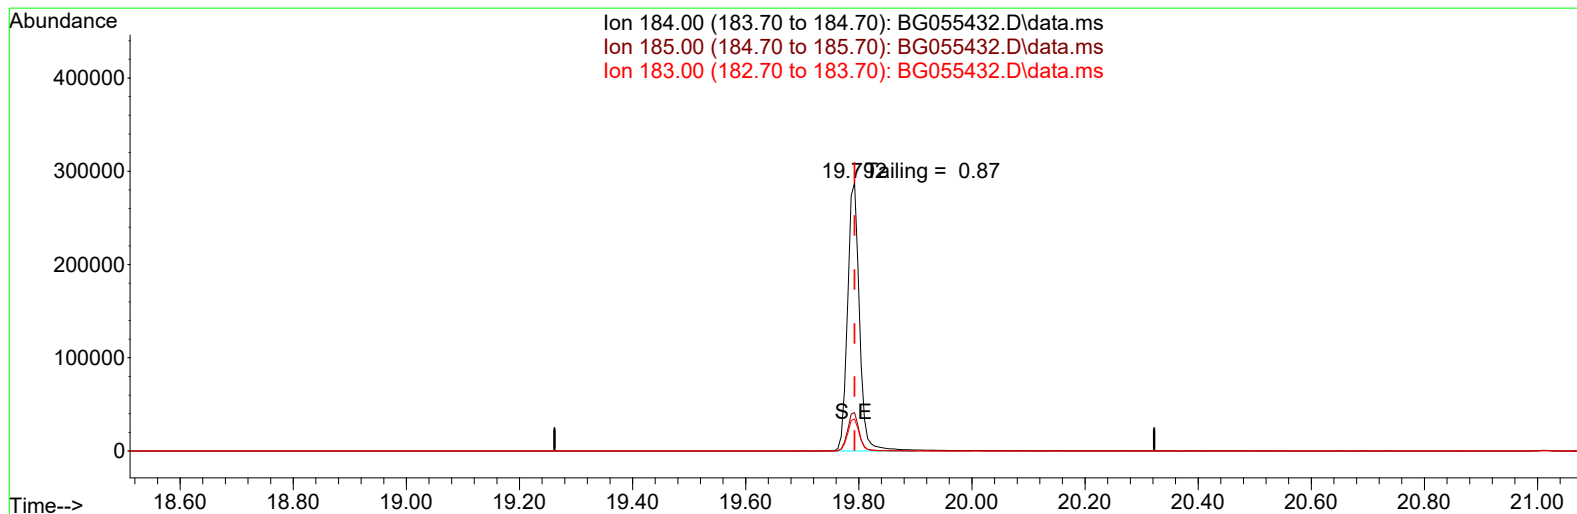

TIC: BG055432.D\data.ms

(77) Benzidine

19.792min (-0.000) 71579.79 ng

response 424719

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.35
183.00	12.30	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2022	BNA_G	<u>BG055432.D</u>
Compound Name	Response	Retention Time
DDT	208208	21.014
DDD	3852	20.615
DDE	165	20.157
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4017	212225	1.89

Instrument :
BNA_G
ClientSampleId :
DFTPP