
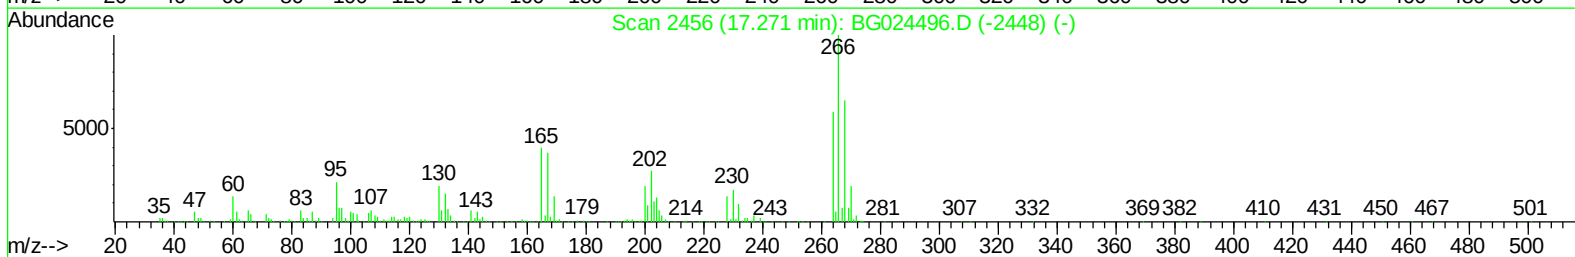
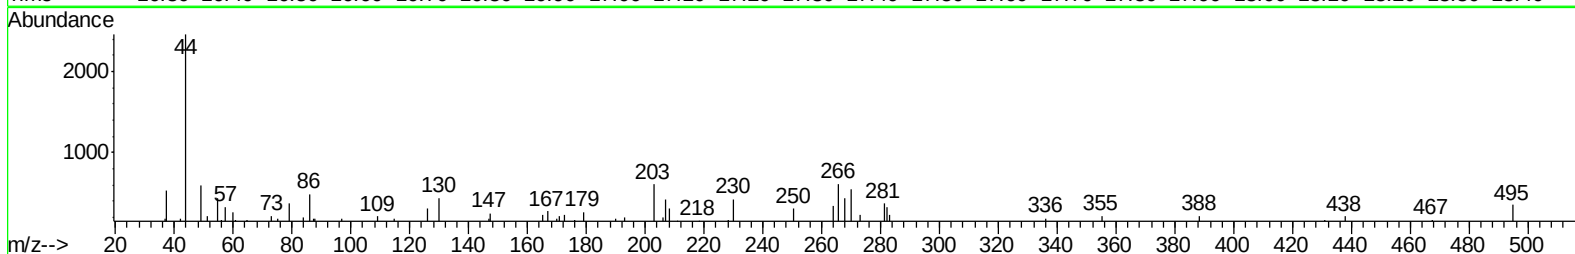


Data Path : Z:\HPCHEM1\BNA_G\Data\BG110416\
Data File : BG024702.D
Acq On : 5 Nov 2016 8:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 01:21:54 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

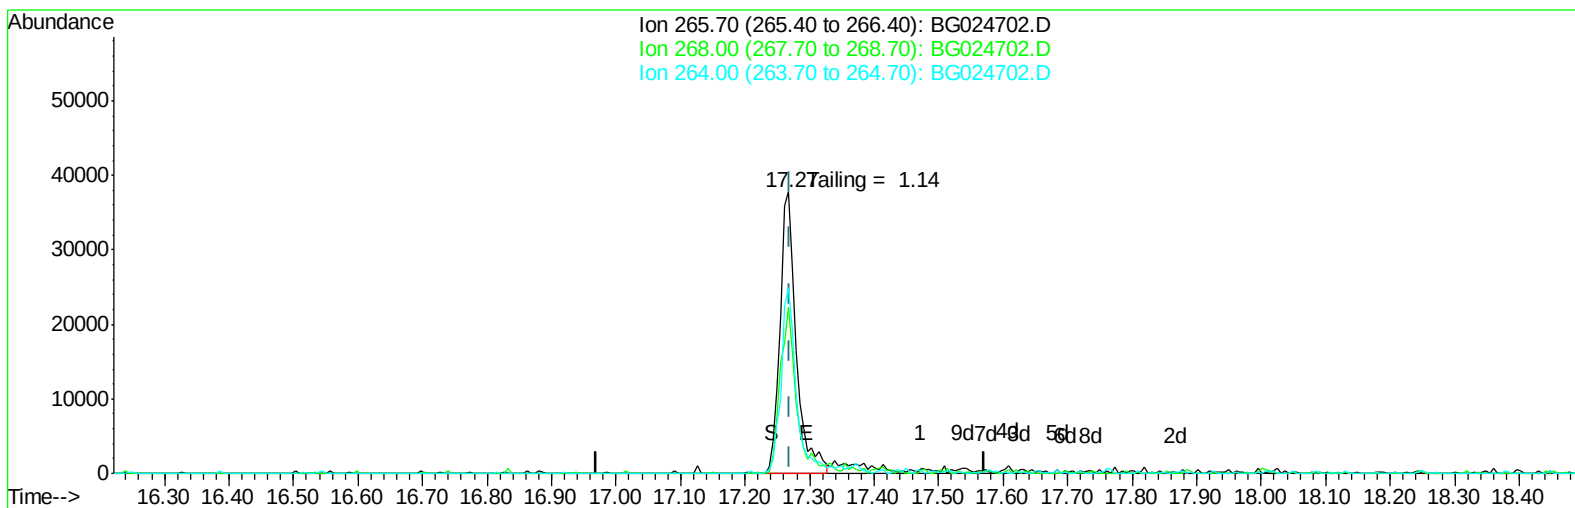

TIC: BG024702.D

(69) Pentachlorophenol (C)




17.473min (+0.202) 86.29ng

response 401

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	72.15
264.00	62.60	56.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110416\
Data File : BG024702.D
Acq On : 5 Nov 2016 8:13
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 01:21:54 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

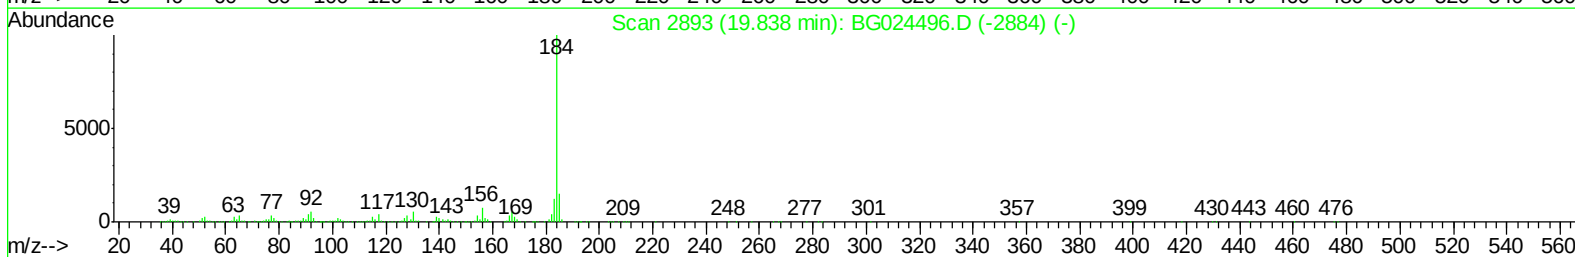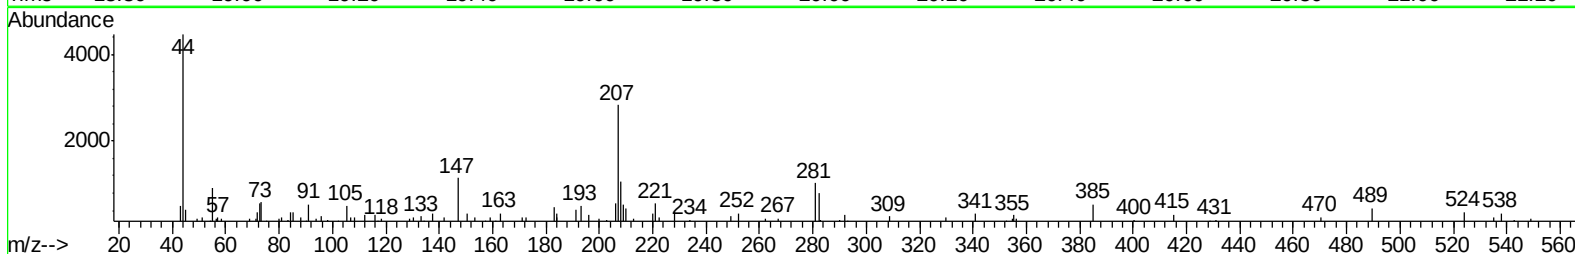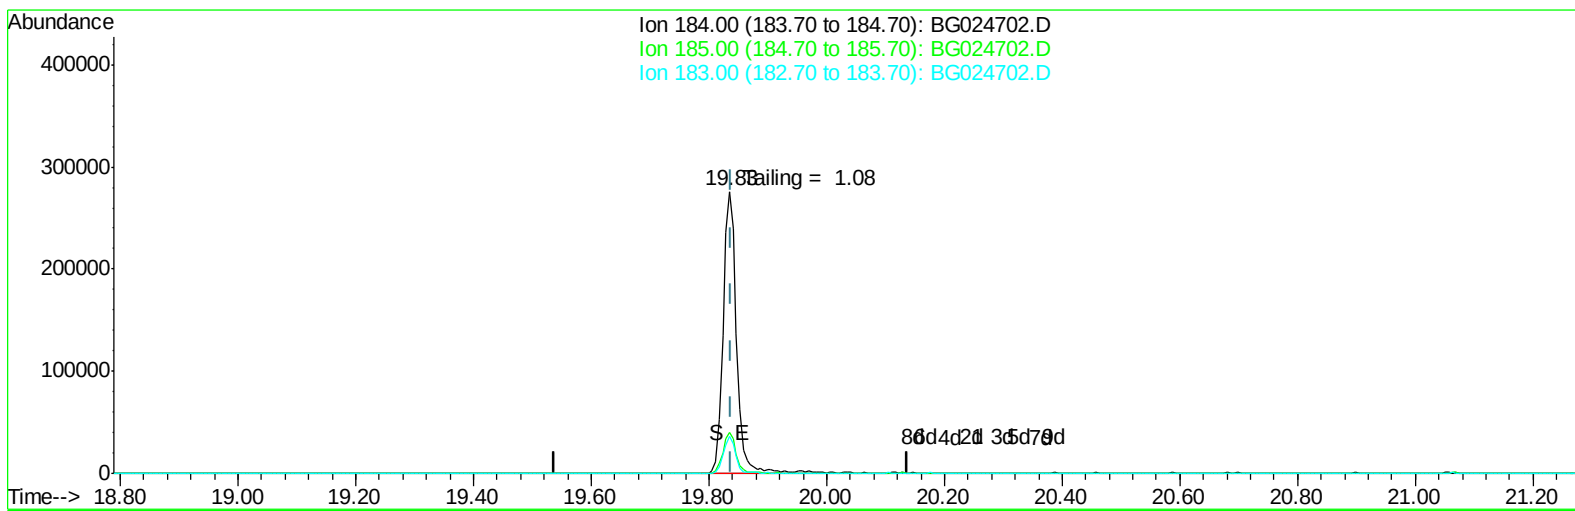

TIC: BG024702.D

(76) Benzidine

20.258min (+0.419) 276.16ng

response 488

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	0.00#
183.00	13.80	82.05#
0.00	0.00	0.00