


Data Path : Z:\HPCHEM1\BNA G\DATA\BG110416\
Data File : BG024684.D
Acq On : 4 Nov 2016 20:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 26 11:14:13 2016

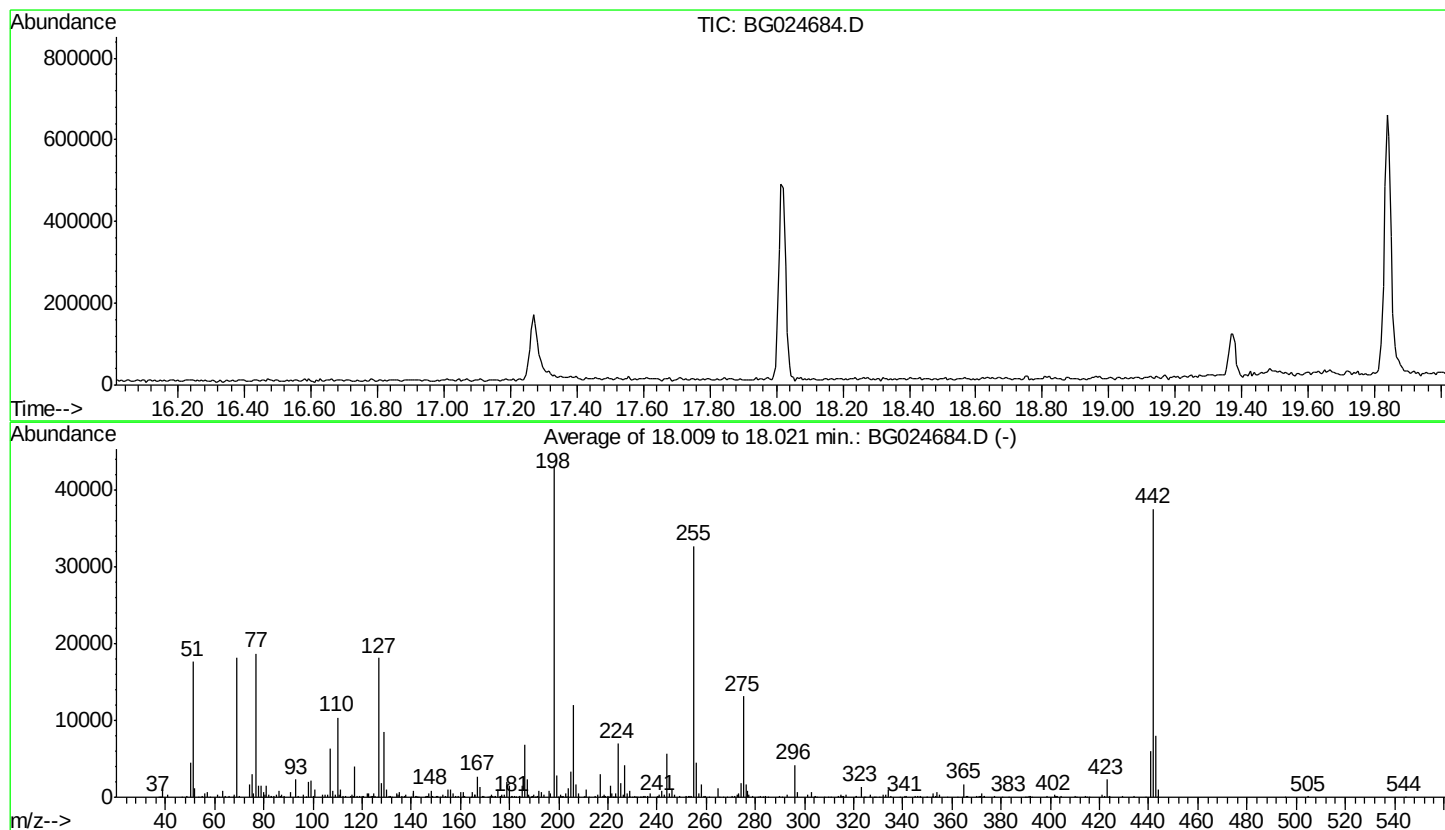

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	17620	PASS
68	69	0.00	2	2.0	362	PASS
69	198	0.00	100	41.9	18132	PASS
70	69	0.00	2	1.2	217	PASS
127	198	10	80	41.9	18130	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43224	PASS
199	198	5	9	6.4	2762	PASS
275	198	10	60	30.4	13146	PASS
365	198	1	100	3.9	1692	PASS
441	442	0.01	24	16.1	6066	PASS
442	198	50	100	86.9	37573	PASS
443	442	15	24	21.3	7997	PASS