


Data Path : Z:\HPCHEM1\BNA G\DATA\BG110416\
 Data File : BG024702.D
 Acq On : 5 Nov 2016 8:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

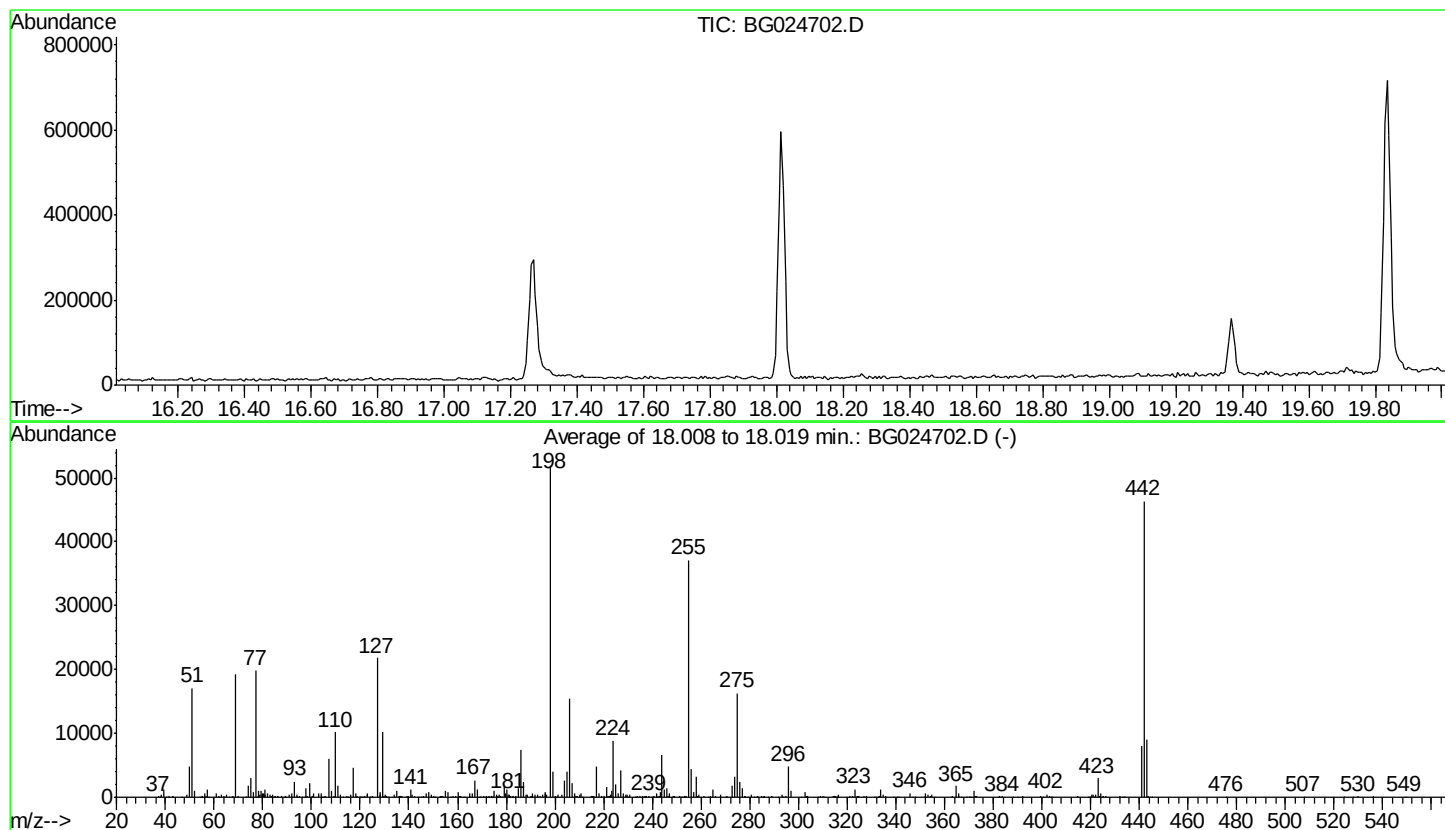

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	17117	PASS
68	69	0.00	2	0.7	143	PASS
69	198	0.00	100	37.2	19298	PASS
70	69	0.00	2	0.8	162	PASS
127	198	10	80	42.0	21829	PASS
197	198	0.00	2	0.7	352	PASS
198	198	100	100	100.0	51928	PASS
199	198	5	9	7.6	3925	PASS
275	198	10	60	31.4	16281	PASS
365	198	1	100	3.4	1744	PASS
441	442	0.01	24	17.2	7973	PASS
442	198	50	100	89.4	46410	PASS
443	442	15	24	19.6	9090	PASS