
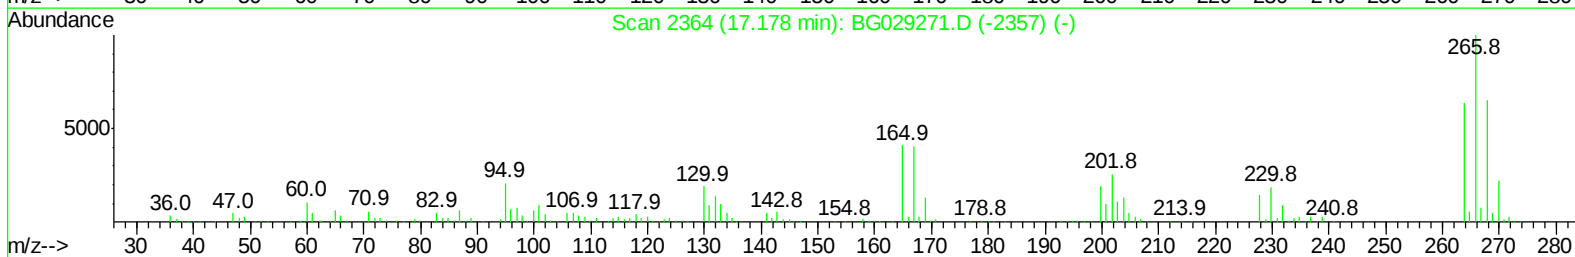
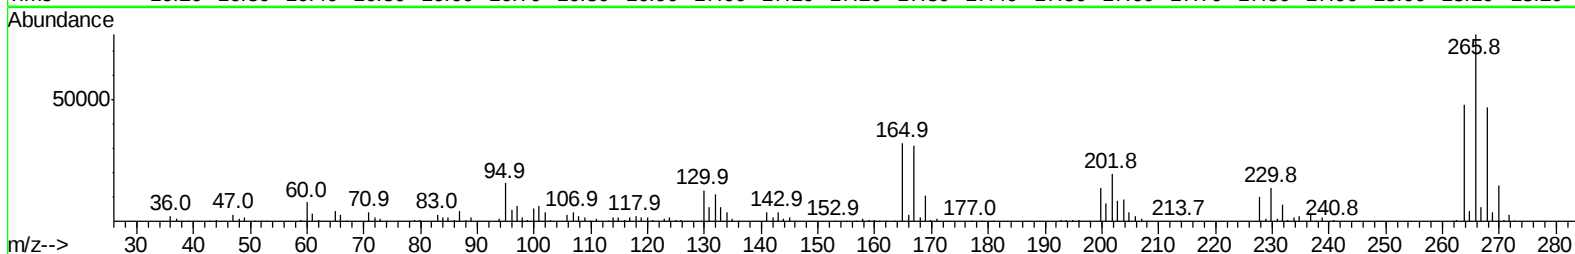


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110417\
Data File : BG030697.D
Acq On : 3 Nov 2017 13:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 07:10:48 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 18:14:01 2017
Response via : Initial Calibration

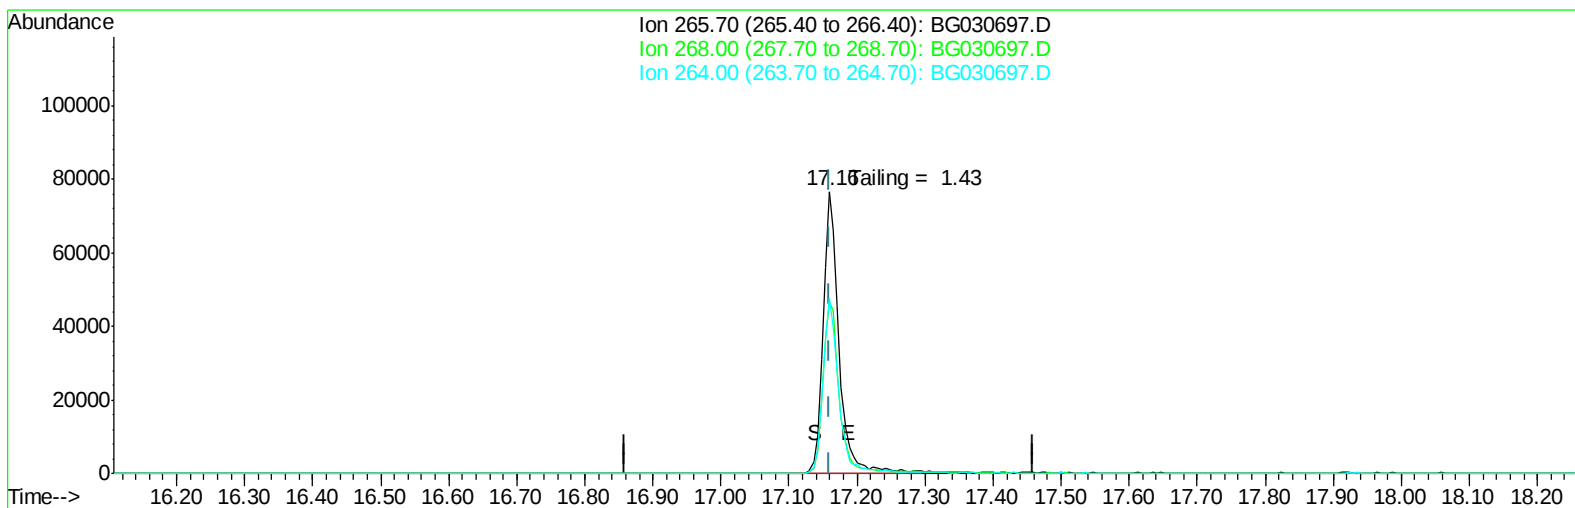

TIC: BG030697.D

(69) Pentachlorophenol (C)




17.159min (-0.000) 218983.01ng

response 124265

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.90
264.00	62.00	62.42
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110417\
Data File : BG030697.D
Acq On : 3 Nov 2017 13:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 07:10:48 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 18:14:01 2017
Response via : Initial Calibration

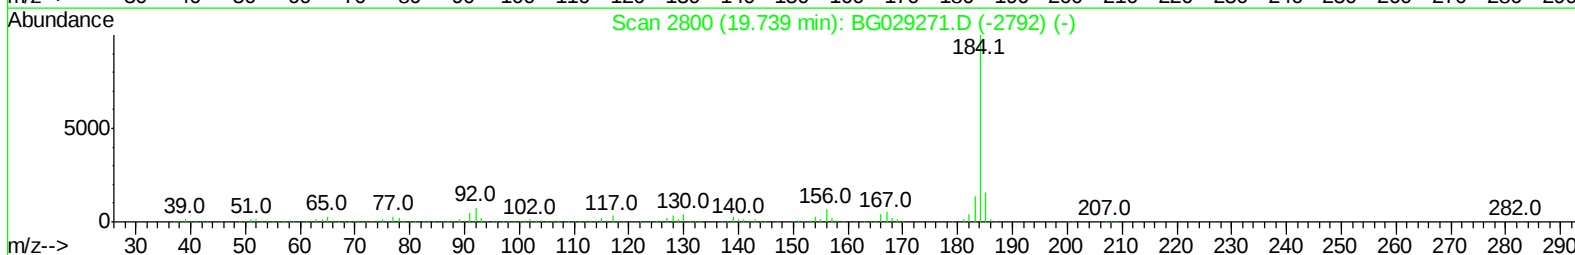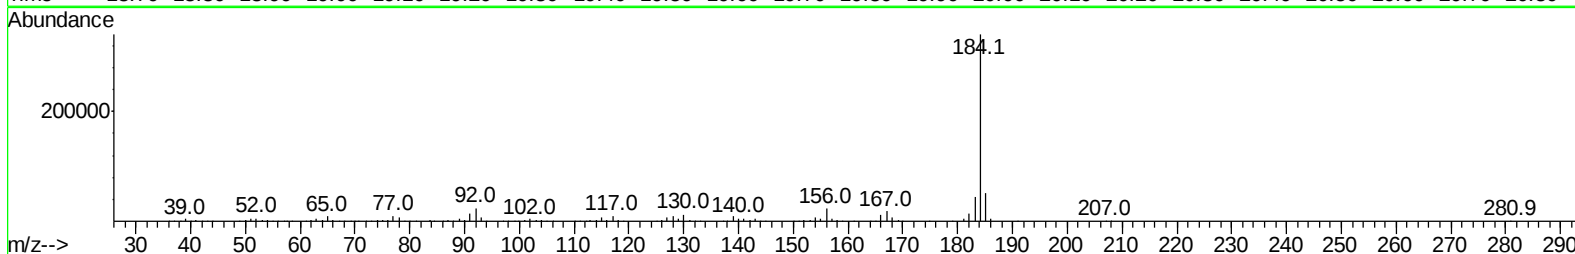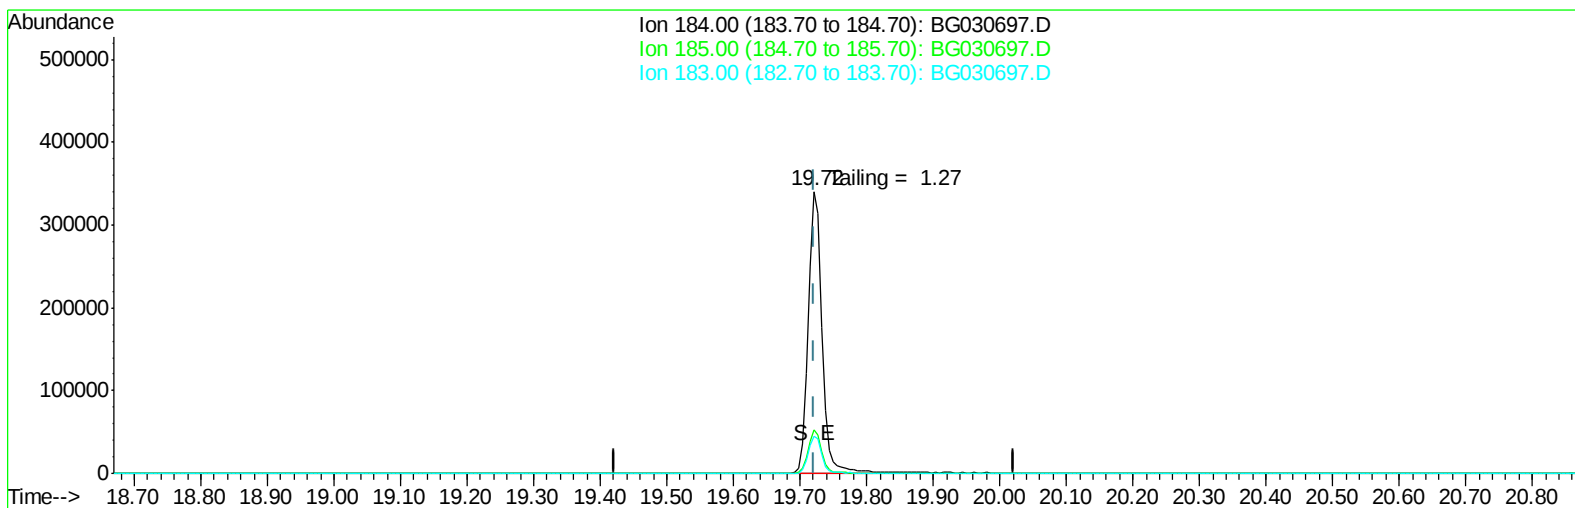

TIC: BG030697.D

(76) Benzidine

19.721min (-0.000) 0.00ng

response 502056

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.26
183.00	13.30	13.00
0.00	0.00	0.00