


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110417\
 Data File : BG030716.D
 Acq On : 4 Nov 2017 1:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 03 18:14:01 2017

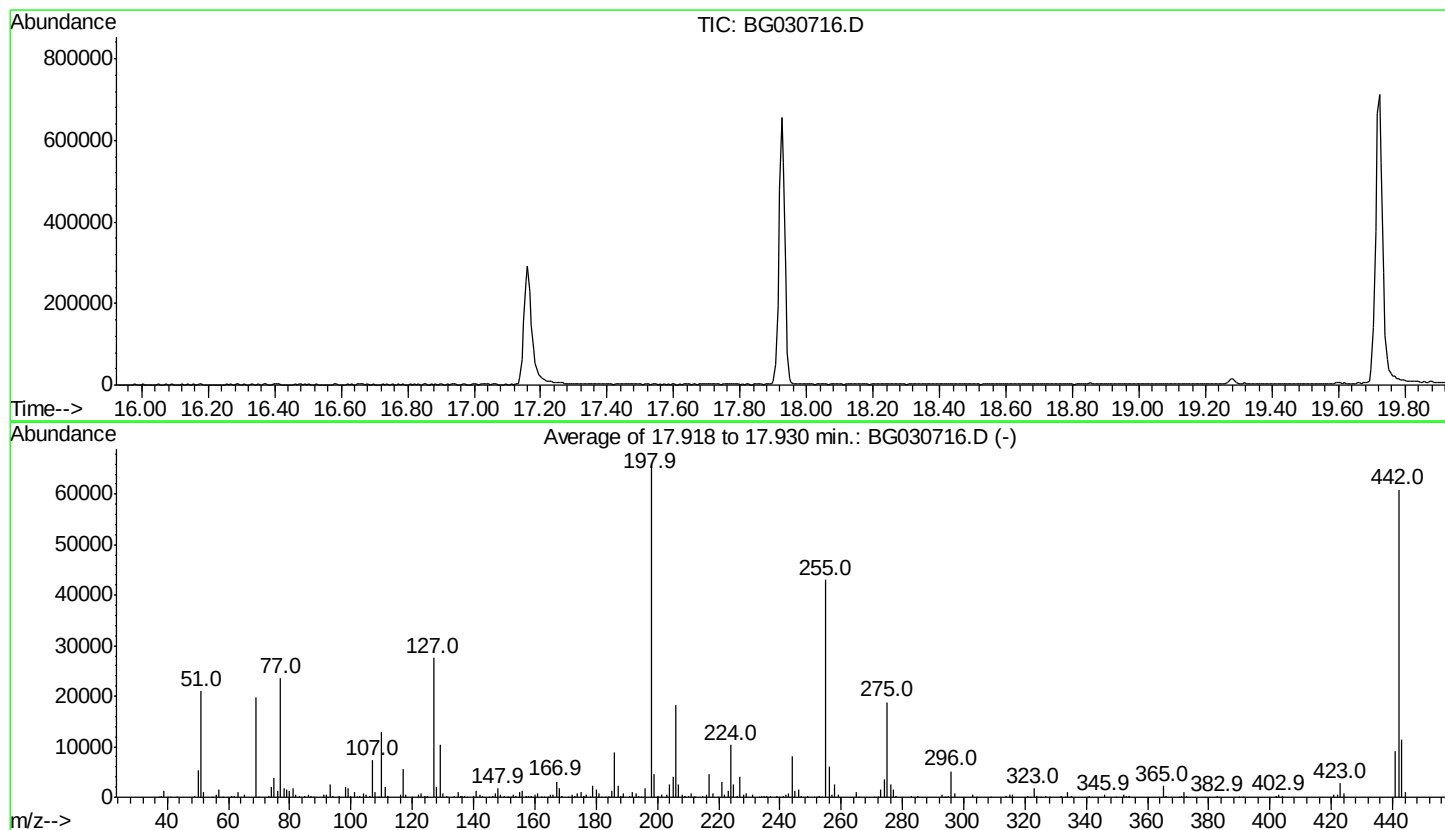

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	20957	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.1	19784	PASS
70	69	0.00	2	0.3	63	PASS
127	198	10	80	42.0	27576	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65669	PASS
199	198	5	9	6.9	4559	PASS
275	198	10	60	28.6	18772	PASS
365	198	1	100	3.3	2177	PASS
441	442	0.01	24	15.2	9235	PASS
442	198	50	100	92.8	60917	PASS
443	442	15	24	18.6	11361	PASS