
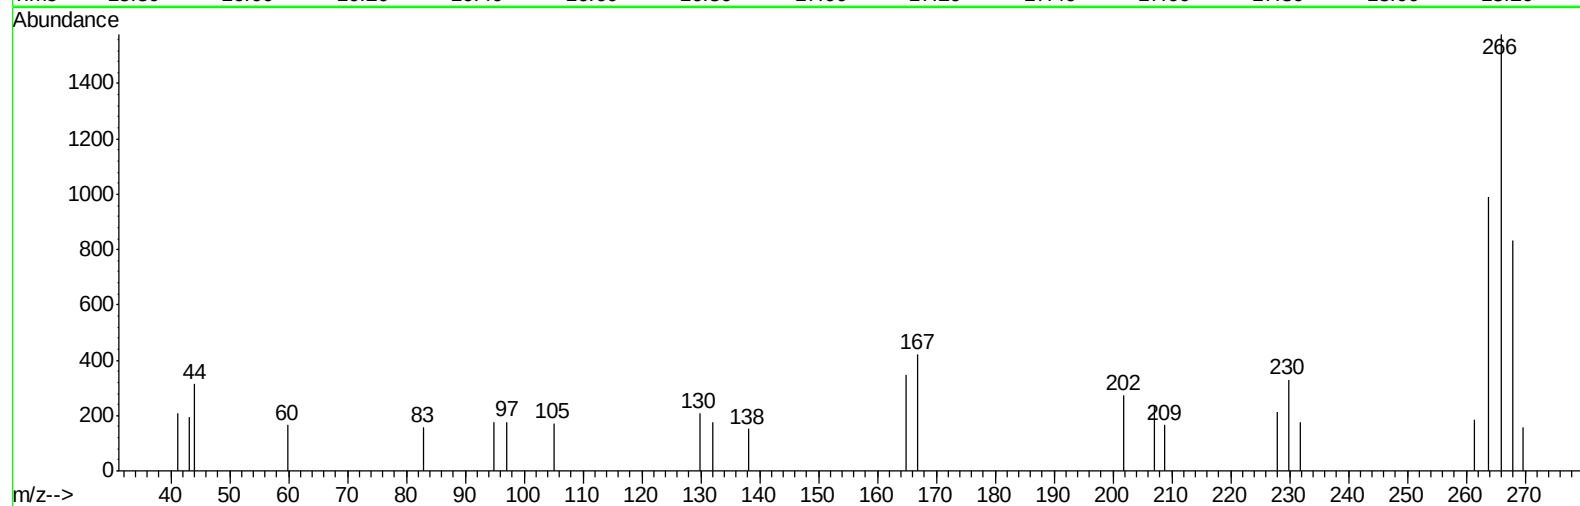


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110419\
Data File : BG043497.D
Acq On : 5 Nov 2019 2:11
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 07:49:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

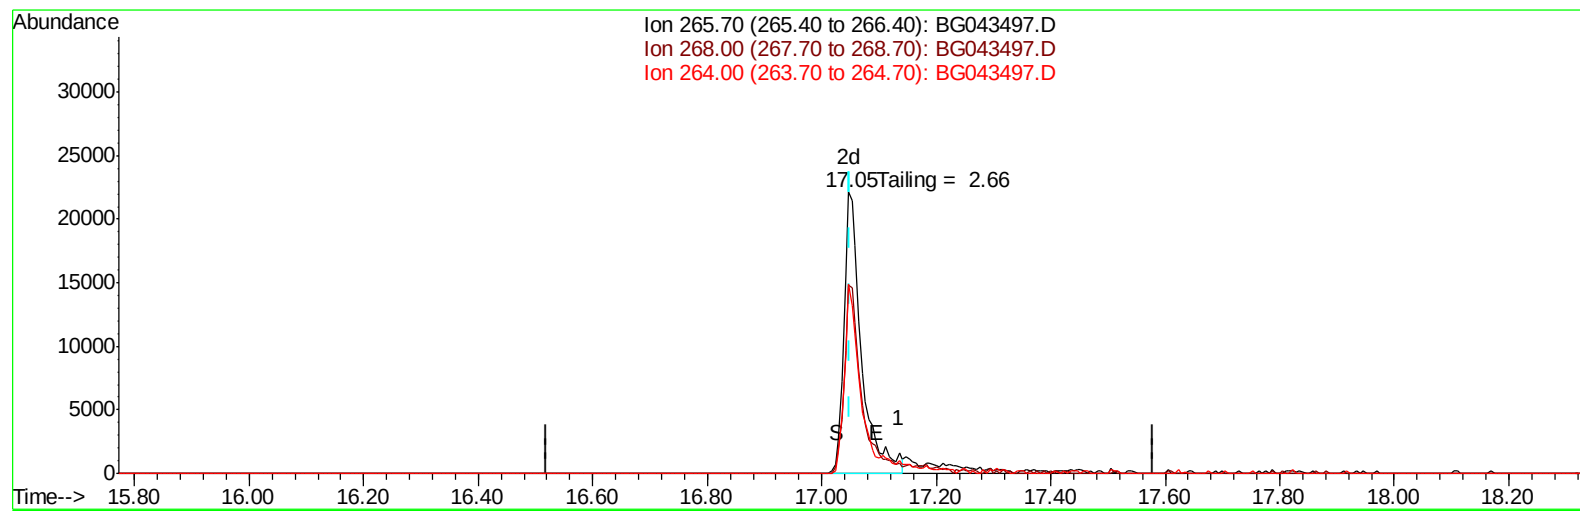

TIC: BG043497.D

(70) Pentachlorophenol (C)



17.135min (+0.085) 617.82ng

response 1496

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	52.92
264.00	61.10	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110419\
Data File : BG043497.D
Acq On : 5 Nov 2019 2:11
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 07:49:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

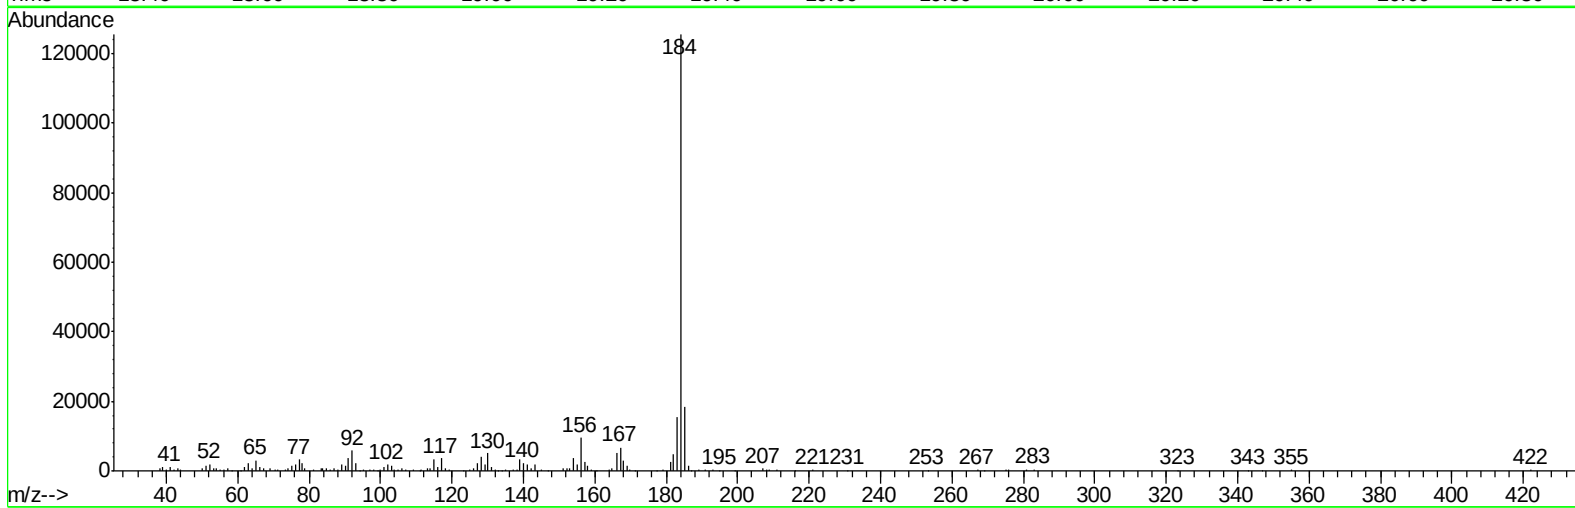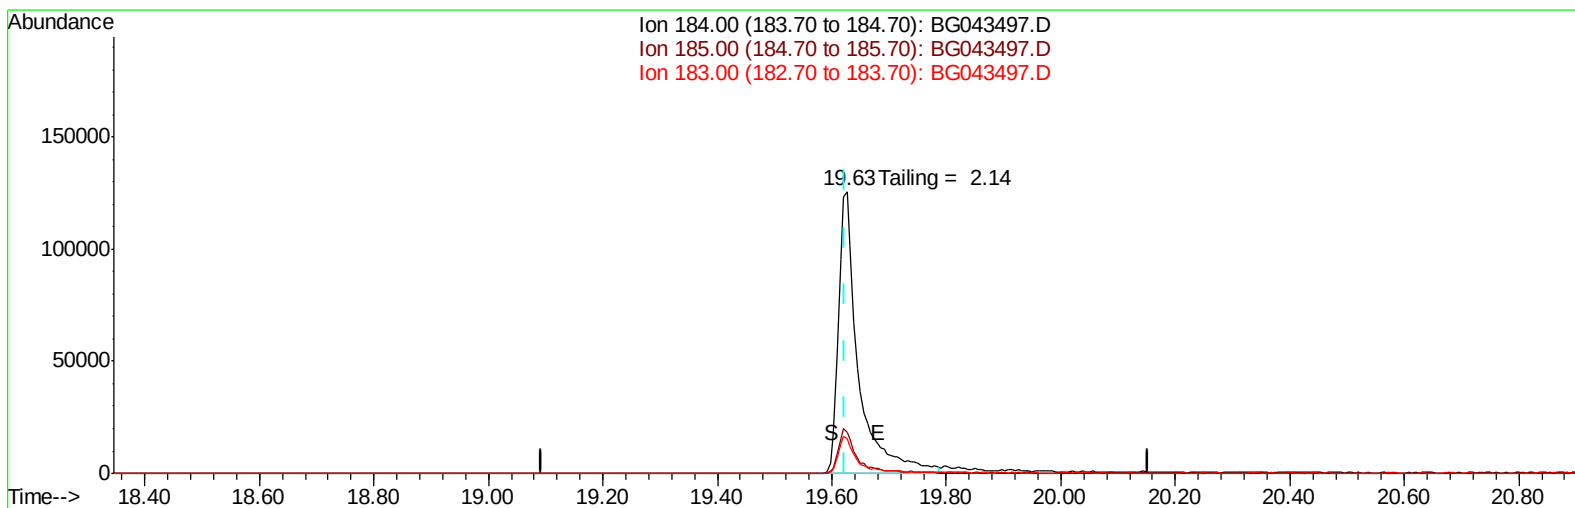

TIC: BG043497.D

(77) Benzidine

19.626min (+0.003) 278439.95ng

response 308203

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	14.69
183.00	12.50	12.39
0.00	0.00	0.00