
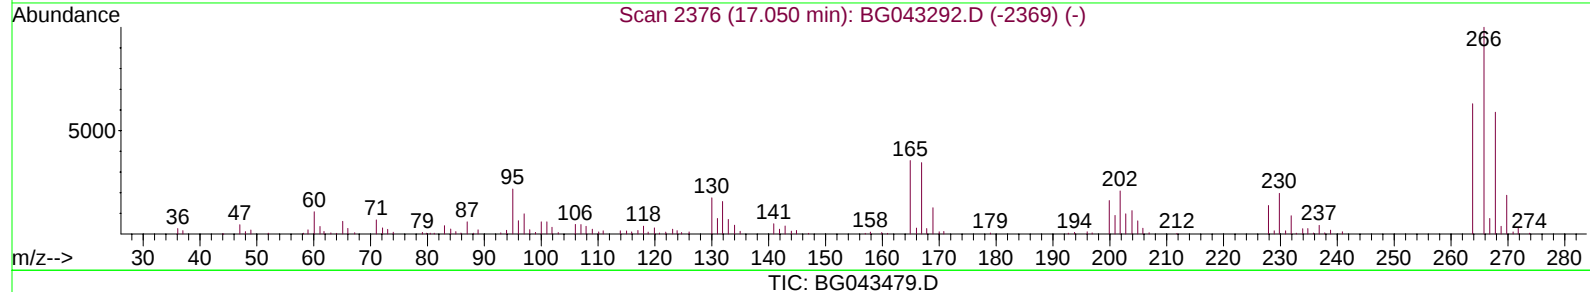
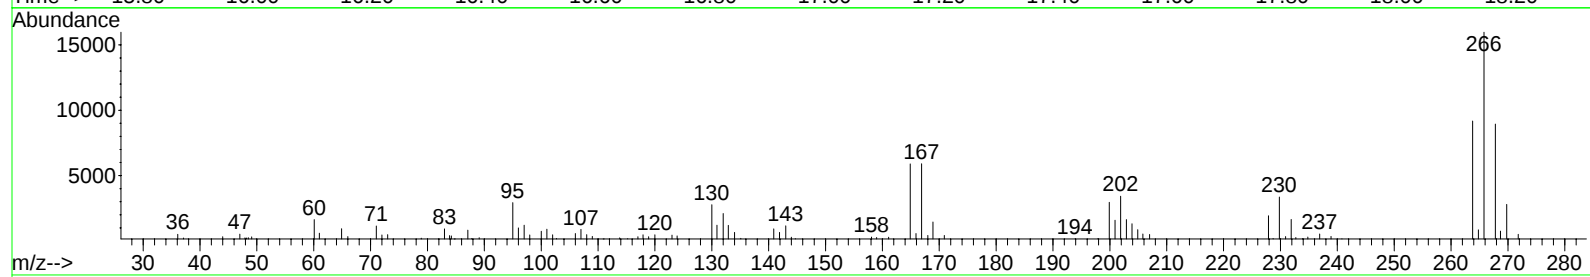


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110419\
Data File : BG043479.D
Acq On : 4 Nov 2019 13:19
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 16:35:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

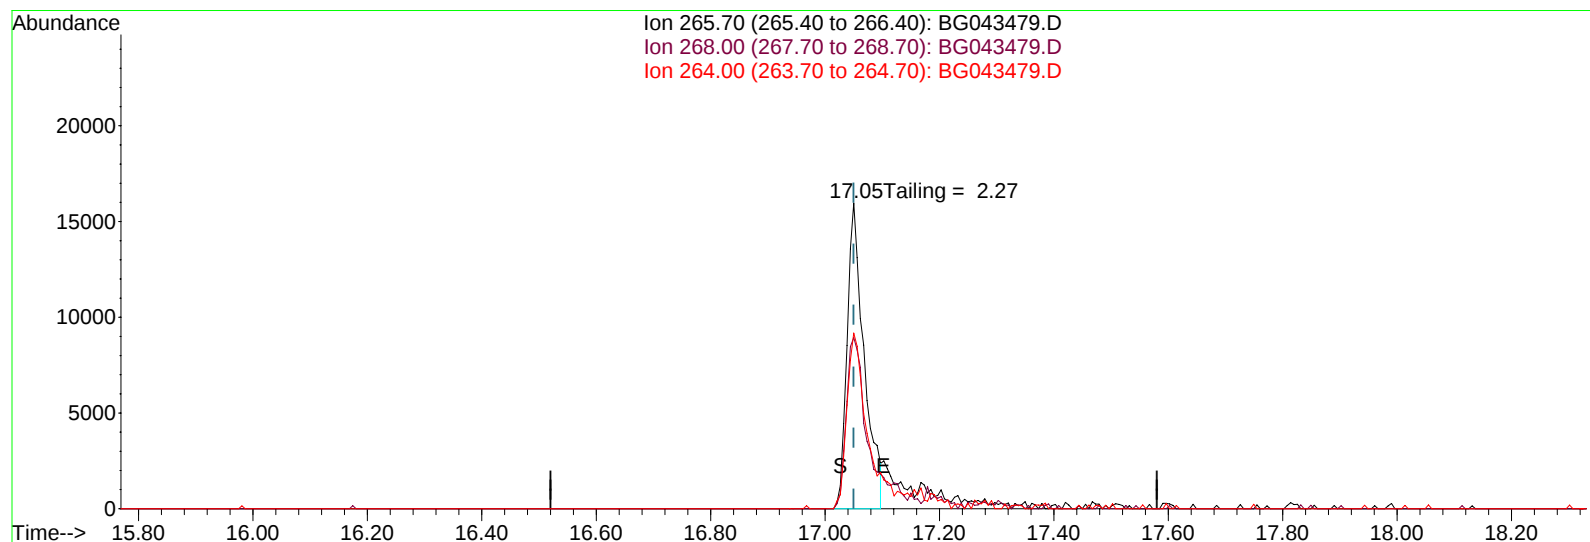

(70) Pentachlorophenol (C)




17.050min (+0.000) 17109.99ng

response 38299

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	60.66
264.00	61.10	57.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG110419\
Data File : BG043479.D
Acq On : 4 Nov 2019 13:19
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 16:35:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 15:22:15 2019
Response via : Initial Calibration

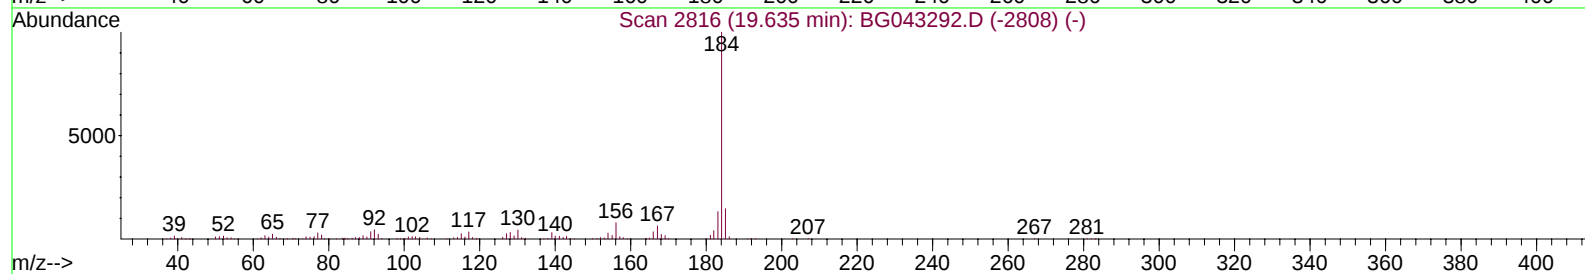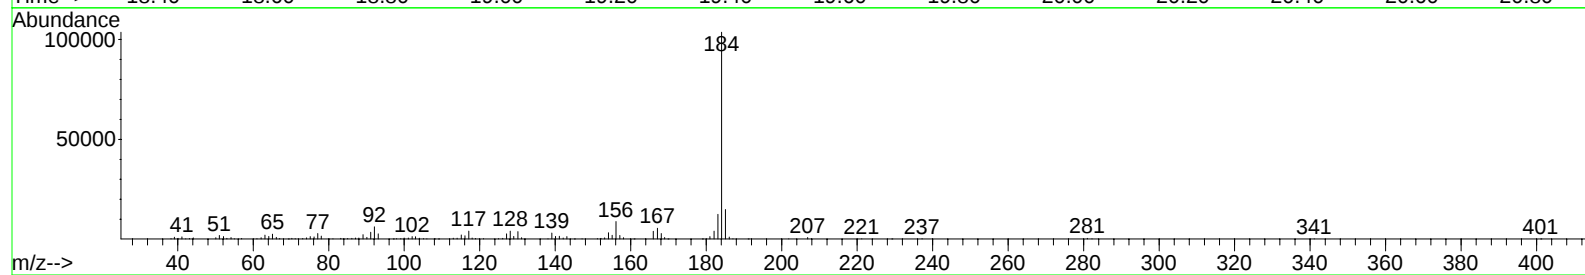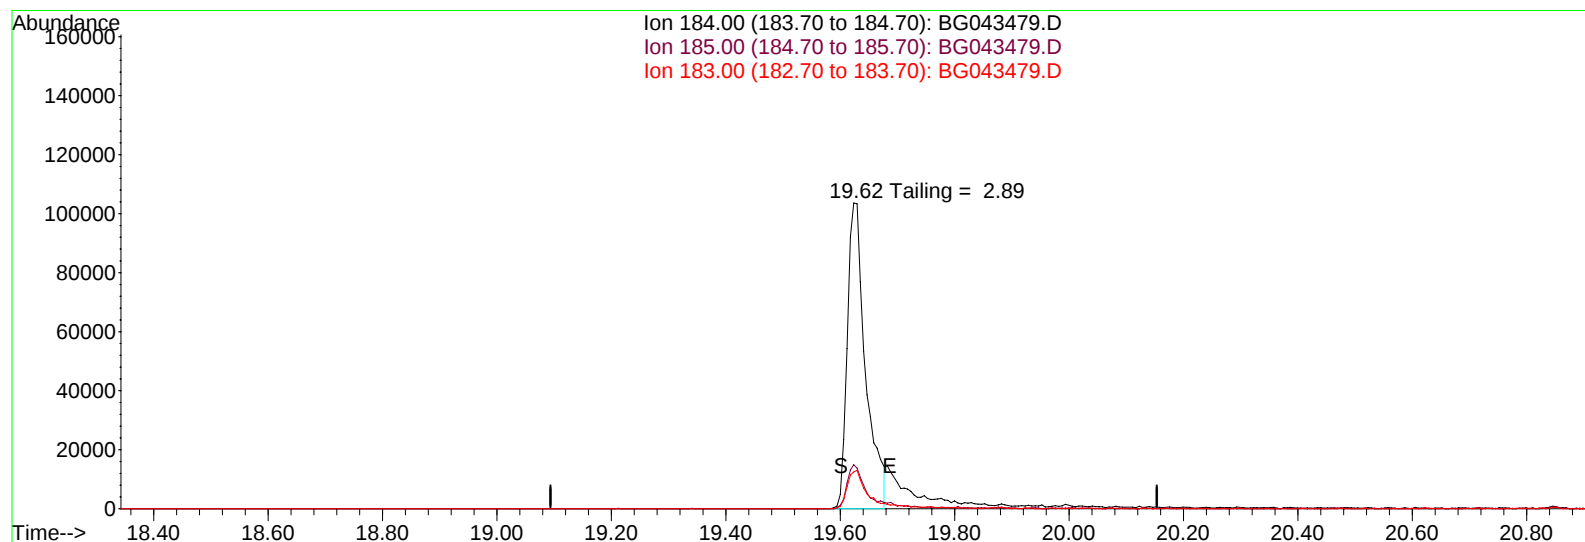

TIC: BG043479.D

(77) Benzidine

19.623min (-19.623) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	13.70	0.00#
183.00	12.50	0.00#
0.00	0.00	0.00