


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110419\
 Data File : BG043479.D
 Acq On : 4 Nov 2019 13:19
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 04 15:22:15 2019

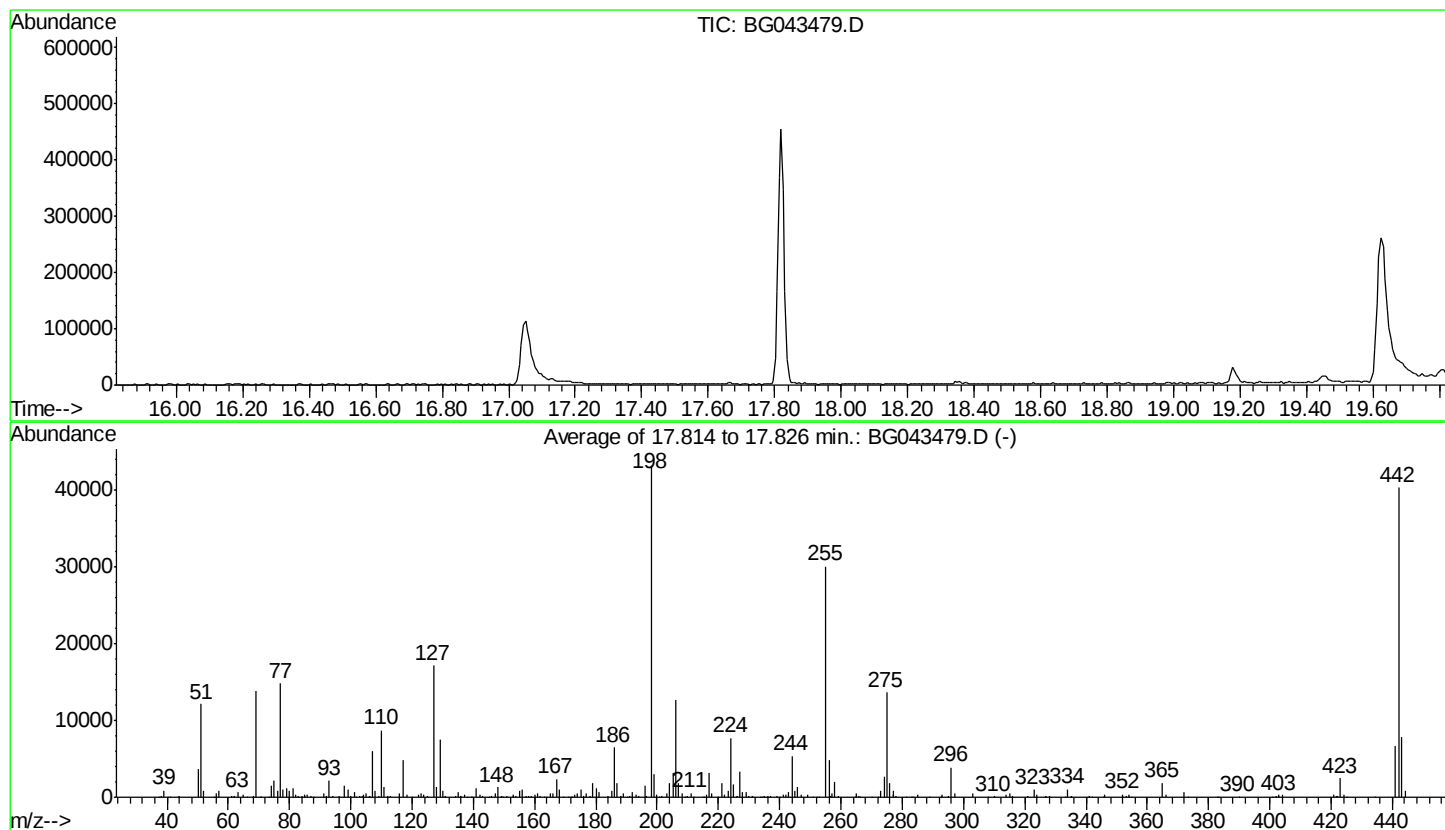

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	12182	PASS
68	69	0.00	2	1.0	133	PASS
69	198	0.00	100	32.0	13858	PASS
70	69	0.00	2	0.5	76	PASS
127	198	10	80	39.7	17170	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43242	PASS
199	198	5	9	7.1	3049	PASS
275	198	10	60	31.6	13669	PASS
365	198	1	100	4.3	1850	PASS
441	198	0.01	100	15.4	6646	PASS
442	198	50	100	93.3	40338	PASS
443	442	15	24	19.7	7935	PASS