


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110419\
 Data File : BG043497.D
 Acq On : 5 Nov 2019 2:11
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 04 15:22:15 2019

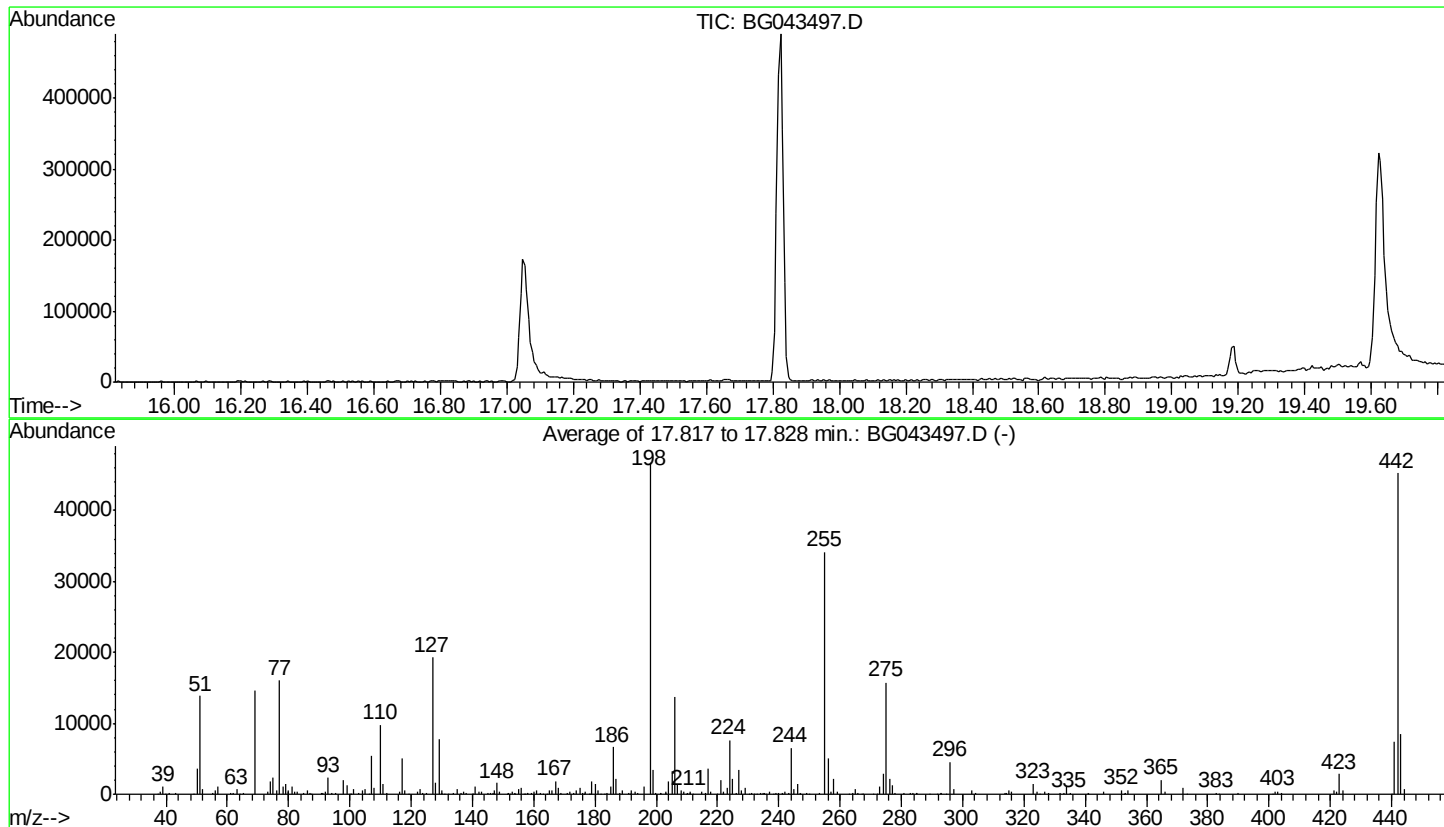

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	13875	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.1	14566	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.2	19261	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46770	PASS
199	198	5	9	7.4	3464	PASS
275	198	10	60	33.7	15759	PASS
365	198	1	100	4.4	2057	PASS
441	198	0.01	100	15.9	7440	PASS
442	198	50	100	96.8	45274	PASS
443	442	15	24	18.6	8404	PASS