
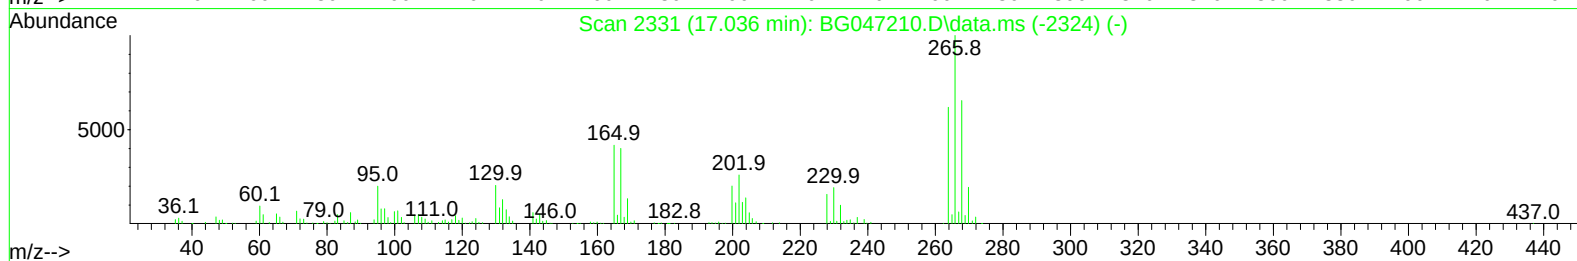
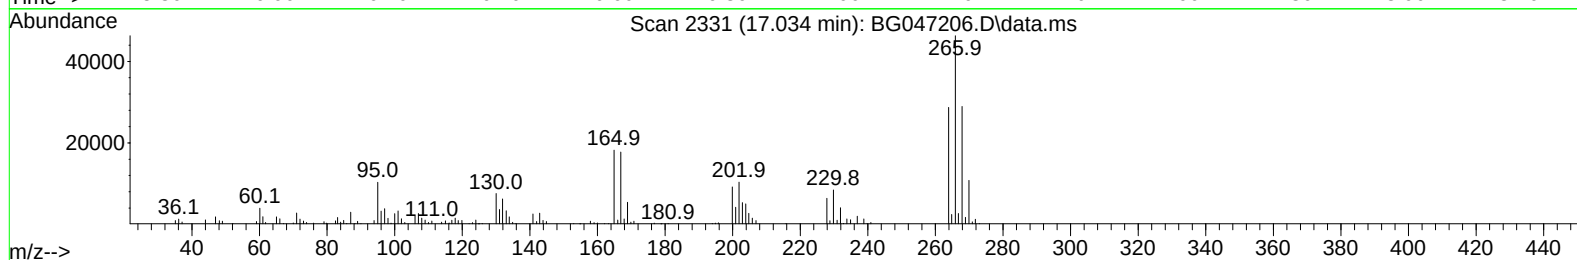


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110420\
Data File : BG047206.D
Acq On : 4 Nov 2020 10:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 02:14:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 04 16:19:40 2020
Response via : Initial Calibration

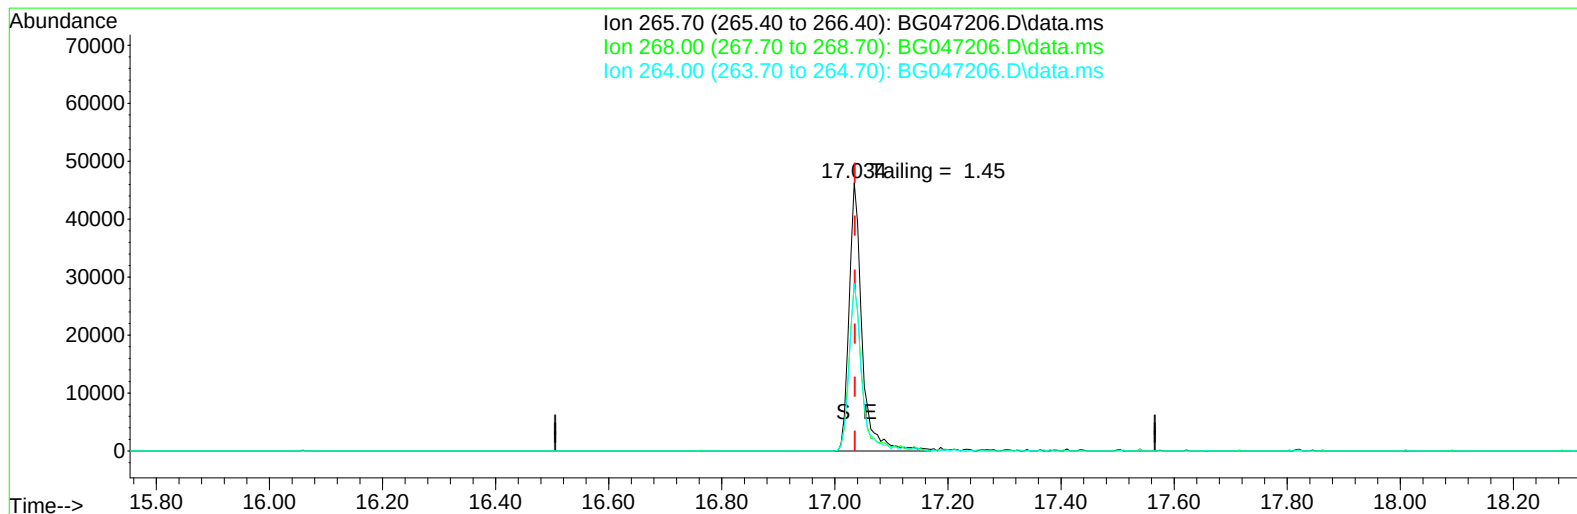

TIC: BG047206.D\data.ms

(70) Pentachlorophenol (C)




17.034min (-0.001) 31744.14 ng

response 74288

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.49
264.00	61.60	62.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110420\
Data File : BG047206.D
Acq On : 4 Nov 2020 10:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 02:14:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 04 16:19:40 2020
Response via : Initial Calibration

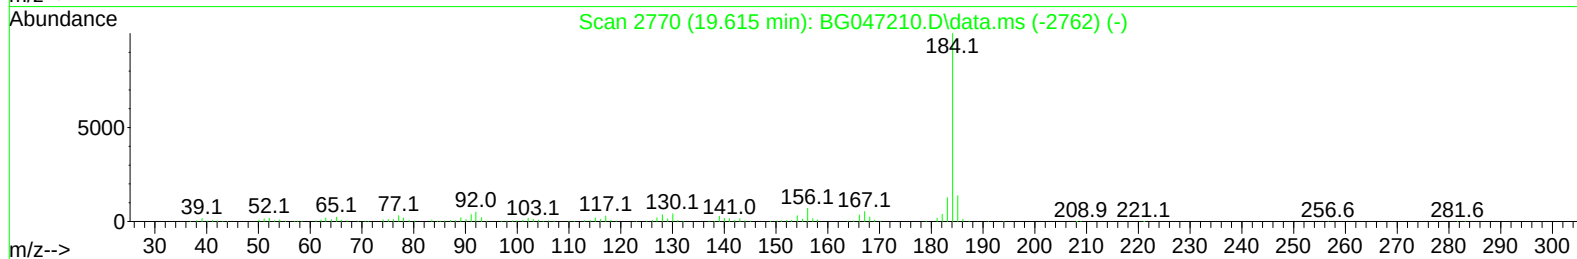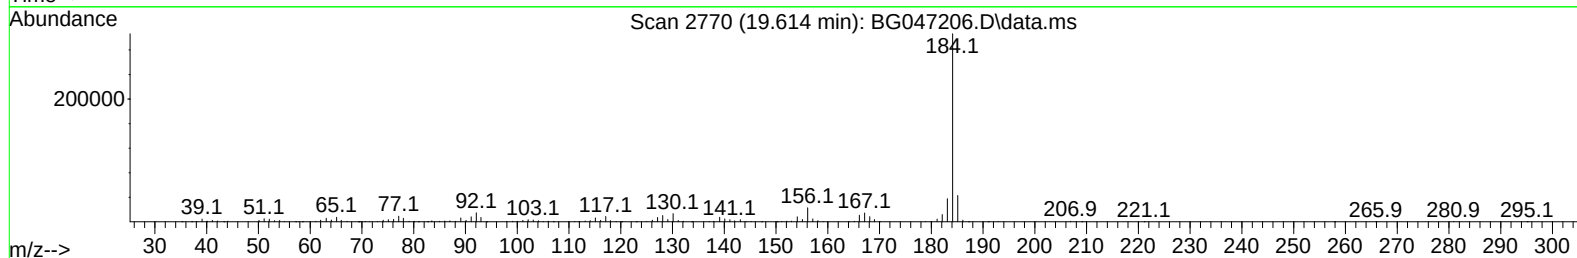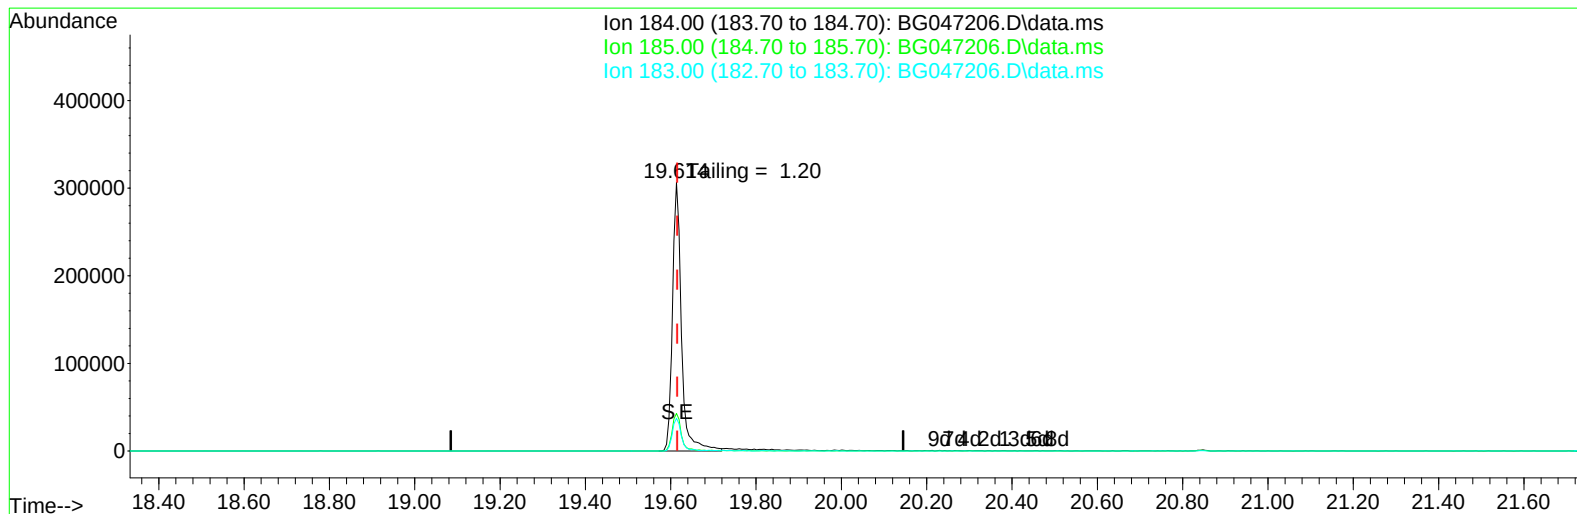

TIC: BG047206.D\data.ms

(77) Benzidine

19.614min (-0.001) 238261.91 ng m

response 487449

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	12.26
0.00	0.00	0.00