


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110420\
 Data File : BG047206.D
 Acq On : 4 Nov 2020 10:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 04 16:19:40 2020

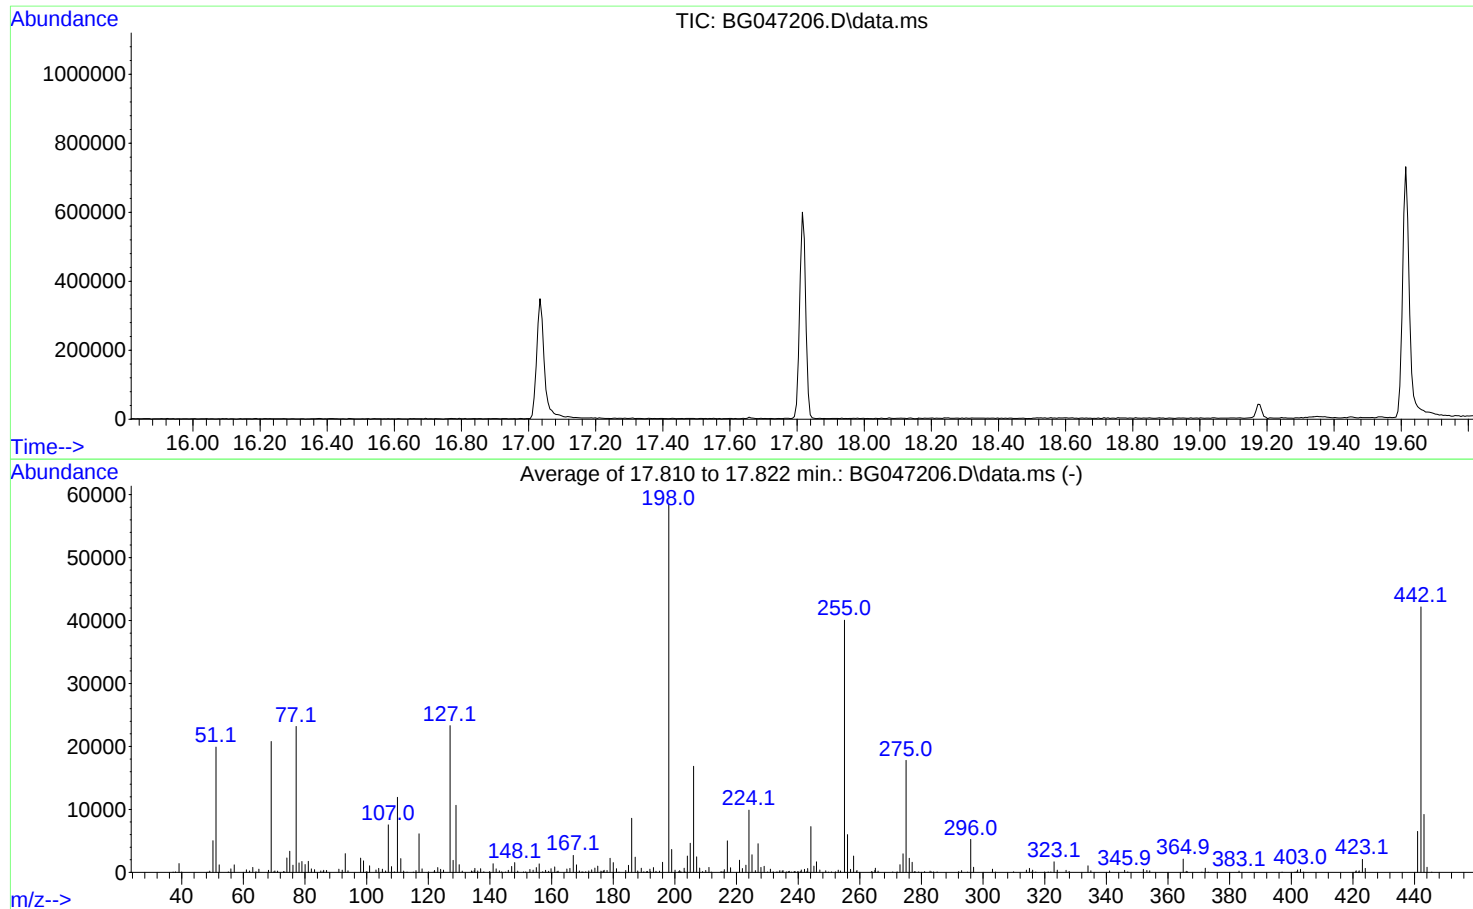

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	19891	PASS
68	69	0.00	2	1.6	336	PASS
69	198	0.00	100	35.6	20781	PASS
70	69	0.00	2	1.1	235	PASS
127	198	10	80	39.9	23309	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58432	PASS
199	198	5	9	6.2	3634	PASS
275	198	10	60	30.4	17780	PASS
365	198	1	100	3.6	2098	PASS
441	198	0.01	100	11.1	6497	PASS
442	198	50	100	72.2	42165	PASS
443	442	15	24	21.9	9214	PASS