
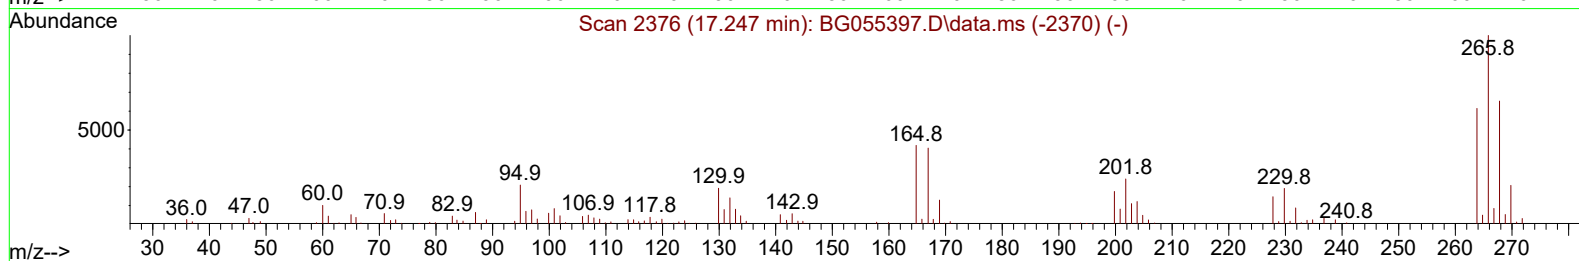
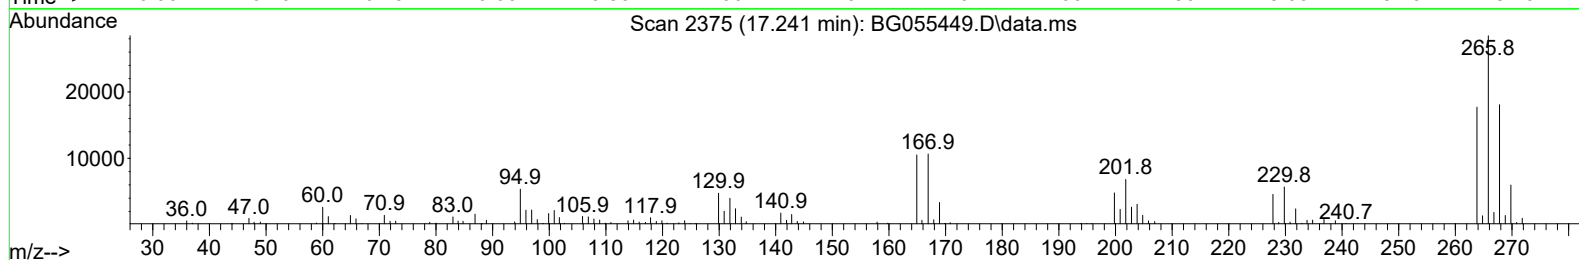


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110422\
Data File : BG055449.D
Acq On : 4 Nov 2022 11:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 05:26:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 05:28:43 2022
Response via : Initial Calibration

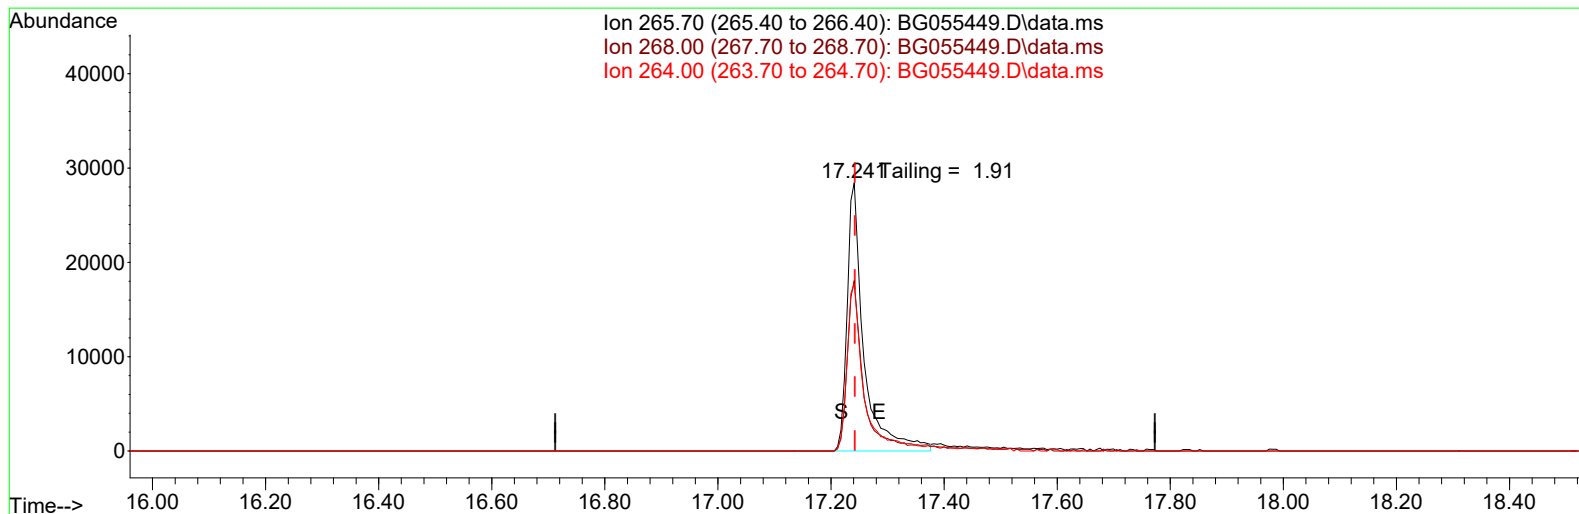

TIC: BG055449.D\data.ms

(70) Pentachlorophenol (C)




17.241min (-0.002) 33335.25 ng

response 58501

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.51
264.00	61.50	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110422\
Data File : BG055449.D
Acq On : 4 Nov 2022 11:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 05:26:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 05:28:43 2022
Response via : Initial Calibration

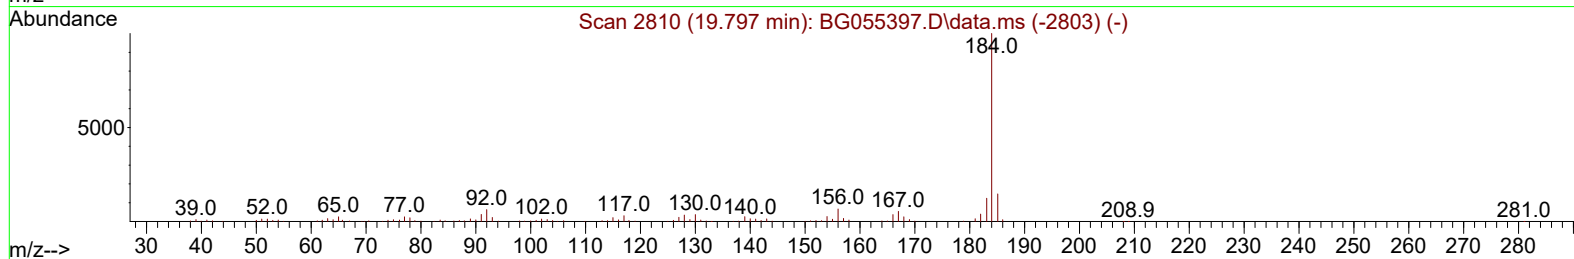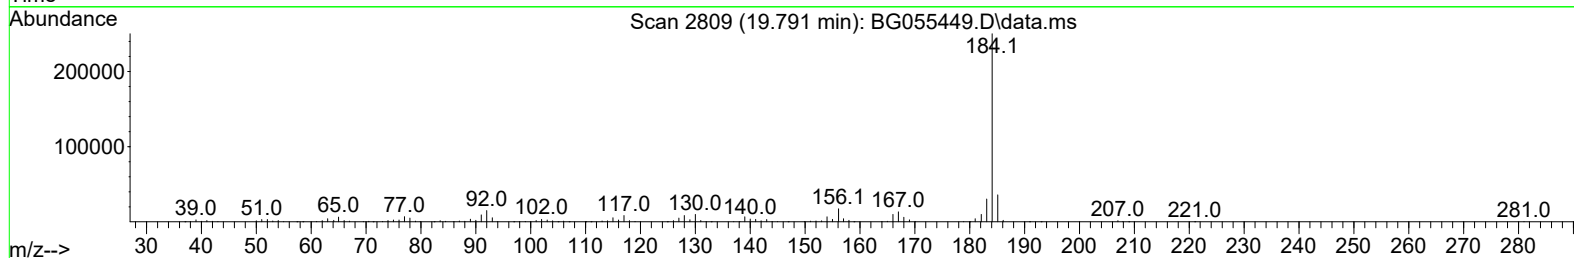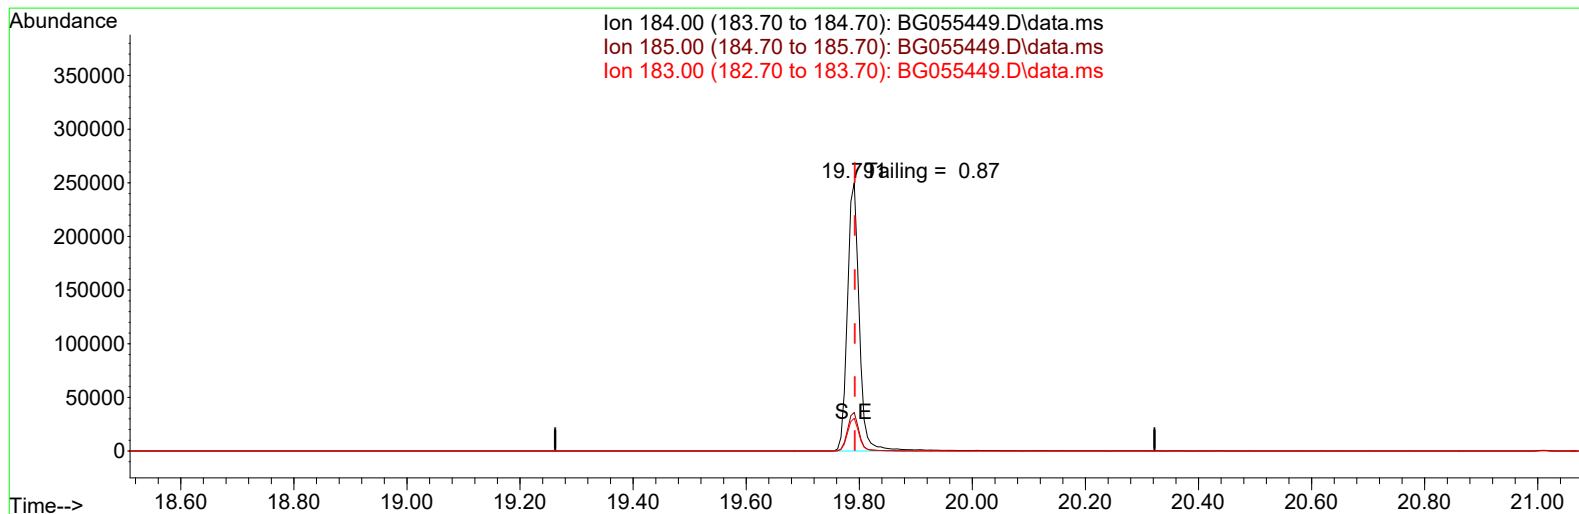

TIC: BG055449.D\data.ms

(77) Benzidine

19.791min (-0.002) 0.00 ng

response 363971

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.36
183.00	12.30	12.17
0.00	0.00	0.00