


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110422\
 Data File : BG055449.D
 Acq On : 4 Nov 2022 11:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 07 00:51:08 2022

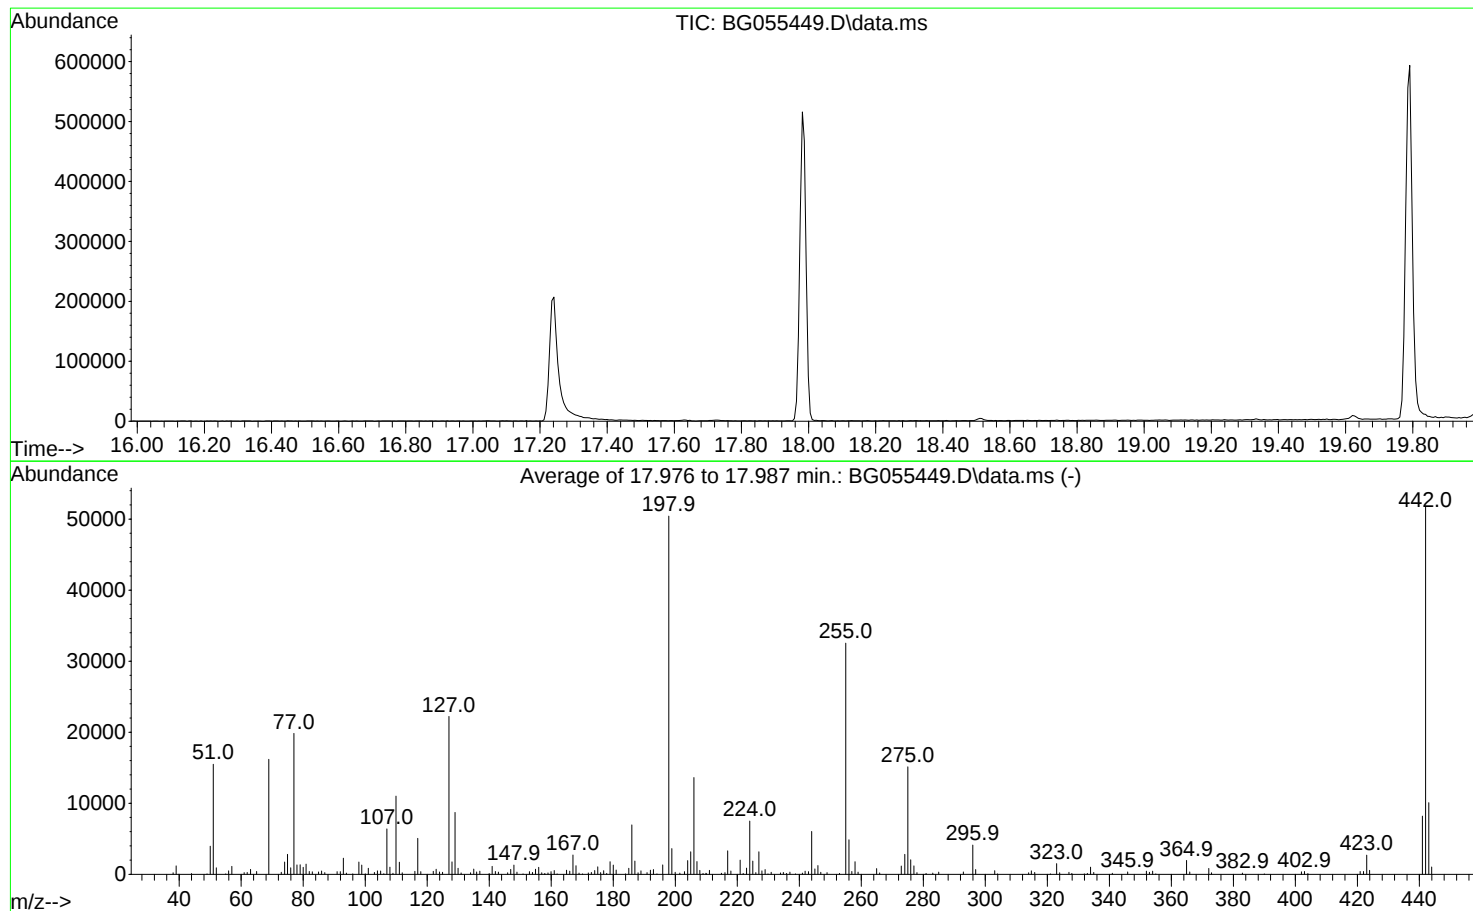




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	15488	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	16183	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.1	22216	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50411	PASS
199	198	5	9	7.2	3620	PASS
275	198	10	60	30.0	15117	PASS
365	198	1	100	3.9	1953	PASS
441	198	0.01	100	16.2	8183	PASS
442	442	50	100	100.0	51784	PASS
443	442	15	24	19.5	10078	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110422\
Data File : BG055449.D
Acq On : 4 Nov 2022 11:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 05 05:26:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 05:28:43 2022
Response via : Initial Calibration

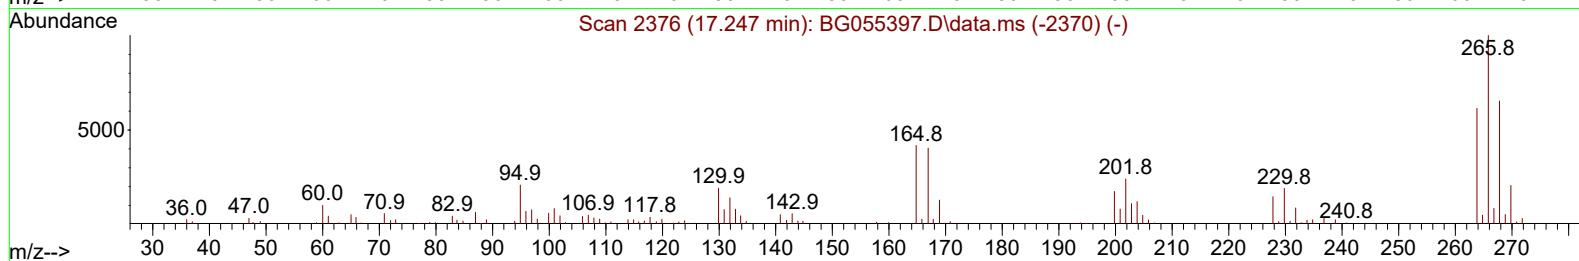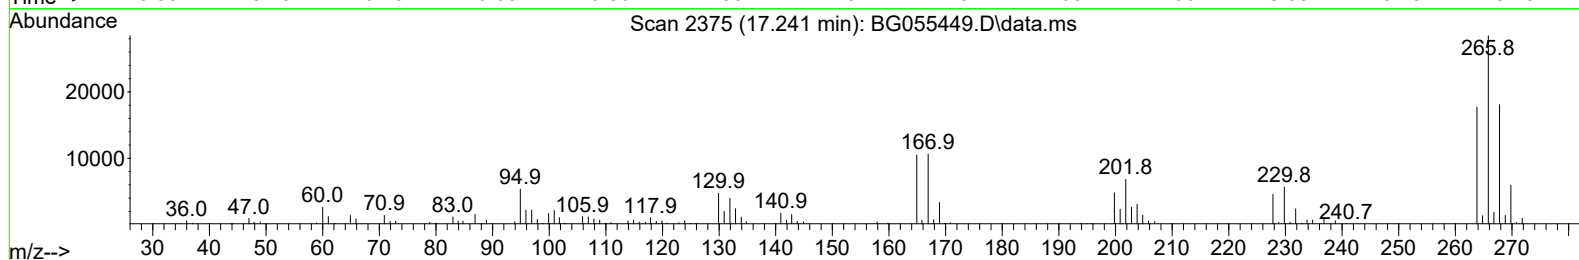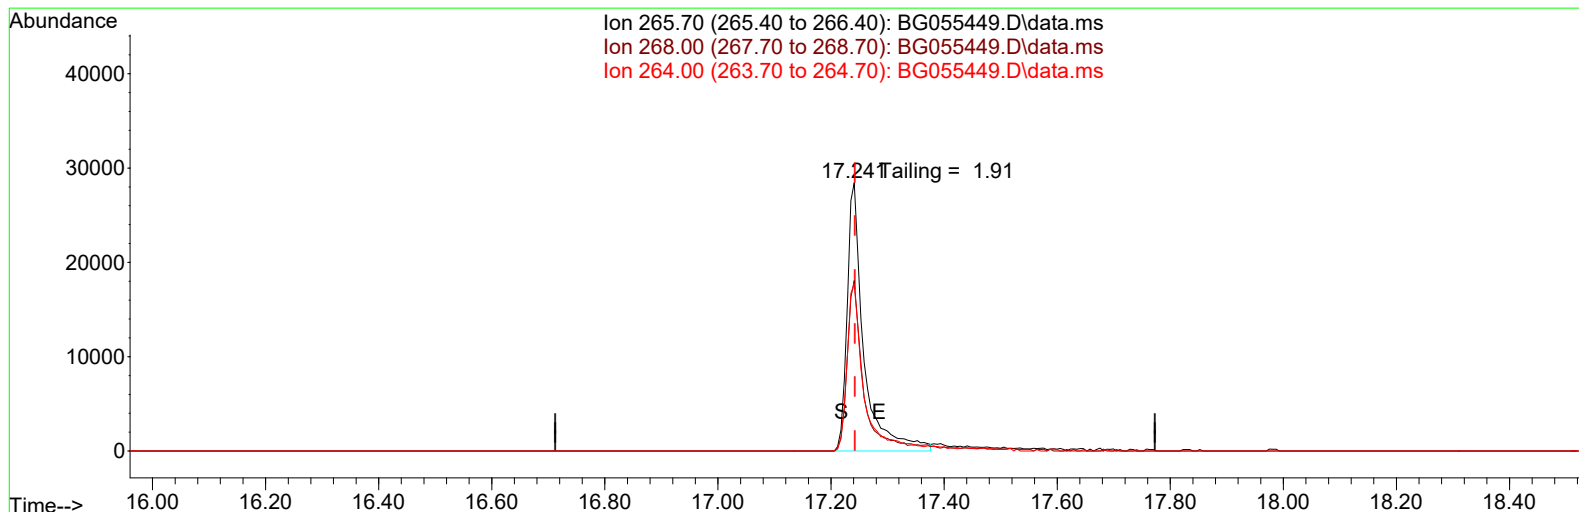

TIC: BG055449.D\data.ms

(70) Pentachlorophenol (C)

17.241min (-0.002) 33335.25 ng




response 58501

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.51
264.00	61.50	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110422\
Data File : BG055449.D
Acq On : 4 Nov 2022 11:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 05 05:26:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 05:28:43 2022
Response via : Initial Calibration

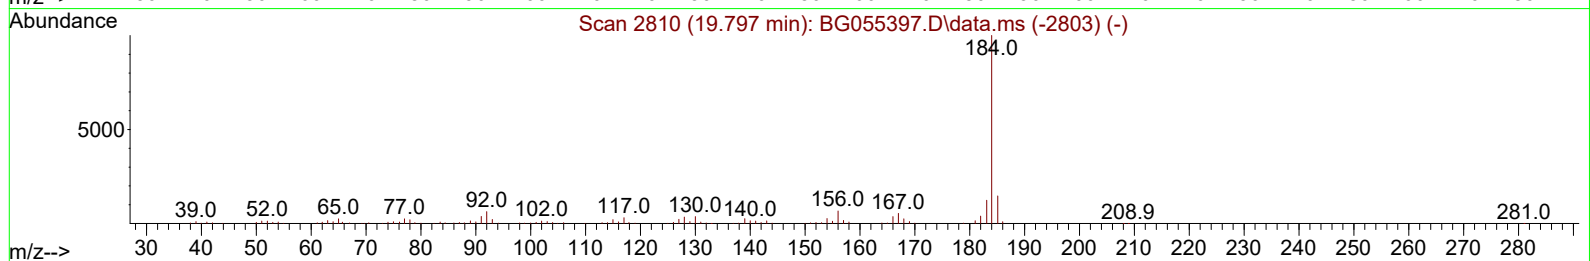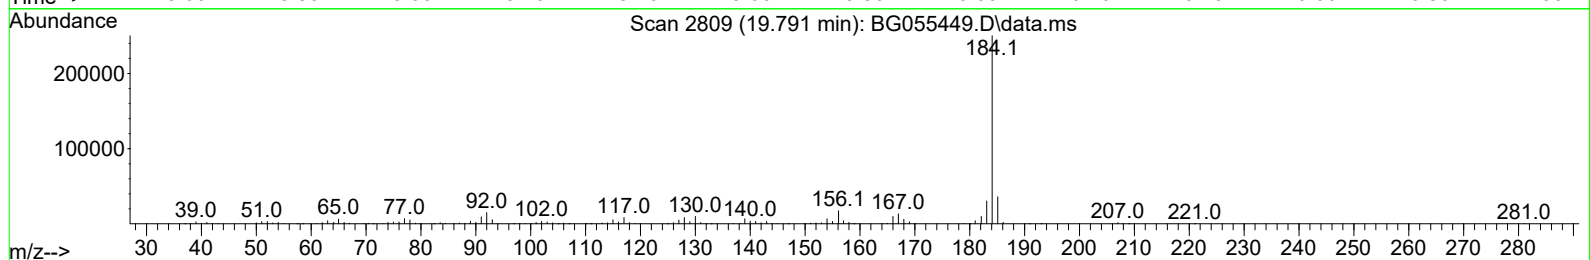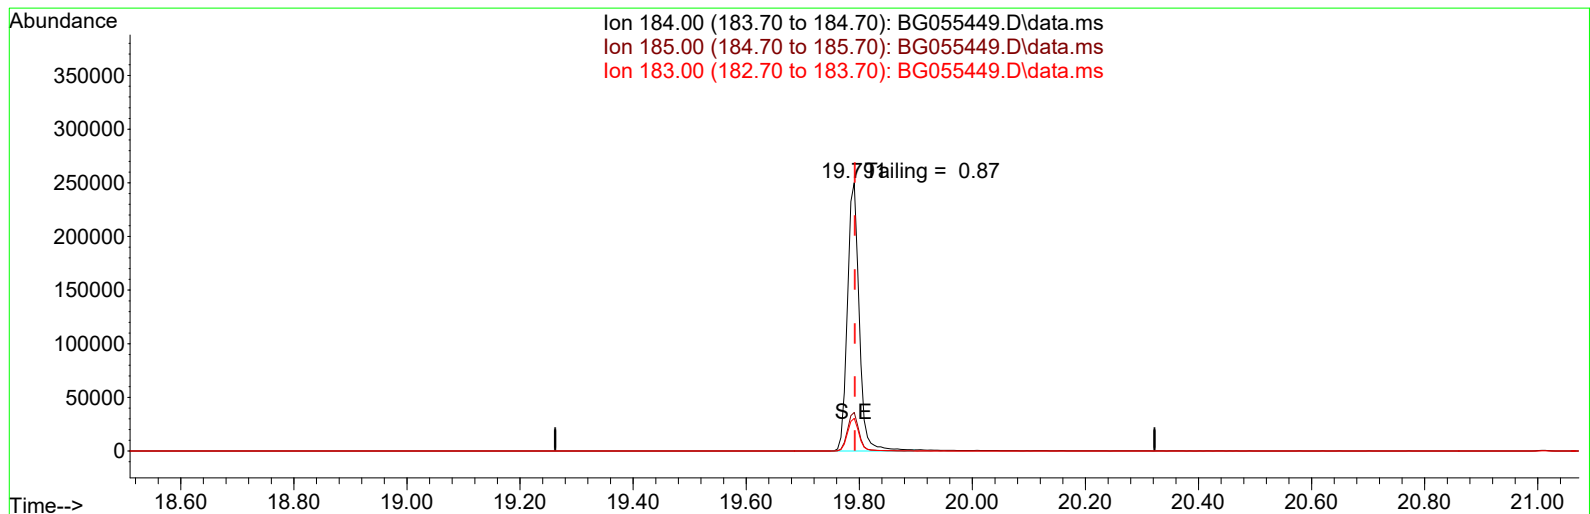

TIC: BG055449.D\data.ms

(77) Benzidine

19.791min (-0.002) 0.00 ng

response 363971

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.36
183.00	12.30	12.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2022	BNA_G	BG055449.D
Compound Name	Response	Retention Time
DDT	174015	21.013
DDD	3734	20.567
DDE	451	20.067
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4185	178200	2.35

Instrument :
BNA_G
ClientSampleId :
DFTPP