

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059615.D
 Acq On : 4 Nov 2023 9:53
 Operator : MA/JU
 Sample : PB156655BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.708	53	54	59	rBV2	5190	4447	0.27%	0.033%
2	4.078	113	117	123	rBV	111070	180944	11.02%	1.344%
3	4.307	155	156	161	rVB3	3591	3571	0.22%	0.027%
4	4.407	171	173	174	rBV	4651	4318	0.26%	0.032%
5	4.419	174	175	179	rVB2	10631	7461	0.45%	0.055%
6	4.483	184	186	191	rVB2	5346	7368	0.45%	0.055%
7	4.724	225	227	229	rBV	3888	3844	0.23%	0.029%
8	4.789	235	238	239	rBV	4779	4638	0.28%	0.034%
9	5.059	281	284	287	rBV	4206	4600	0.28%	0.034%
10	5.894	423	426	427	rBV	5420	4019	0.24%	0.030%
11	6.029	447	449	452	rBV	3711	4402	0.27%	0.033%
12	6.434	515	518	519	rBV	4785	4256	0.26%	0.032%
13	6.969	607	609	613	rBV	3695	5529	0.34%	0.041%
14	7.069	624	626	630	rVB	4026	4092	0.25%	0.030%
15	7.245	654	656	659	rBV	3287	3620	0.22%	0.027%
16	7.462	685	693	702	rVB2	194468	346563	21.11%	2.573%
17	7.633	719	722	723	rBV	7174	9010	0.55%	0.067%
18	7.668	723	728	736	rVB	126451	215553	13.13%	1.600%
19	7.868	755	762	769	rBV2	192529	338454	20.62%	2.513%
20	8.350	839	844	852	rVB2	138478	247337	15.07%	1.836%
21	8.526	872	874	876	rBV	3701	3796	0.23%	0.028%
22	8.773	914	916	918	rBV	4409	3773	0.23%	0.028%
23	8.925	940	942	945	rVB	4641	4510	0.27%	0.033%
24	9.031	954	960	968	rBV	265476	475326	28.96%	3.529%
25	9.501	1036	1040	1041	rBV	6161	7319	0.45%	0.054%
26	9.548	1041	1048	1055	rVV2	183740	329077	20.05%	2.443%
27	9.836	1095	1097	1101	rBV2	5047	6886	0.42%	0.051%
28	9.942	1114	1115	1117	rVB2	5532	3606	0.22%	0.027%
29	9.983	1120	1122	1125	rBV2	3823	4031	0.25%	0.030%
30	10.230	1162	1164	1165	rBV2	5201	4075	0.25%	0.030%
31	10.271	1165	1171	1178	rVB	145834	270927	16.51%	2.012%
32	10.553	1217	1219	1221	rBV	3920	3648	0.22%	0.027%
33	10.641	1233	1234	1237	rBV	4514	3955	0.24%	0.029%
34	10.794	1254	1260	1270	rVB	253945	452939	27.59%	3.363%
35	10.970	1287	1290	1291	rVB	4704	3960	0.24%	0.029%
36	11.082	1307	1309	1312	rBV	4371	4534	0.28%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059615.D
 Acq On : 4 Nov 2023 9:53
 Operator : MA/JU
 Sample : PB156655BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

37	11.117	1312	1315	1316	rBV	6067	5009	0.31%	0.037%
38	11.199	1322	1329	1336	rVB	211787	375577	22.88%	2.789%
39	11.340	1343	1353	1363	rBV2	266861	511188	31.14%	3.796%
40	11.558	1387	1390	1393	rBV2	3476	4977	0.30%	0.037%
41	11.699	1412	1414	1415	rBV2	4588	3530	0.22%	0.026%
42	12.063	1472	1476	1480	rBV2	5444	7320	0.45%	0.054%
43	12.568	1559	1562	1564	rBV	3421	3562	0.22%	0.026%
44	12.750	1591	1593	1595	rBV	5422	4972	0.30%	0.037%
45	13.731	1758	1760	1762	rVB	7003	4752	0.29%	0.035%
46	13.808	1771	1773	1774	rBV	10517	7225	0.44%	0.054%
47	13.855	1779	1781	1783	rBV	4258	3676	0.22%	0.027%
48	13.914	1789	1791	1794	rVB	6353	5979	0.36%	0.044%
49	14.243	1843	1847	1850	rBV	4771	4723	0.29%	0.035%
50	14.372	1864	1869	1875	rVB	552675	798281	48.63%	5.927%
51	14.466	1882	1885	1887	rVB	4706	5205	0.32%	0.039%
52	14.683	1916	1922	1929	rVB2	583864	921920	56.16%	6.845%
53	14.871	1953	1954	1957	rBV2	4975	5595	0.34%	0.042%
54	14.983	1966	1973	1981	rVB	337330	517354	31.52%	3.841%
55	15.153	1995	2002	2008	rBV2	239966	393410	23.97%	2.921%
56	15.271	2020	2022	2023	rBV2	4616	3597	0.22%	0.027%
57	15.418	2045	2047	2050	rBV2	3913	3964	0.24%	0.029%
58	15.500	2059	2061	2064	rBV2	3516	3578	0.22%	0.027%
59	15.565	2071	2072	2077	rBV2	5599	5224	0.32%	0.039%
60	15.835	2116	2118	2121	rVB2	5448	5816	0.35%	0.043%
61	15.876	2121	2125	2127	rBV2	4587	4966	0.30%	0.037%
62	15.970	2134	2141	2149	rBV	726273	1077485	65.64%	8.000%
63	16.070	2152	2158	2164	rBV2	189088	288978	17.60%	2.146%
64	16.140	2167	2170	2172	rBV	5086	5199	0.32%	0.039%
65	16.370	2207	2209	2212	rBV	4052	6255	0.38%	0.046%
66	16.581	2243	2245	2248	rBV	3419	3710	0.23%	0.028%
67	16.945	2305	2307	2309	rVB	6641	3512	0.21%	0.026%
68	17.098	2331	2333	2336	rBV	5695	5631	0.34%	0.042%
69	17.139	2338	2340	2342	rBV	4749	3655	0.22%	0.027%
70	17.462	2394	2395	2398	rVB2	4293	3565	0.22%	0.026%
71	17.627	2417	2423	2424	rBV	6416	9969	0.61%	0.074%
72	17.733	2435	2441	2449	rVB	419391	635595	38.72%	4.719%
73	17.833	2451	2458	2464	rVB	800961	1188740	72.42%	8.826%
74	18.026	2487	2491	2492	rBV2	4713	4804	0.29%	0.036%
75	18.632	2593	2594	2598	rBV2	3553	4571	0.28%	0.034%
76	19.184	2687	2688	2690	rVB	6490	4026	0.25%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059615.D
Acq On : 4 Nov 2023 9:53
Operator : MA/JU
Sample : PB156655BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK655

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Title : SVOA CALIBRATION

77	19.666	2767	2770	2774	rBV4	16241	22338	1.36%	0.166%
78	20.065	2836	2838	2839	rBV2	9252	6506	0.40%	0.048%
79	20.100	2839	2844	2850	rVB	910251	1310932	79.86%	9.734%
80	22.063	3173	3178	3185	rVB2	357635	643163	39.18%	4.776%
81	25.418	3740	3749	3762	rVB3	558660	1641482	100.00%	12.188%




Sum of corrected areas: 13467904

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059615.D
Acq On : 4 Nov 2023 9:53
Operator : MA/JU
Sample : PB156655BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK655

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

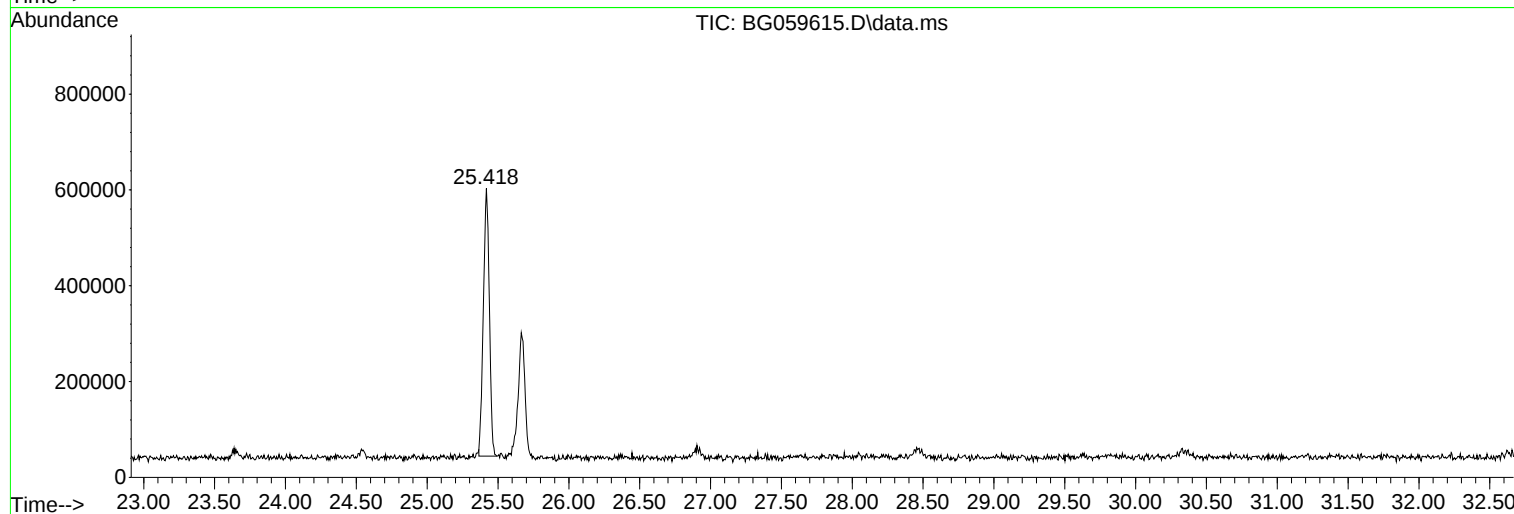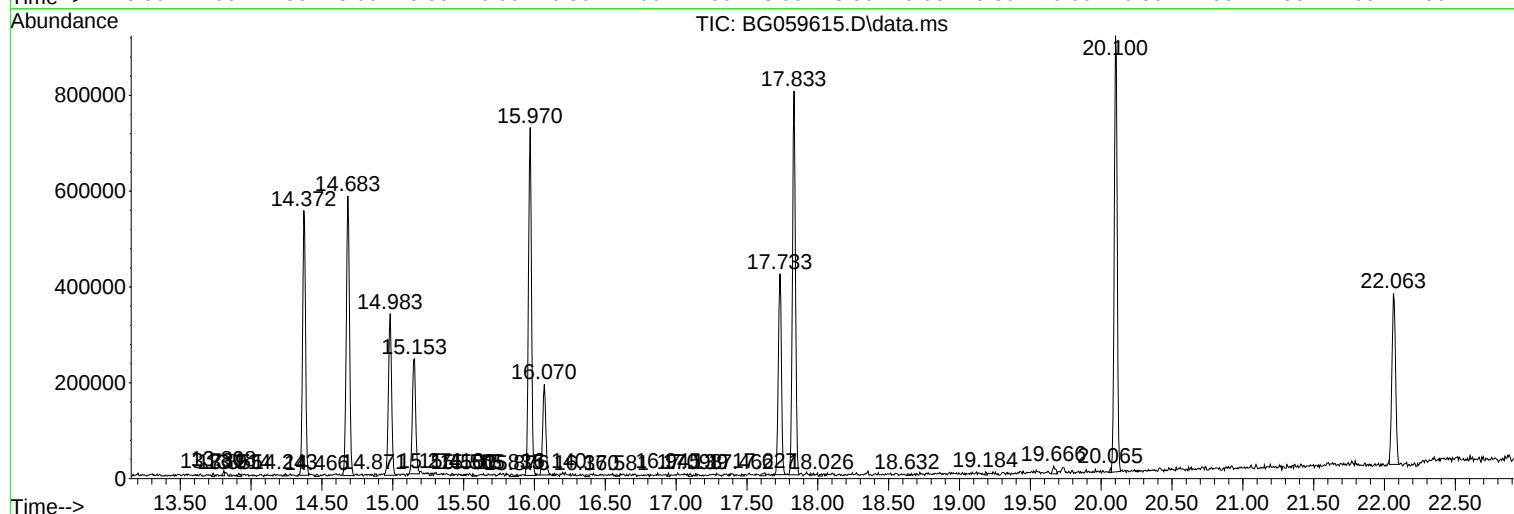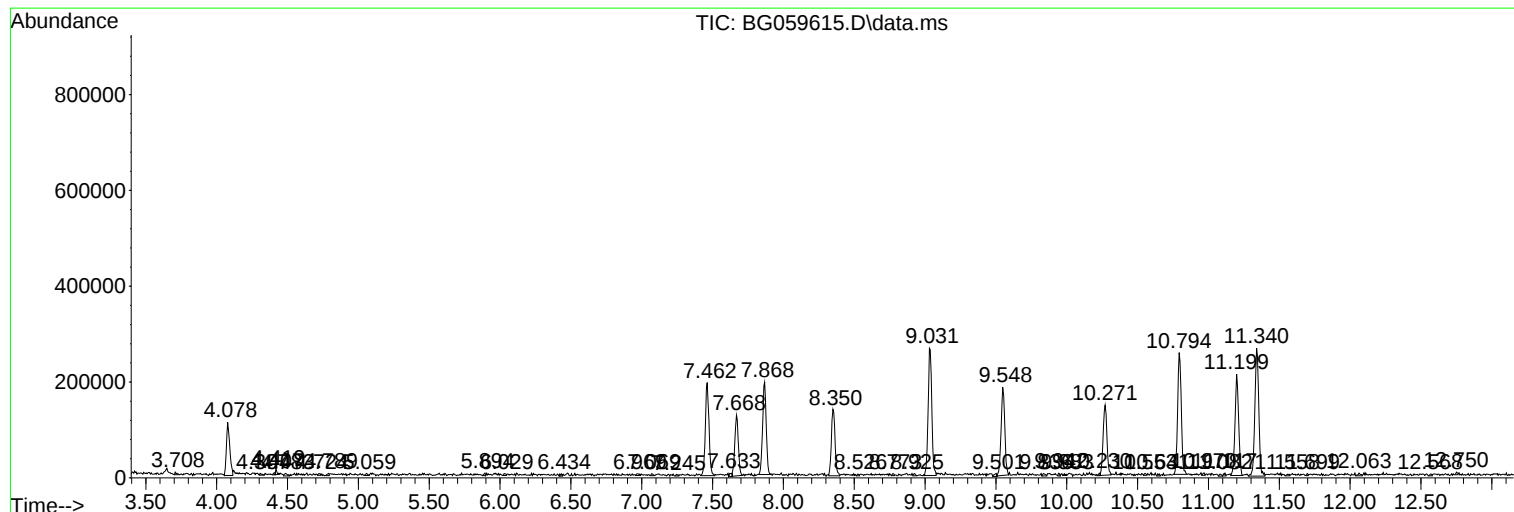

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059615.D
Acq On : 4 Nov 2023 9:53
Operator : MA/JU
Sample : PB156655BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK655

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059615.D
Acq On : 4 Nov 2023 9:53
Operator : MA/JU
Sample : PB156655BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK655

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc