

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059628.D
 Acq On : 4 Nov 2023 19:21
 Operator : MA/JU
 Sample : PB156655BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.725	55	57	60	rVB2	9442	6671	0.49%	0.063%
2	4.078	113	117	125	rVB	102894	158938	11.77%	1.510%
3	4.213	138	140	143	rBV3	3793	3869	0.29%	0.037%
4	4.424	174	176	178	rBV	4336	4218	0.31%	0.040%
5	4.753	229	232	236	rBV	4430	7220	0.53%	0.069%
6	4.853	248	249	252	rBV	4706	4754	0.35%	0.045%
7	5.370	335	337	341	rBV	3703	3966	0.29%	0.038%
8	5.405	341	343	345	rVB	6620	5828	0.43%	0.055%
9	5.435	345	348	349	rBV	4249	4684	0.35%	0.044%
10	5.746	398	401	402	rVB	4171	3966	0.29%	0.038%
11	5.770	402	405	408	rBV2	7010	7960	0.59%	0.076%
12	5.975	438	440	444	rBV2	4536	5837	0.43%	0.055%
13	6.081	454	458	459	rBV	4368	4073	0.30%	0.039%
14	6.504	529	530	533	rBV	4211	3826	0.28%	0.036%
15	6.798	578	580	582	rBV	6984	5034	0.37%	0.048%
16	6.898	594	597	600	rBV	5898	7879	0.58%	0.075%
17	6.939	602	604	608	rVB	5377	4915	0.36%	0.047%
18	6.986	608	612	613	rBV	4627	4555	0.34%	0.043%
19	7.109	631	633	636	rBV	3221	3738	0.28%	0.036%
20	7.462	686	693	699	rBV2	145112	251009	18.58%	2.385%
21	7.503	699	700	704	rVV	4323	4278	0.32%	0.041%
22	7.668	722	728	734	rBV	88540	151534	11.22%	1.440%
23	7.744	737	741	744	rBV	4029	6995	0.52%	0.066%
24	7.861	755	761	768	rBV	136990	237919	17.61%	2.260%
25	8.008	784	786	789	rBV	4233	4080	0.30%	0.039%
26	8.173	812	814	816	rBV	3476	3972	0.29%	0.038%
27	8.355	839	845	851	rVB	136220	226785	16.79%	2.155%
28	8.408	851	854	856	rVB	4698	5665	0.42%	0.054%
29	8.590	882	885	887	rBV	3230	3848	0.28%	0.037%
30	8.872	932	933	937	rBV	4031	4386	0.32%	0.042%
31	8.907	937	939	945	rBV	4135	5798	0.43%	0.055%
32	9.031	953	960	967	rBV	191129	333796	24.71%	3.171%
33	9.272	999	1001	1004	rBV	3722	4747	0.35%	0.045%
34	9.377	1017	1019	1023	rBV	3637	5640	0.42%	0.054%
35	9.430	1026	1028	1031	rBV	3749	4011	0.30%	0.038%
36	9.507	1038	1041	1042	rBV	4500	5101	0.38%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059628.D
 Acq On : 4 Nov 2023 19:21
 Operator : MA/JU
 Sample : PB156655BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

37	9.548	1042	1048	1057	rVB2	142000	249260	18.45%	2.368%
38	9.671	1066	1069	1070	rVB2	6540	5024	0.37%	0.048%
39	9.753	1081	1083	1085	rVB2	4444	3708	0.27%	0.035%
40	9.818	1093	1094	1096	rBV2	6394	3904	0.29%	0.037%
41	9.988	1121	1123	1125	rVB2	4896	4107	0.30%	0.039%
42	10.018	1125	1128	1130	rBV	3840	3995	0.30%	0.038%
43	10.182	1153	1156	1158	rBV	4687	4467	0.33%	0.042%
44	10.270	1164	1171	1177	rBV3	124324	223540	16.55%	2.124%
45	10.576	1222	1223	1226	rVB3	6684	3980	0.29%	0.038%
46	10.617	1226	1230	1233	rBV	3517	5509	0.41%	0.052%
47	10.646	1233	1235	1238	rVB	3902	4525	0.34%	0.043%
48	10.793	1253	1260	1267	rBV3	195263	353653	26.18%	3.360%
49	10.970	1288	1290	1292	rBV3	4086	4162	0.31%	0.040%
50	11.140	1314	1319	1322	rBV3	3301	6984	0.52%	0.066%
51	11.199	1322	1329	1337	rVV2	200764	368702	27.30%	3.503%
52	11.340	1346	1353	1362	rVB2	211490	388491	28.76%	3.691%
53	11.633	1402	1403	1407	rBV	3872	4015	0.30%	0.038%
54	11.686	1410	1412	1414	rBV	4308	4479	0.33%	0.043%
55	11.939	1452	1455	1458	rBV	4844	6552	0.49%	0.062%
56	12.239	1504	1506	1508	rVB	5077	3911	0.29%	0.037%
57	12.303	1514	1517	1518	rBV	4185	3799	0.28%	0.036%
58	12.497	1545	1550	1551	rVB	5025	6035	0.45%	0.057%
59	12.691	1580	1583	1588	rVB	2996	3961	0.29%	0.038%
60	12.756	1592	1594	1598	rVB3	8089	8054	0.60%	0.077%
61	12.903	1613	1619	1620	rBV2	5873	6067	0.45%	0.058%
62	12.944	1624	1626	1628	rBV2	4107	3772	0.28%	0.036%
63	13.026	1638	1640	1643	rBV	3446	4186	0.31%	0.040%
64	13.567	1730	1732	1734	rBV	6127	5518	0.41%	0.052%
65	13.948	1794	1797	1798	rBV	3781	3983	0.29%	0.038%
66	14.125	1825	1827	1828	rBV	3994	3771	0.28%	0.036%
67	14.371	1863	1869	1876	rVB	461091	642305	47.55%	6.102%
68	14.548	1897	1899	1902	rBV	3718	4543	0.34%	0.043%
69	14.683	1916	1922	1930	rVB2	436629	705466	52.23%	6.702%
70	14.983	1967	1973	1980	rVB2	320650	519437	38.46%	4.935%
71	15.147	1995	2001	2009	rBV2	198933	333597	24.70%	3.169%
72	15.341	2032	2034	2037	rVB2	5099	4223	0.31%	0.040%
73	15.453	2051	2053	2055	rBV2	5001	4520	0.33%	0.043%
74	15.570	2072	2073	2075	rBV2	4303	3868	0.29%	0.037%
75	15.970	2134	2141	2149	rVB	558700	872279	64.58%	8.287%
76	16.069	2152	2158	2164	rVB2	151218	233284	17.27%	2.216%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059628.D
Acq On : 4 Nov 2023 19:21
Operator : MA/JU
Sample : PB156655BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs : 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Title : SVOA CALIBRATION

77	16.804	2281	2283	2285	rBV	4358	4611	0.34%	0.044%
78	17.732	2433	2441	2447	rBV	483364	708770	52.47%	6.734%
79	17.832	2451	2458	2464	rBV2	651542	986805	73.06%	9.375%
80	17.932	2473	2475	2478	rBV2	6514	7495	0.55%	0.071%
81	18.455	2562	2564	2568	rBV2	5170	7434	0.55%	0.071%
82	19.154	2680	2683	2684	rBV	5406	4713	0.35%	0.045%
83	20.100	2839	2844	2850	rBV	942356	1350719	100.00%	12.832%
84	22.062	3173	3178	3186	rVB2	508931	918297	67.99%	8.724%




Sum of corrected areas: 10525975

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059628.D
Acq On : 4 Nov 2023 19:21
Operator : MA/JU
Sample : PB156655BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK655

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

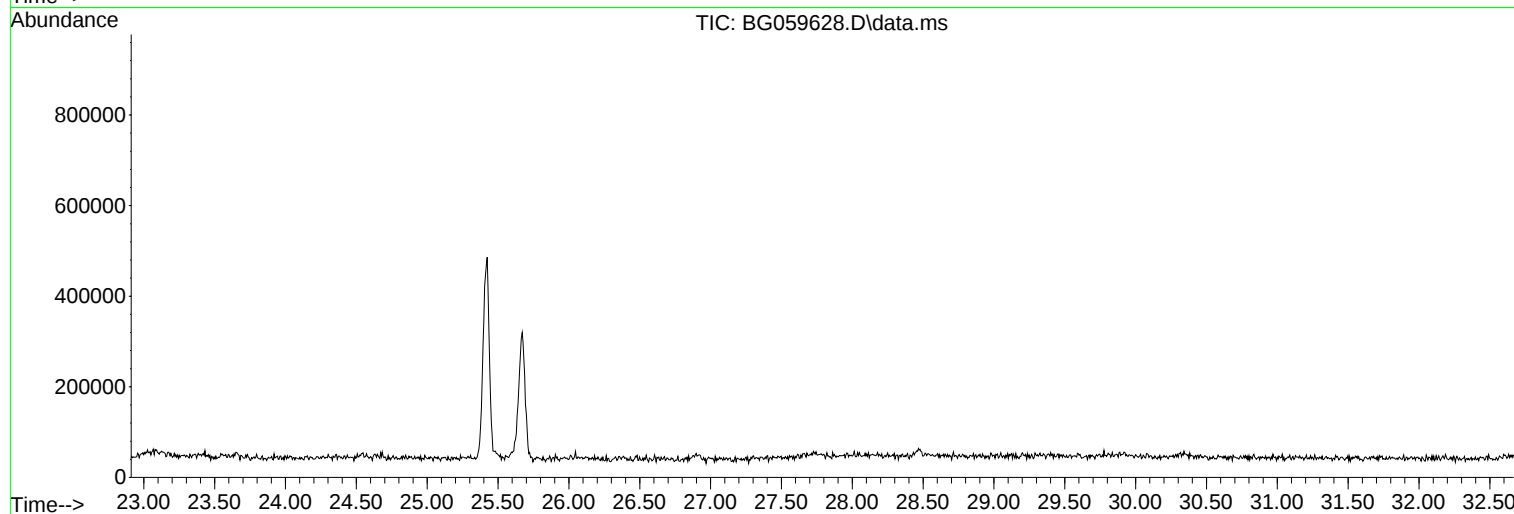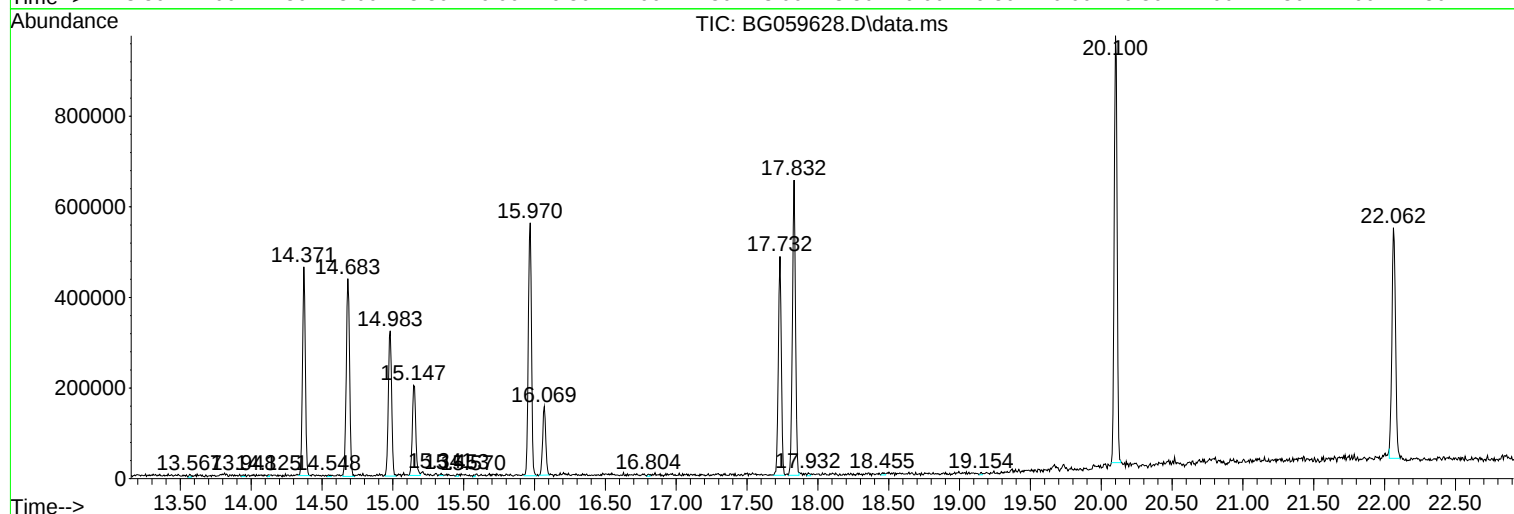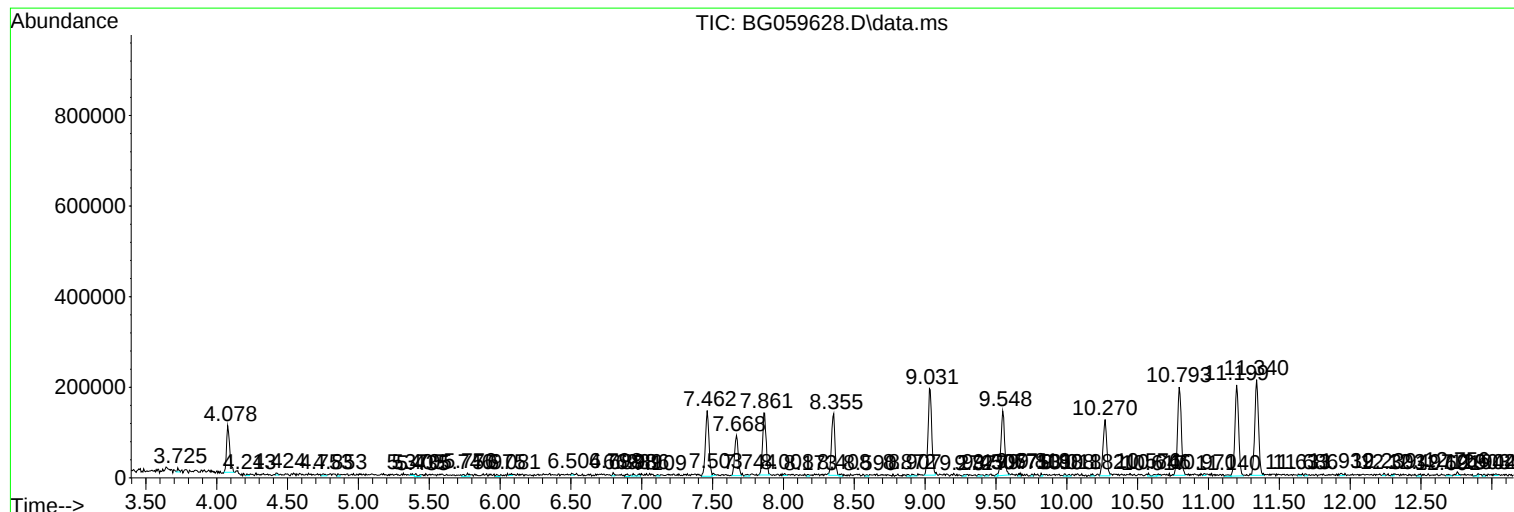

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059628.D
Acq On : 4 Nov 2023 19:21
Operator : MA/JU
Sample : PB156655BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK655

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059628.D
Acq On : 4 Nov 2023 19:21
Operator : MA/JU
Sample : PB156655BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK655

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc