

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059629.D
 Acq On : 4 Nov 2023 20:01
 Operator : MA/JU
 Sample : PB156797BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK797

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059629.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.493	16	18	21	rBV2	8187	9367	0.56%	0.069%
2	4.080	114	118	126	rVB	96861	160201	9.52%	1.184%
3	4.239	142	145	148	rBV3	7386	8343	0.50%	0.062%
4	5.937	428	434	435	rBV3	7455	11841	0.70%	0.088%
5	6.566	539	541	542	rBV3	9517	8143	0.48%	0.060%
6	6.736	568	570	574	rBV2	6109	6839	0.41%	0.051%
7	7.165	641	643	646	rBV	8230	7845	0.47%	0.058%
8	7.465	687	694	702	rBV	251702	423138	25.13%	3.128%
9	7.664	723	728	736	rVB	153383	258713	15.37%	1.912%
10	7.864	756	762	769	rVB	246212	411340	24.43%	3.040%
11	7.964	775	779	781	rVB	6192	7952	0.47%	0.059%
12	8.052	792	794	796	rBV	5376	6601	0.39%	0.049%
13	8.352	840	845	851	rVB2	113973	210852	12.52%	1.559%
14	9.033	953	961	968	rBV	235795	403026	23.94%	2.979%
15	9.157	981	982	987	rBV	3961	4692	0.28%	0.035%
16	9.550	1042	1049	1056	rVB	157637	284506	16.90%	2.103%
17	9.627	1059	1062	1063	rBV	3903	4696	0.28%	0.035%
18	10.267	1165	1171	1181	rVB2	148382	275736	16.38%	2.038%
19	10.455	1201	1203	1206	rVB2	5905	5437	0.32%	0.040%
20	10.790	1252	1260	1272	rVB2	236367	444016	26.37%	3.282%
21	10.925	1278	1283	1286	rBV2	5270	7475	0.44%	0.055%
22	11.090	1310	1311	1315	rBV2	4568	5131	0.30%	0.038%
23	11.196	1323	1329	1336	rVB	162499	313743	18.64%	2.319%
24	11.337	1346	1353	1363	rVB	231921	439339	26.10%	3.247%
25	11.407	1363	1365	1367	rBV	4223	4924	0.29%	0.036%
26	11.501	1378	1381	1384	rBV	4849	6424	0.38%	0.047%
27	12.265	1508	1511	1514	rBV	4026	4847	0.29%	0.036%
28	12.435	1537	1540	1543	rVB2	4094	5884	0.35%	0.043%
29	12.606	1568	1569	1574	rBV2	4686	6456	0.38%	0.048%
30	12.758	1591	1595	1599	rVB3	8489	11456	0.68%	0.085%
31	14.104	1820	1824	1827	rBV3	5605	9271	0.55%	0.069%
32	14.139	1828	1830	1832	rBV	8977	6380	0.38%	0.047%
33	14.374	1864	1870	1875	rVB	694928	996585	59.19%	7.366%
34	14.686	1916	1923	1929	rBV	687004	1117585	66.38%	8.261%
35	14.903	1958	1960	1963	rBV	6521	7337	0.44%	0.054%
36	14.979	1967	1973	1981	rVB2	364144	573997	34.09%	4.243%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059629.D
 Acq On : 4 Nov 2023 20:01
 Operator : MA/JU
 Sample : PB156797BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK797

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

37	15.150	1996	2002	2007	rBV2	328666	520572	30.92%	3.848%
38	15.297	2025	2027	2029	rBV2	8819	7701	0.46%	0.057%
39	15.726	2098	2100	2102	rBV	8885	7055	0.42%	0.052%
40	15.966	2135	2141	2149	rBV	881093	1334970	79.29%	9.868%
41	16.072	2153	2159	2165	rVB2	240360	385662	22.91%	2.851%
42	17.083	2329	2331	2333	rBV	6945	5980	0.36%	0.044%
43	17.500	2400	2402	2403	rBV	8723	5703	0.34%	0.042%
44	17.729	2435	2441	2449	rVB	494657	771727	45.84%	5.704%
45	17.835	2452	2459	2466	rVB	1014260	1554500	92.33%	11.490%
46	20.103	2839	2845	2852	rBV	1208175	1683578	100.00%	12.444%
47	22.065	3173	3179	3187	rVB2	436901	781322	46.41%	5.775%




Sum of corrected areas: 13528888

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059629.D
Acq On : 4 Nov 2023 20:01
Operator : MA/JU
Sample : PB156797BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK797

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

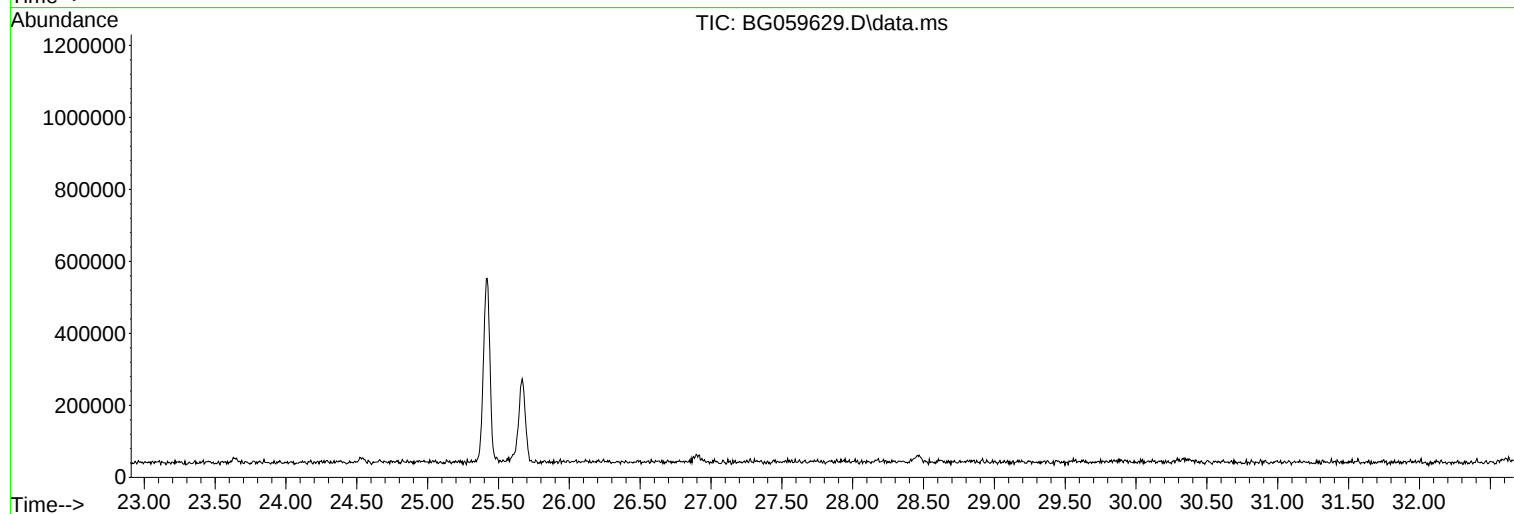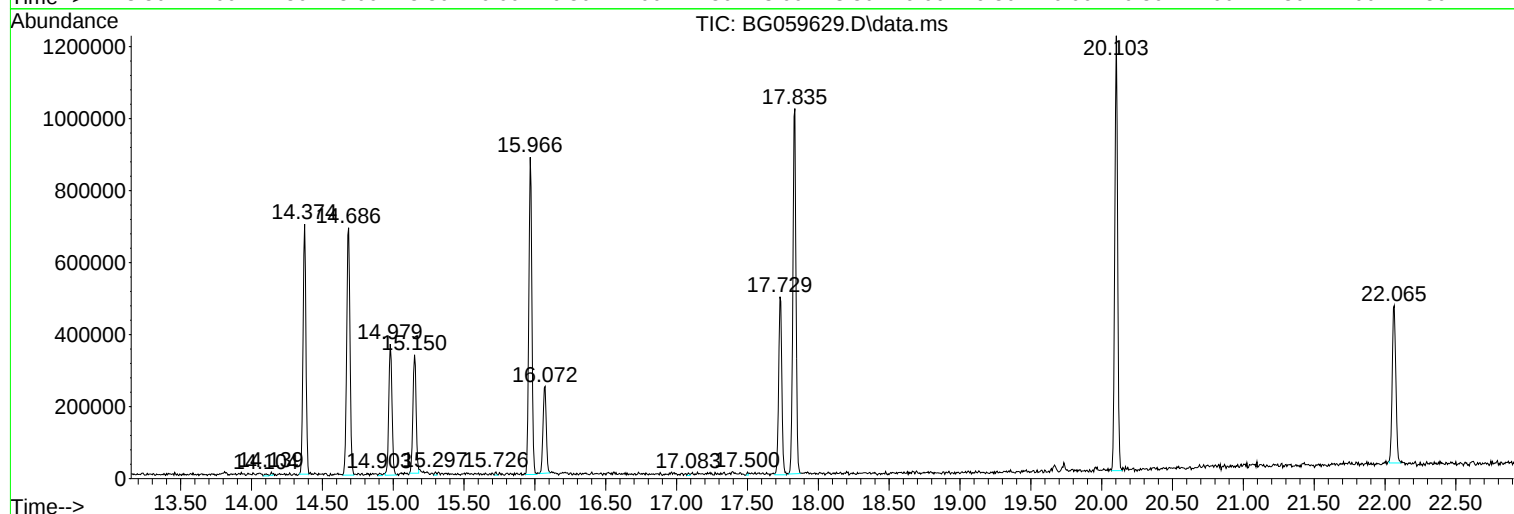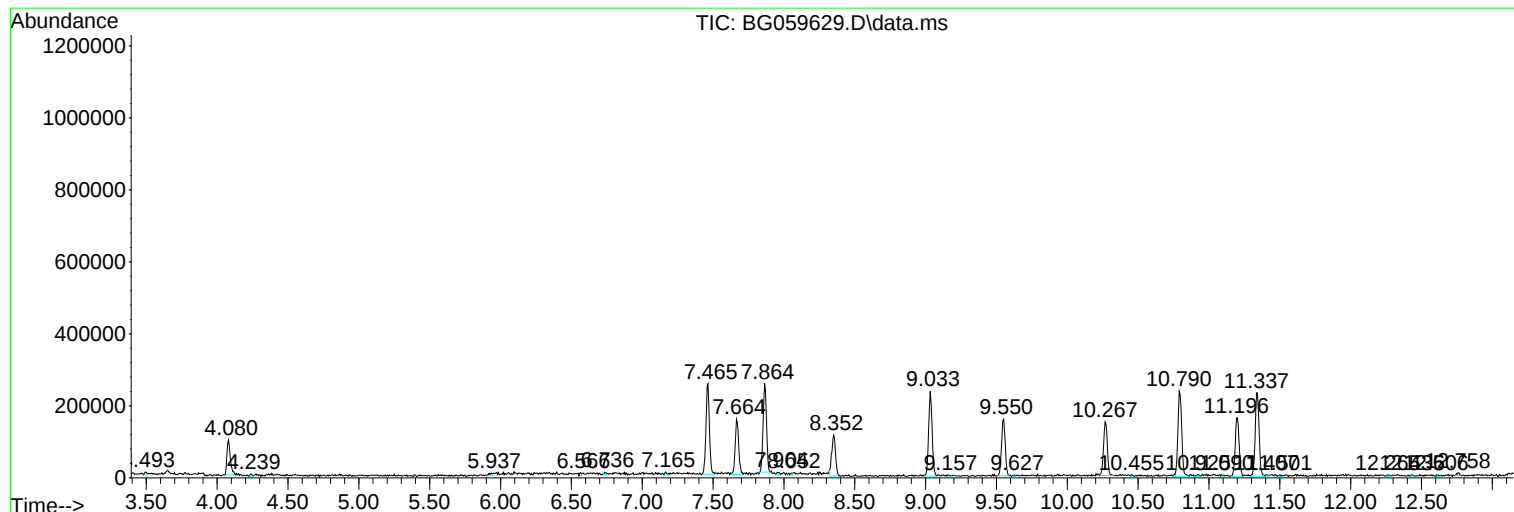

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059629.D
Acq On : 4 Nov 2023 20:01
Operator : MA/JU
Sample : PB156797BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK797

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059629.D
Acq On : 4 Nov 2023 20:01
Operator : MA/JU
Sample : PB156797BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK797

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
